
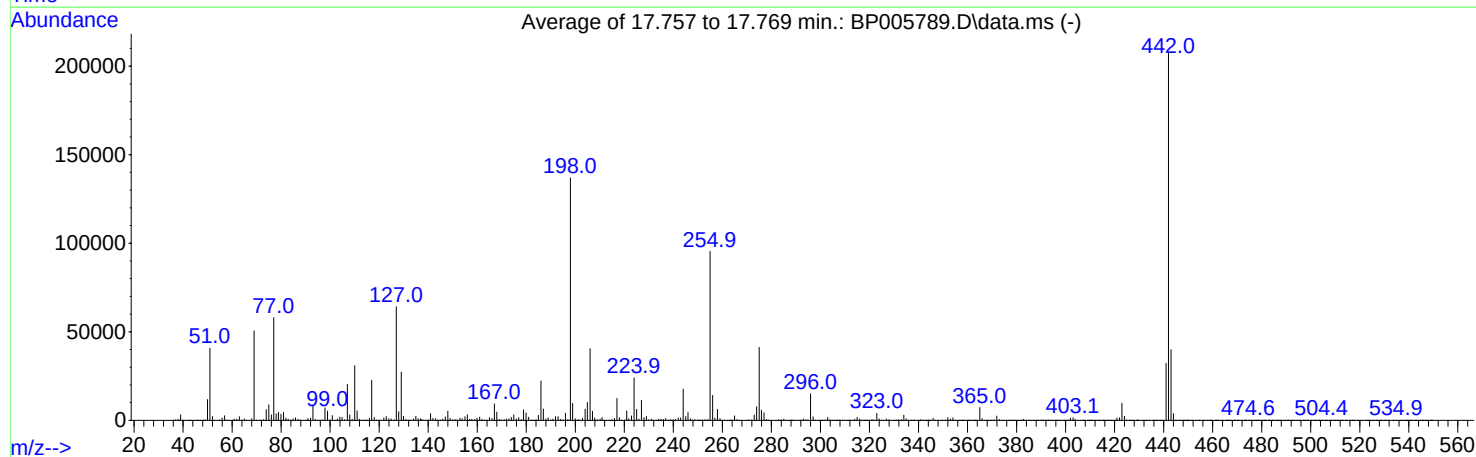


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060821\
 Data File : BP005789.D
 Acq On : 09 Jun 2021 00:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 09 11:54:55 2021

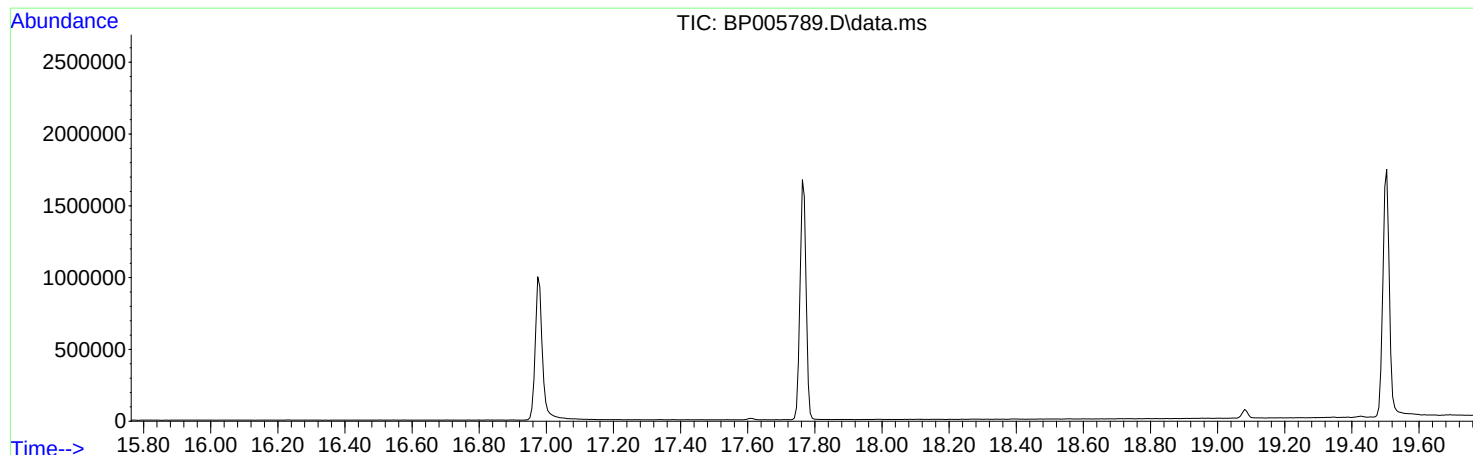




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.8	40784	PASS
68	69	0.00	2	1.8	933	PASS
69	198	0.00	100	36.9	50486	PASS
70	69	0.00	2	0.4	224	PASS
127	198	10	80	46.9	64168	PASS
197	198	0.00	2	0.2	318	PASS
198	198	100	100	100.0	136901	PASS
199	198	5	9	7.0	9601	PASS
275	198	10	60	30.1	41245	PASS
365	198	1	100	5.3	7268	PASS
441	198	0.01	100	23.6	32253	PASS
442	442	100	100	100.0	207701	PASS
443	442	15	24	19.2	39968	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060821\
Data File : BP005789.D
Acq On : 09 Jun 2021 00:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 09 07:16:41 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 09 02:47:38 2021
Response via : Initial Calibration

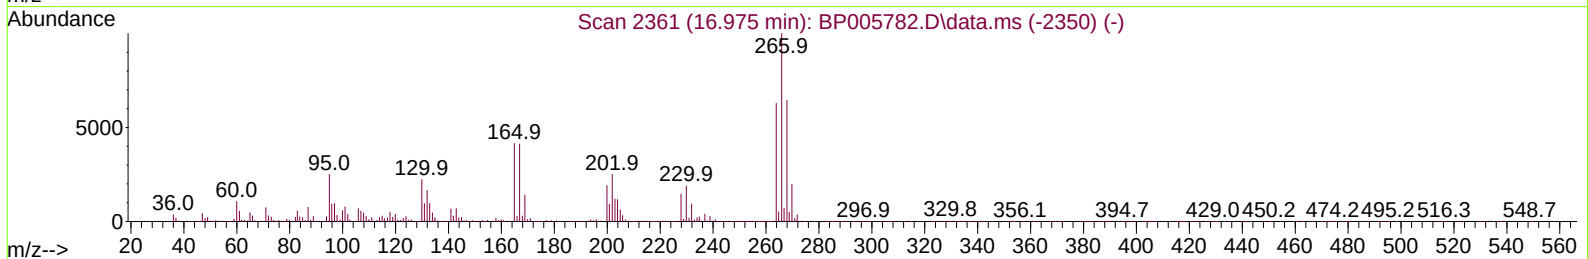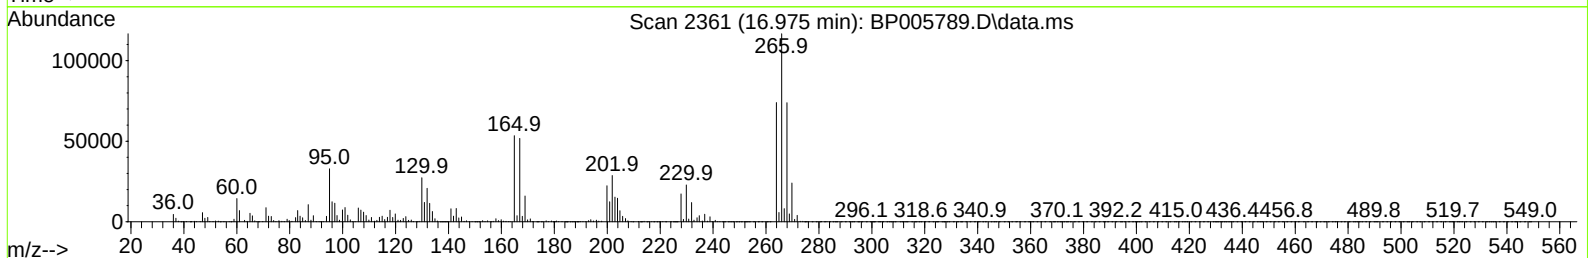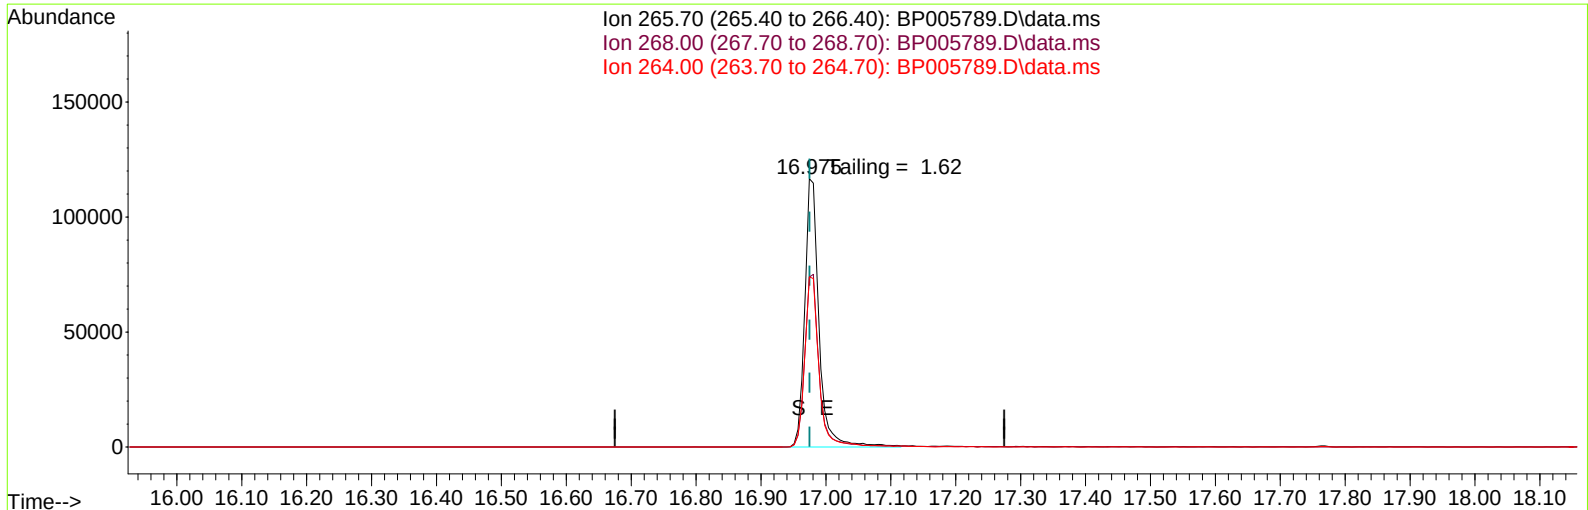

TIC: BP005789.D\data.ms

(70) Pentachlorophenol (C)

16.975min (-0.000) 116107.24 ng




response 178781

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.32
264.00	62.90	63.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060821\
 Data File : BP005789.D
 Acq On : 09 Jun 2021 00:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 09 07:16:41 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 09 02:47:38 2021
 Response via : Initial Calibration

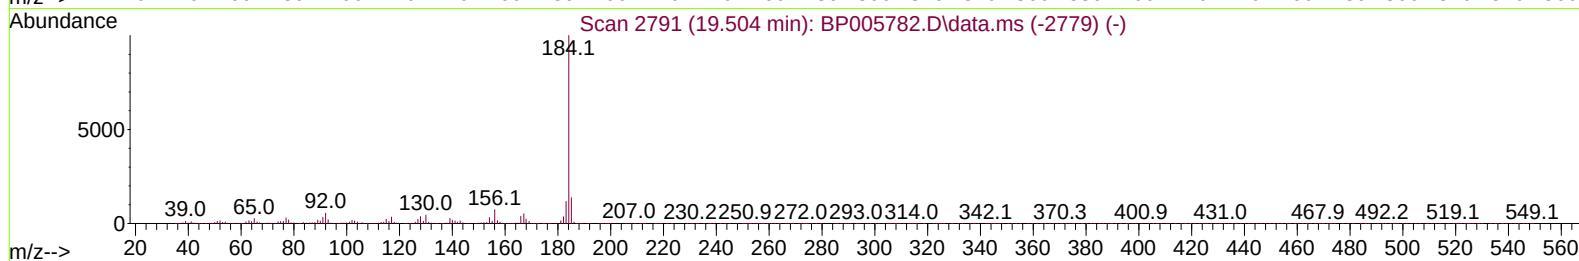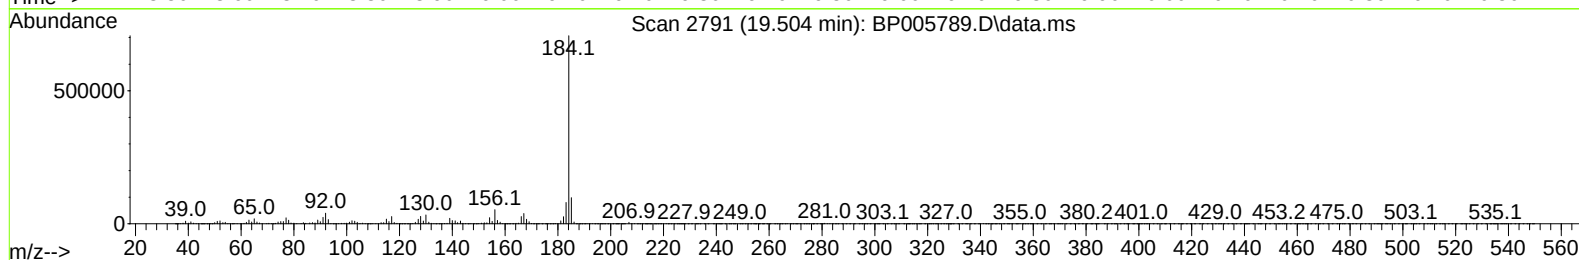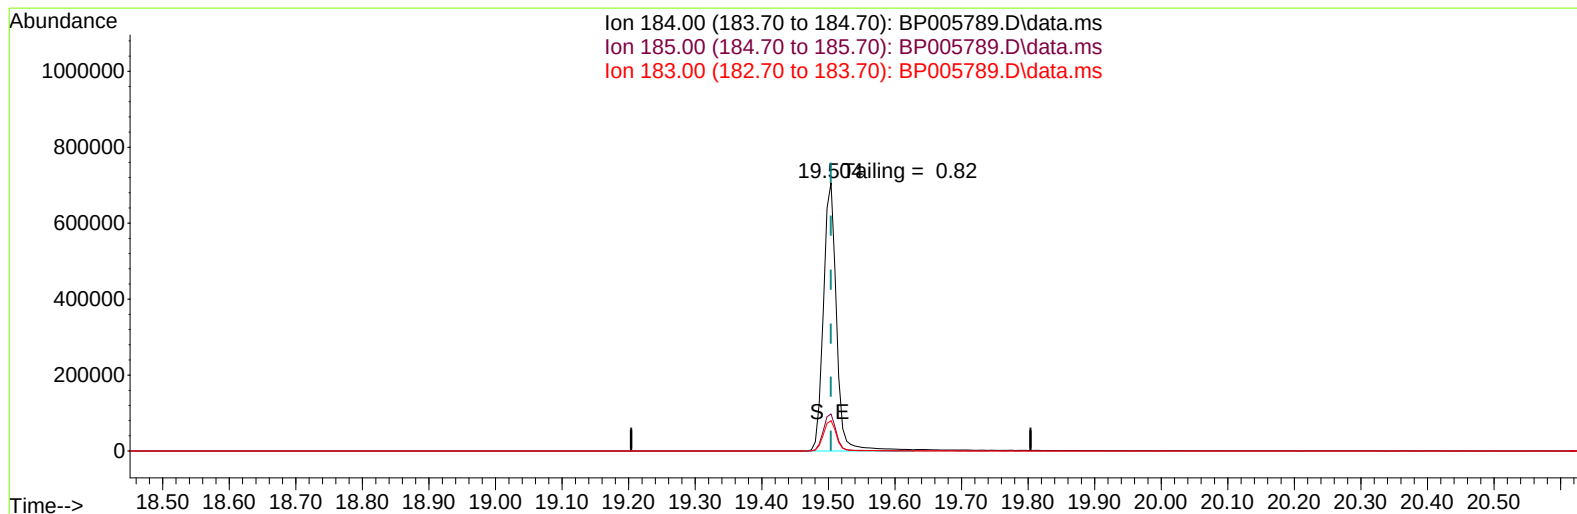

TIC: BP005789.D\data.ms

(77) Benzidine

19.504min (-0.000) 104754.00 ng

response 969976

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.86
183.00	11.90	11.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/8/2021	BNA_P	BP005789.D
Compound Name	Response	Retention Time
DDT	548104	20.698
DDD	6719	20.269
DDE	1144	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7863	555967	1.41

Instrument :
BNA_P
ClientSampleId :
DFTPP