
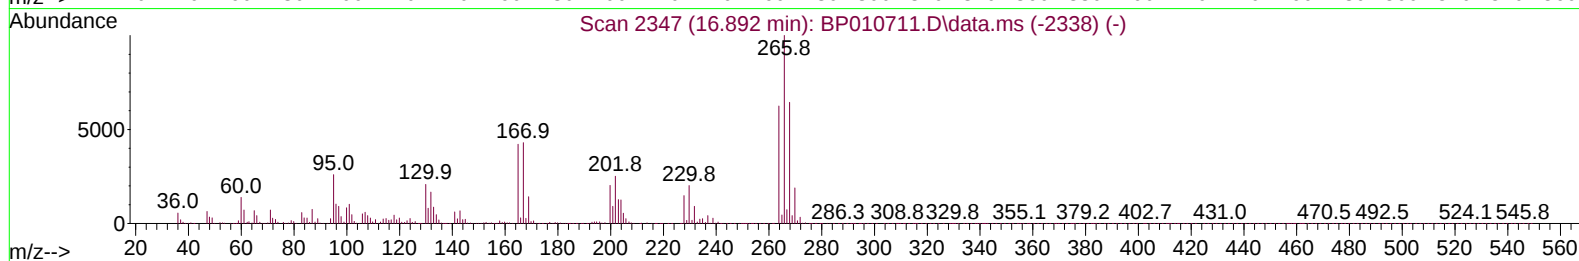
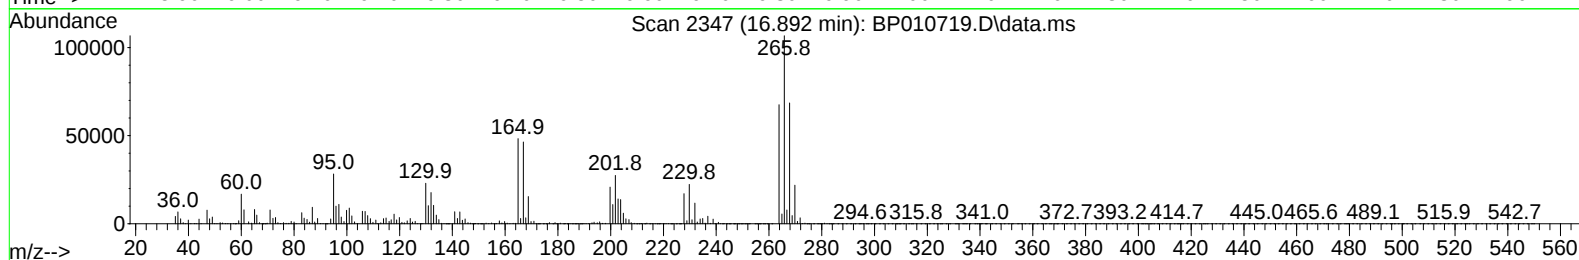


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060822\
Data File : BP010719.D
Acq On : 08 Jun 2022 10:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 12:36:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 07 19:29:31 2022
Response via : Initial Calibration

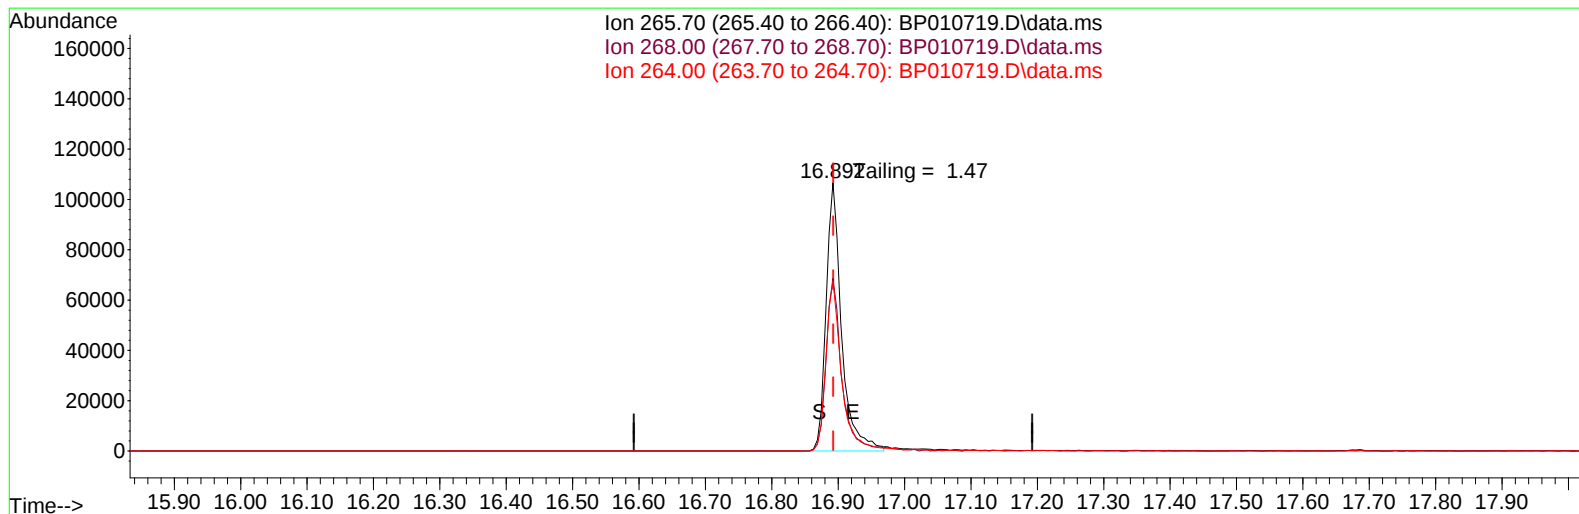

TIC: BP010719.D\data.ms

(70) Pentachlorophenol (C)




16.892min (-0.000) 1280454.54 ng

response 175675

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.27
264.00	63.00	63.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060822\
Data File : BP010719.D
Acq On : 08 Jun 2022 10:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 08 12:36:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 07 19:29:31 2022
Response via : Initial Calibration

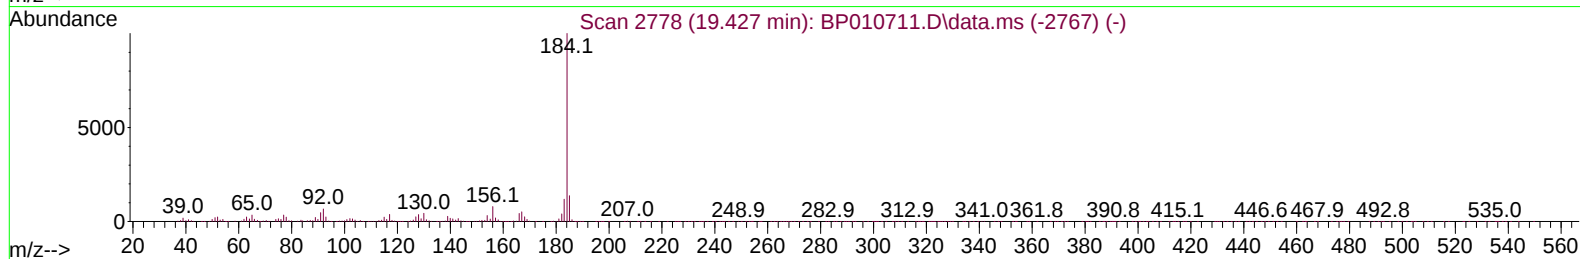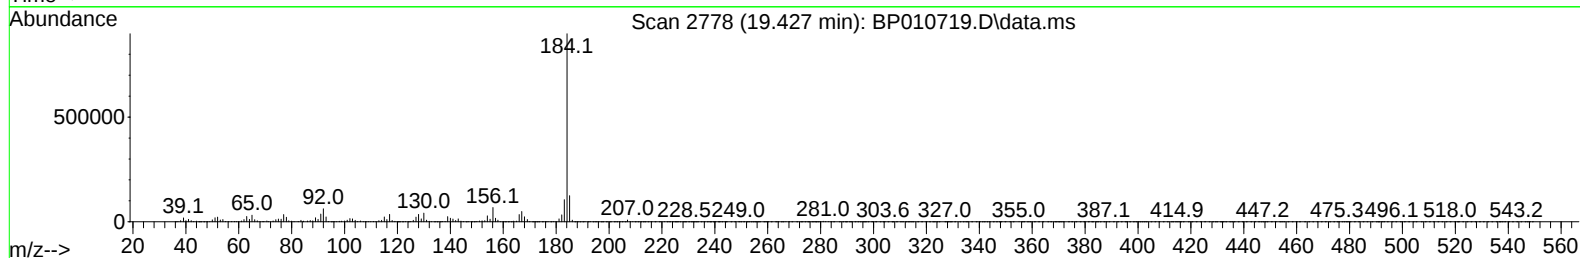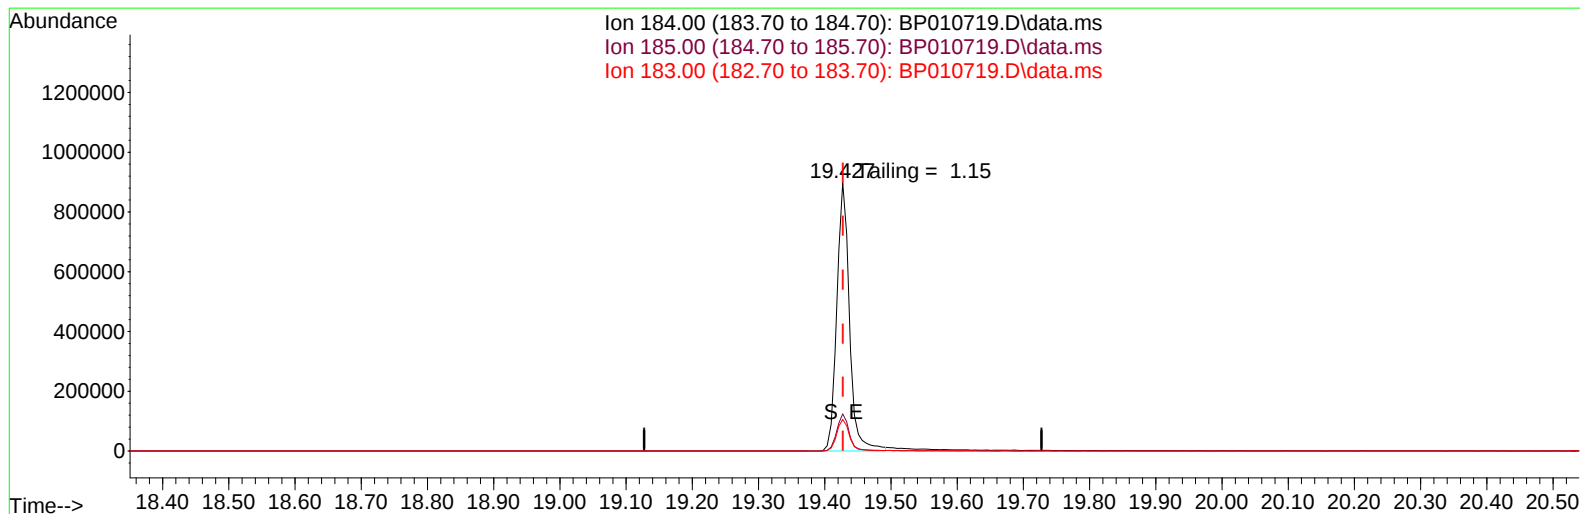

TIC: BP010719.D\data.ms

(77) Benzidine**19.427min (-0.000) 693843.76 ng****response 1220285**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.87
183.00	11.30	11.75
0.00	0.00	0.00