

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060822\
 Data File : BP010721.D
 Acq On : 08 Jun 2022 11:17
 Operator : CG/JU
 Sample : PB145377BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB145377BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP010721.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.422	391	397	415	rBV	2116443	3125991	53.03%	9.819%
2	7.016	661	668	684	rBV	1959939	3172804	53.83%	9.966%
3	7.840	801	808	820	rVB	371214	605627	10.27%	1.902%
4	8.999	997	1005	1027	rBV	1205026	2101456	35.65%	6.601%
5	10.640	1276	1284	1300	rBV	418394	802156	13.61%	2.520%
6	13.099	1693	1702	1719	rBV	2750756	4199151	71.24%	13.190%
7	14.475	1928	1936	1949	rBV	624229	999632	16.96%	3.140%
8	15.969	2182	2190	2211	rBV	2039799	3107283	52.72%	9.761%
9	17.234	2398	2405	2419	rBV	742210	1125054	19.09%	3.534%
10	19.792	2834	2840	2851	rBV	4951747	5894409	100.00%	18.515%
11	21.322	3095	3100	3108	rBV	808209	1135433	19.26%	3.567%
12	21.439	3114	3120	3133	rBV	2987645	4501553	76.37%	14.140%
13	23.727	3503	3509	3518	rVB2	505931	1064640	18.06%	3.344%




Sum of corrected areas: 31835189

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060822\
Data File : BP010721.D
Acq On : 08 Jun 2022 11:17
Operator : CG/JU
Sample : PB145377BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145377BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

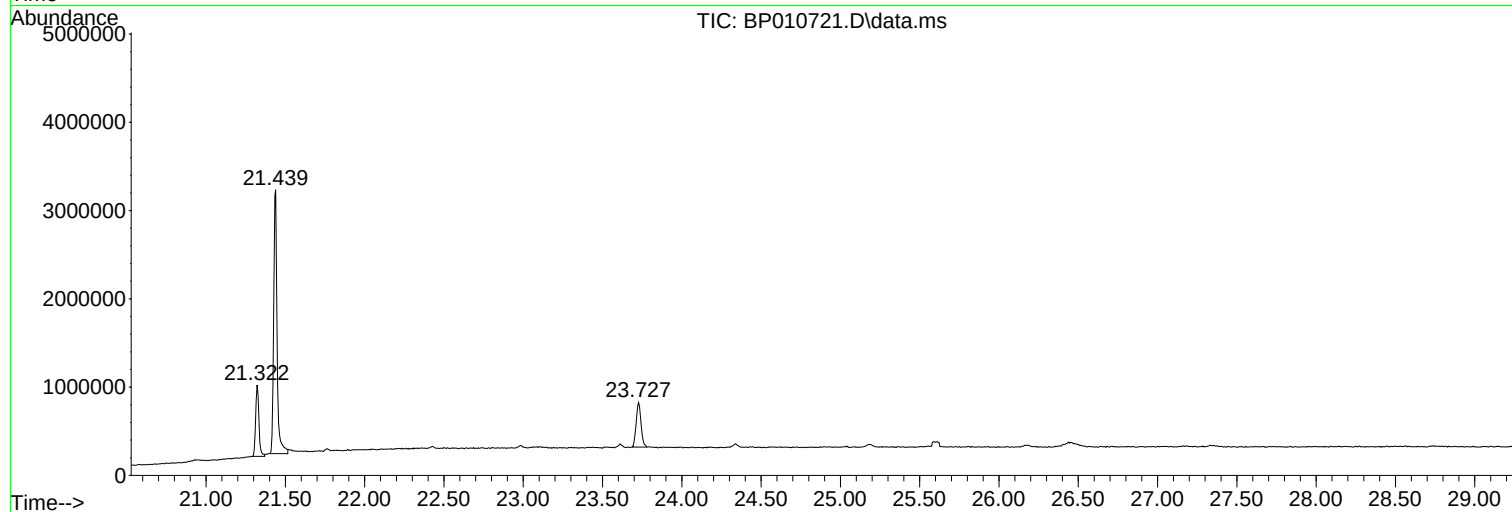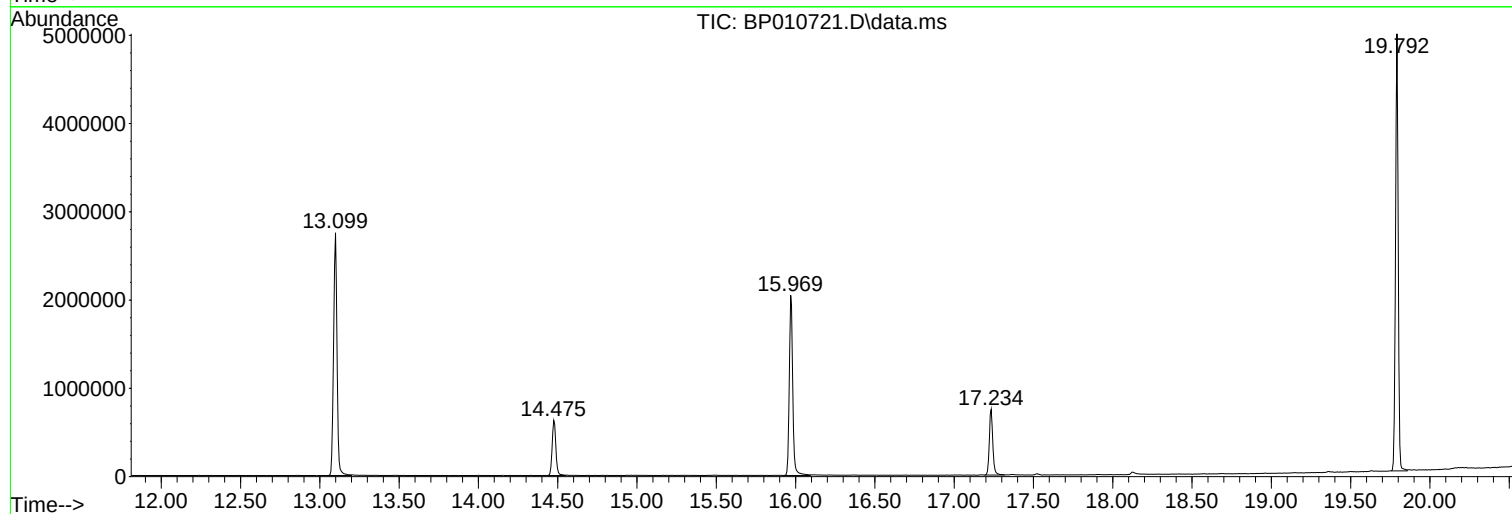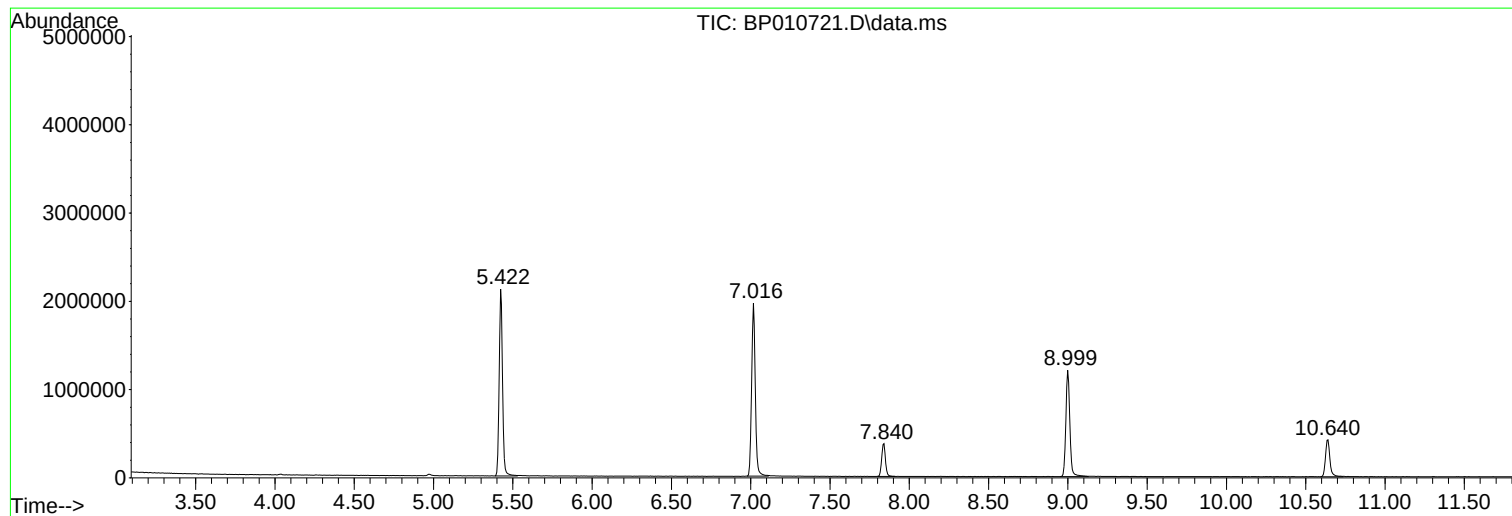

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060822\
Data File : BP010721.D
Acq On : 08 Jun 2022 11:17
Operator : CG/JU
Sample : PB145377BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145377BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.439	79.29 ng	4501550	Chrysene-d12	21.322

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	94
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	64
4			1H-Indole-3-acetic acid, 5-[(tri...	277	C14H19NO3Si	072101-35-0	32
5			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	25

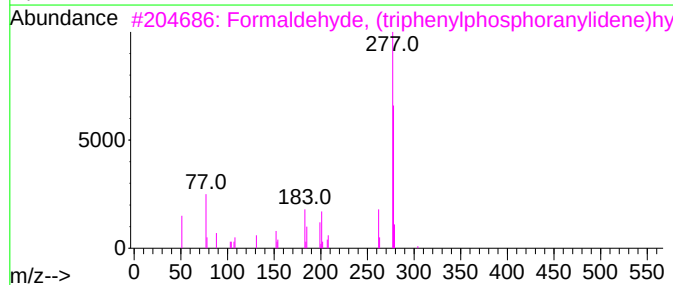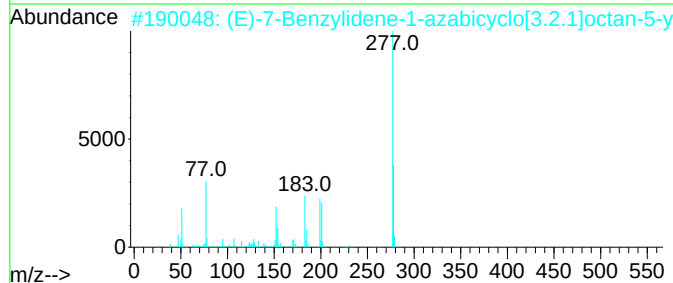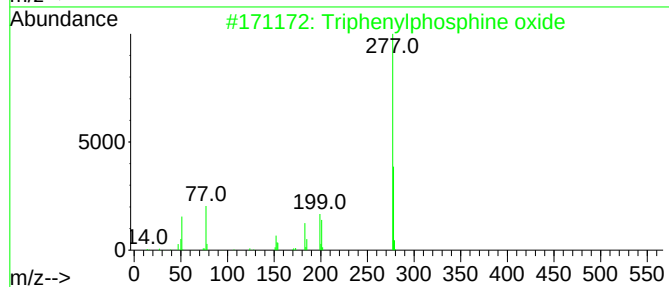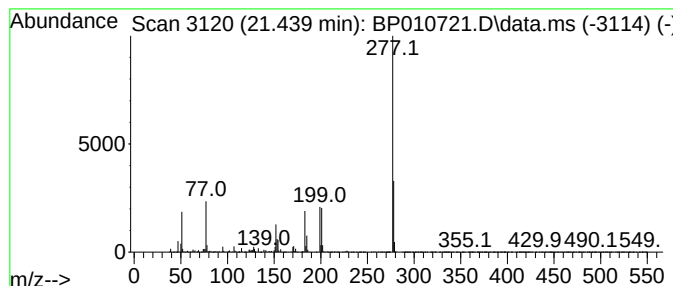

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060822\
Data File : BP010721.D
Acq On : 08 Jun 2022 11:17
Operator : CG/JU
Sample : PB145377BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145377BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
Triphenylphosph...	21.439	79.3	ng	4501550	5	21.322	1135430	20.0