
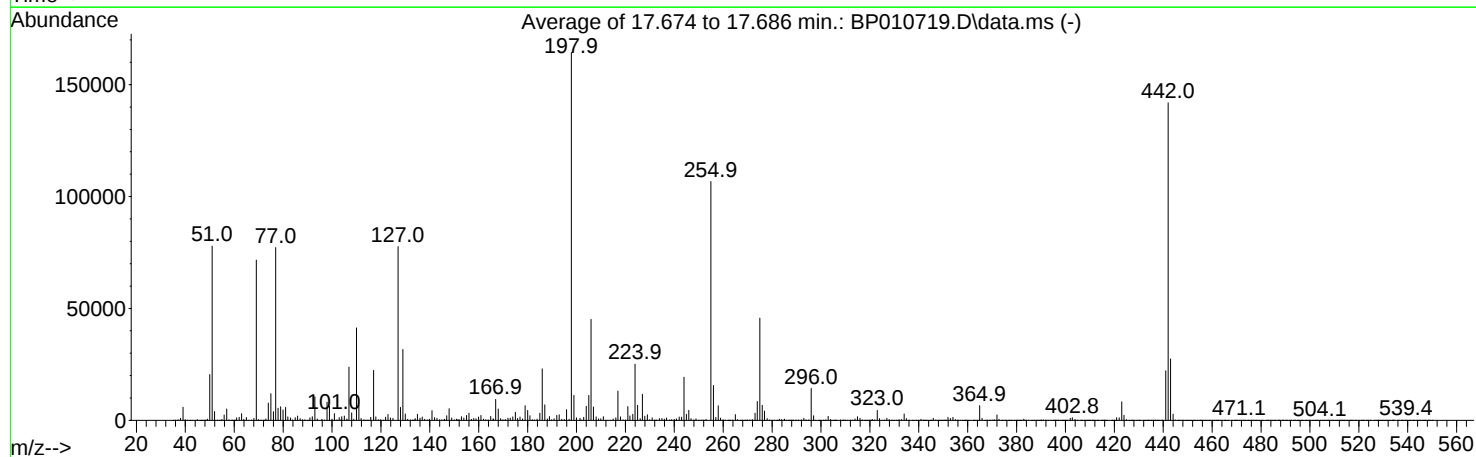


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060822\
 Data File : BP010719.D
 Acq On : 08 Jun 2022 10:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 07 19:29:31 2022

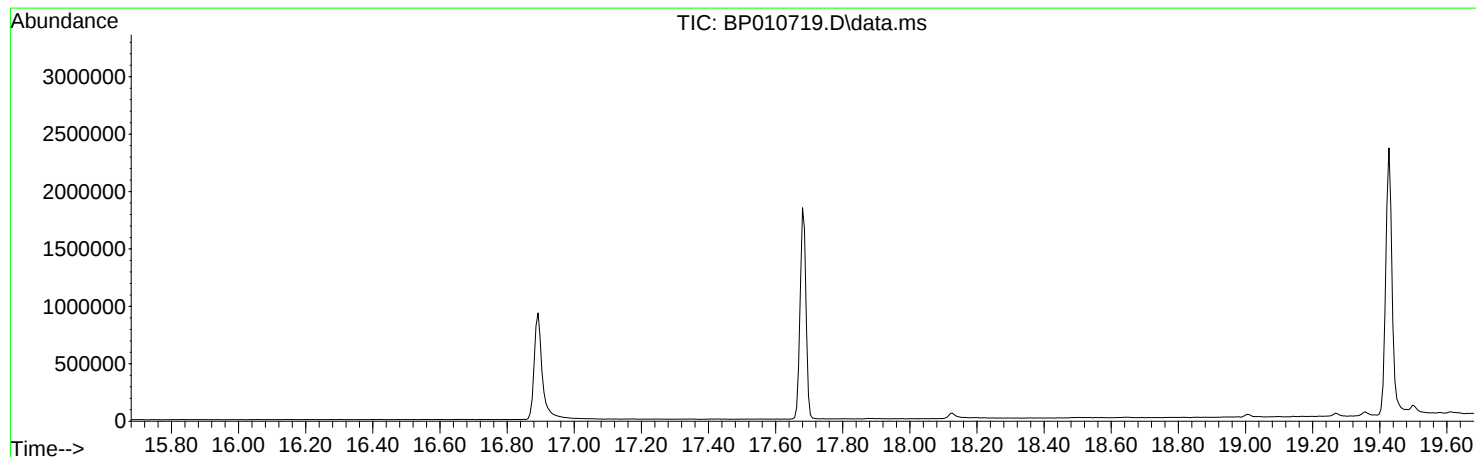




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.4	77875	PASS
68	69	0.00	2	1.2	860	PASS
69	198	0.00	100	43.6	71660	PASS
70	69	0.00	2	0.5	346	PASS
127	198	10	80	47.2	77629	PASS
197	198	0.00	2	0.3	513	PASS
198	198	100	100	100.0	164352	PASS
199	198	5	9	6.8	11122	PASS
275	198	10	60	27.8	45707	PASS
365	198	1	100	4.0	6578	PASS
441	198	0.01	100	13.5	22196	PASS
442	442	100	100	100.0	141935	PASS
443	442	15	24	19.4	27467	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060822\
 Data File : BP010719.D
 Acq On : 08 Jun 2022 10:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 08 12:36:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 07 19:29:31 2022
 Response via : Initial Calibration

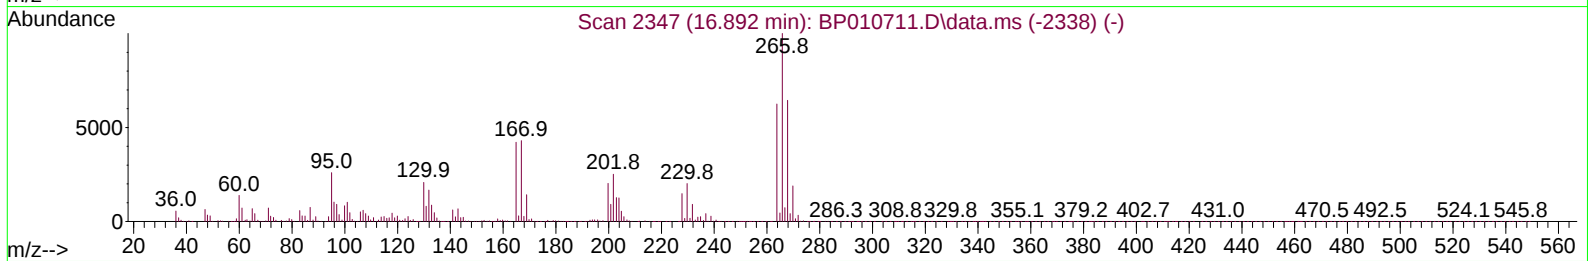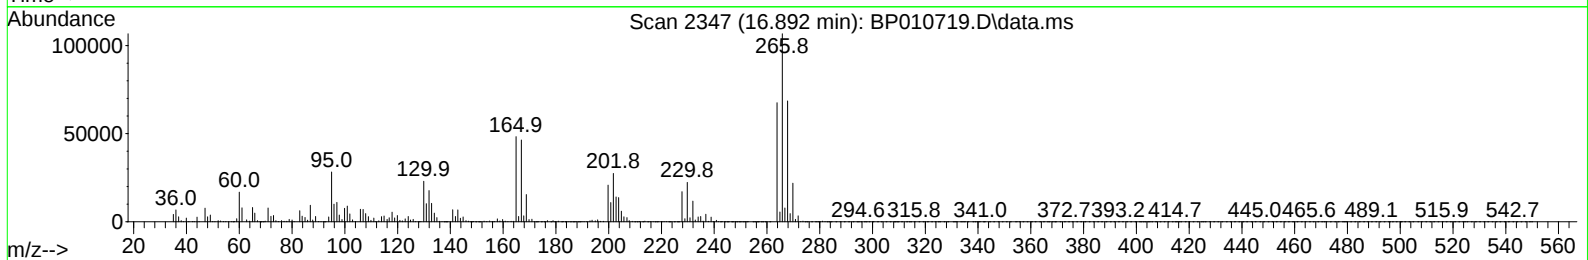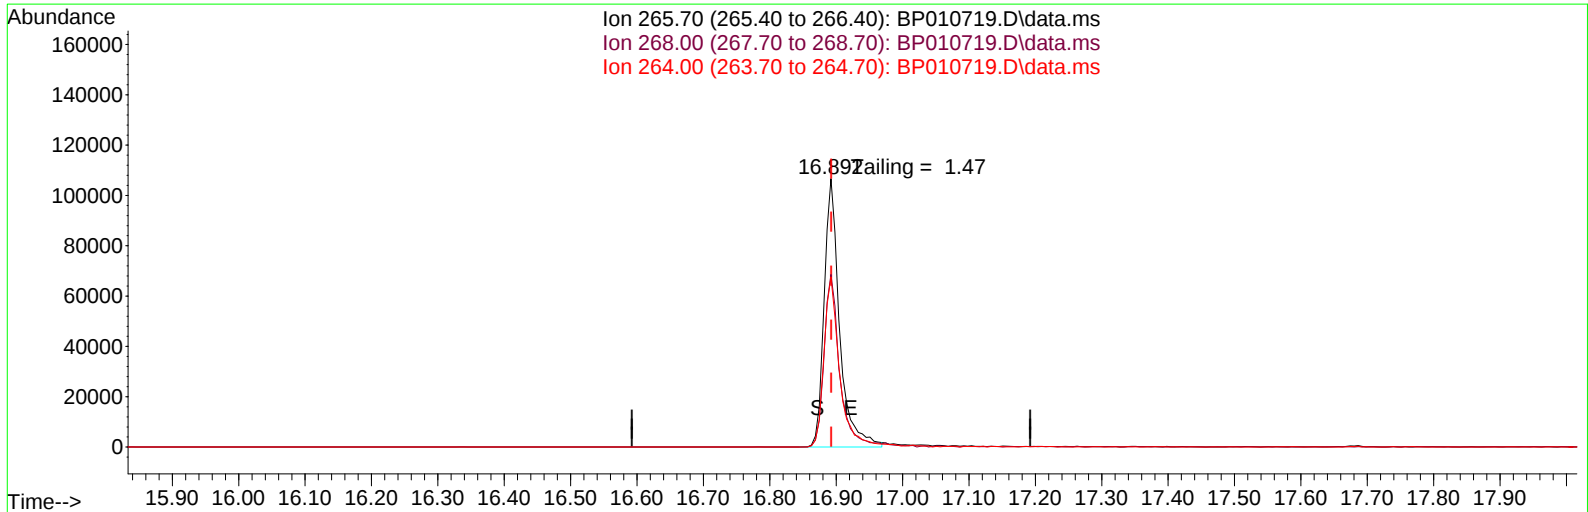

TIC: BP010719.D\data.ms

(70) Pentachlorophenol (C)

16.892min (-0.000) 1280454.54 ng




response 175675

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.27
264.00	63.00	63.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060822\
Data File : BP010719.D
Acq On : 08 Jun 2022 10:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 08 12:36:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 07 19:29:31 2022
Response via : Initial Calibration

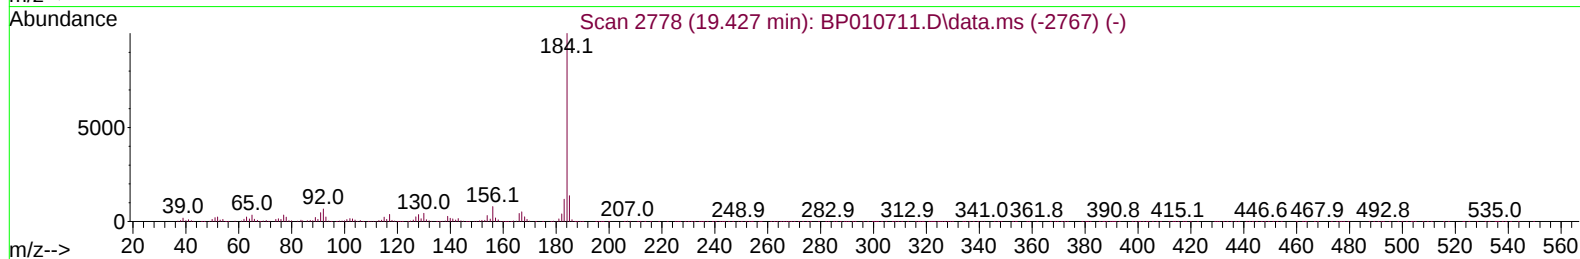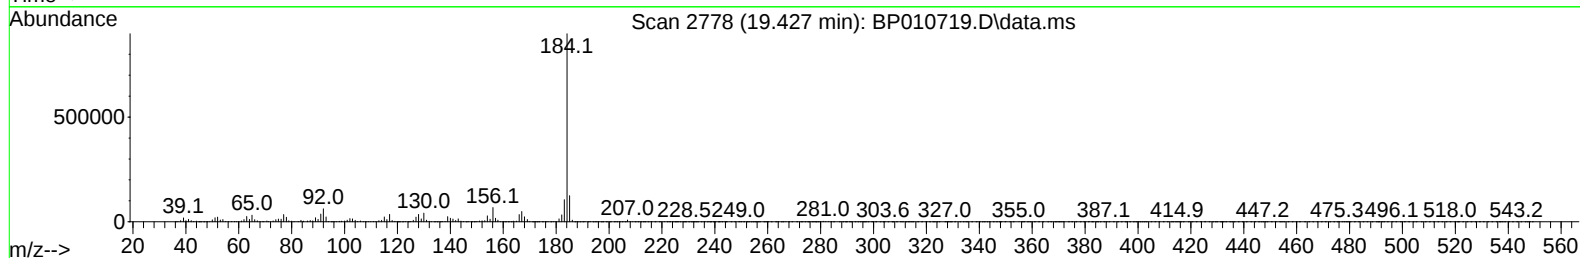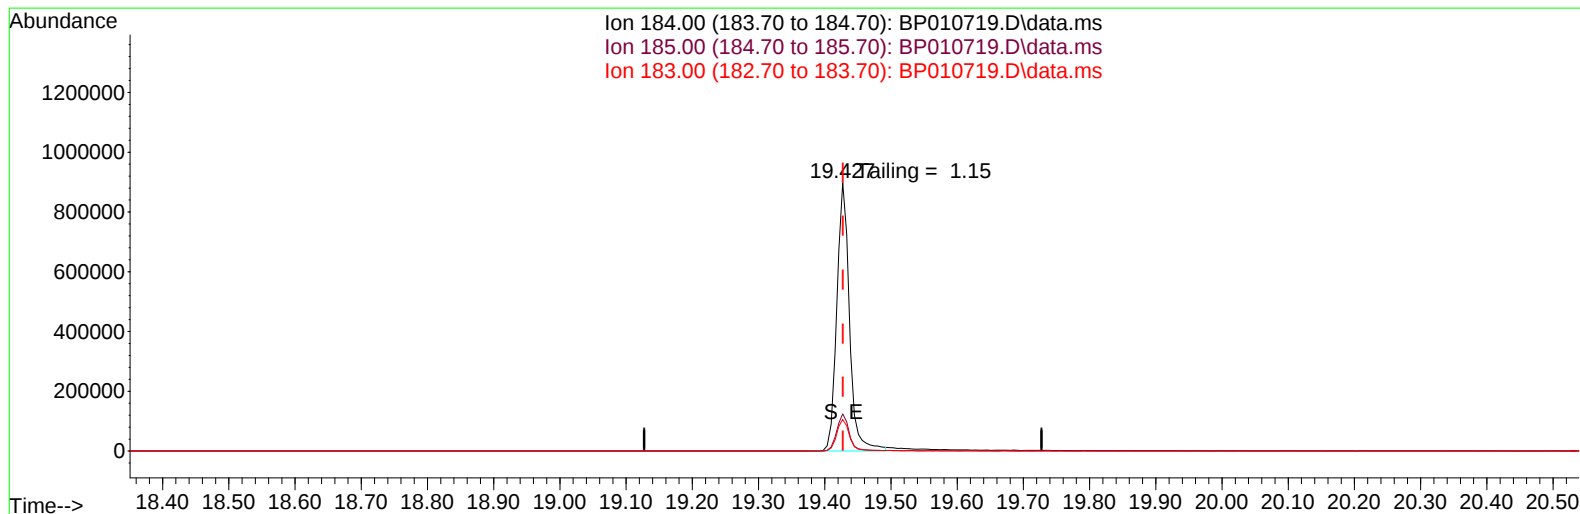

TIC: BP010719.D\data.ms

(77) Benzidine

19.427min (-0.000) 693843.76 ng

response 1220285

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.87
183.00	11.30	11.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/8/2022	BNA_P	<u>BP010719.D</u>
Compound Name	Response	Retention Time
DDT	683210	20.62
DDD	6481	20.2
DDE	1446	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7927	691137	1.15

Instrument :
BNA_P
ClientSampleId :
DFTPP