

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060921\
 Data File : BP005811.D
 Acq On : 09 Jun 2021 16:15
 Operator : CG/JU
 Sample : PB136947BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB136947BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005811.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.517	407	413	436	rBV	1704689	2495279	49.57%	10.974%
2	7.122	678	686	705	rBV	1494220	2382595	47.33%	10.478%
3	7.952	821	827	836	rBV	306808	497620	9.89%	2.188%
4	9.116	1017	1025	1048	rBV	882585	1498424	29.77%	6.590%
5	10.763	1295	1305	1317	rBV	348383	621011	12.34%	2.731%
6	13.210	1712	1721	1740	rBV	2339385	3443308	68.40%	15.143%
7	14.581	1947	1954	1963	rBV	520870	779915	15.49%	3.430%
8	16.069	2199	2207	2228	rBV	1920367	2858025	56.78%	12.569%
9	17.322	2414	2420	2431	rBV	589027	904815	17.97%	3.979%
10	19.869	2848	2853	2862	rBV	4090798	5033925	100.00%	22.138%
11	21.392	3107	3112	3121	rBV	823228	1083982	21.53%	4.767%
12	23.816	3518	3524	3532	rVB2	561910	1140010	22.65%	5.013%




Sum of corrected areas: 22738909

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060921\
Data File : BP005811.D
Acq On : 09 Jun 2021 16:15
Operator : CG/JU
Sample : PB136947BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136947BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

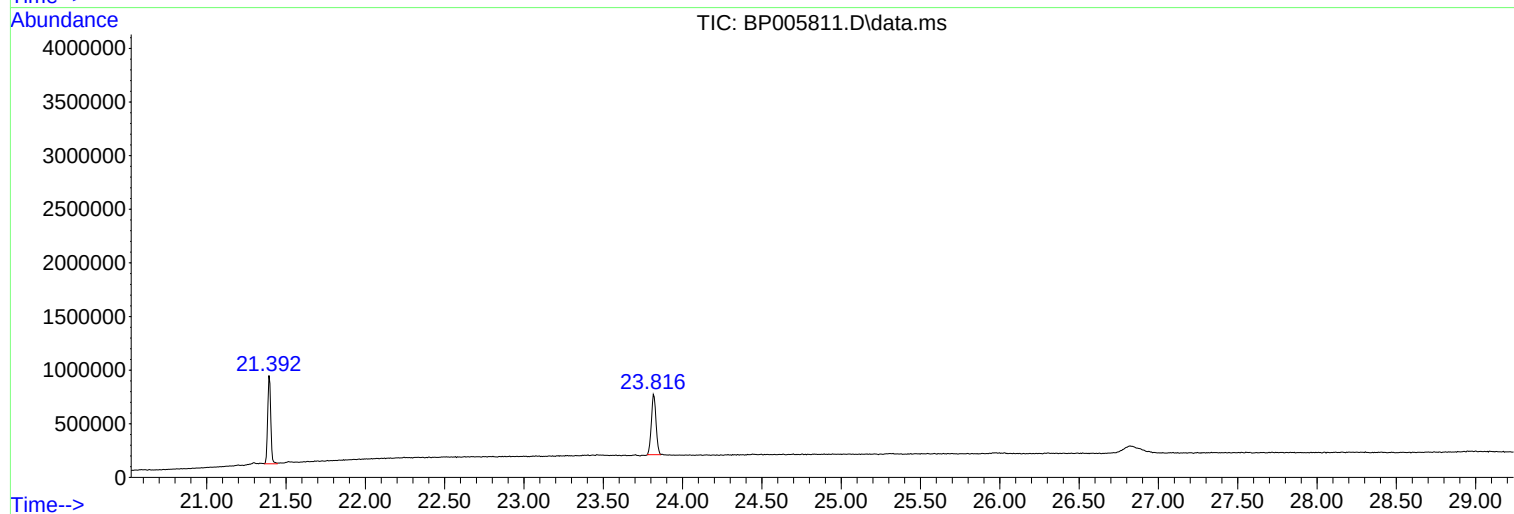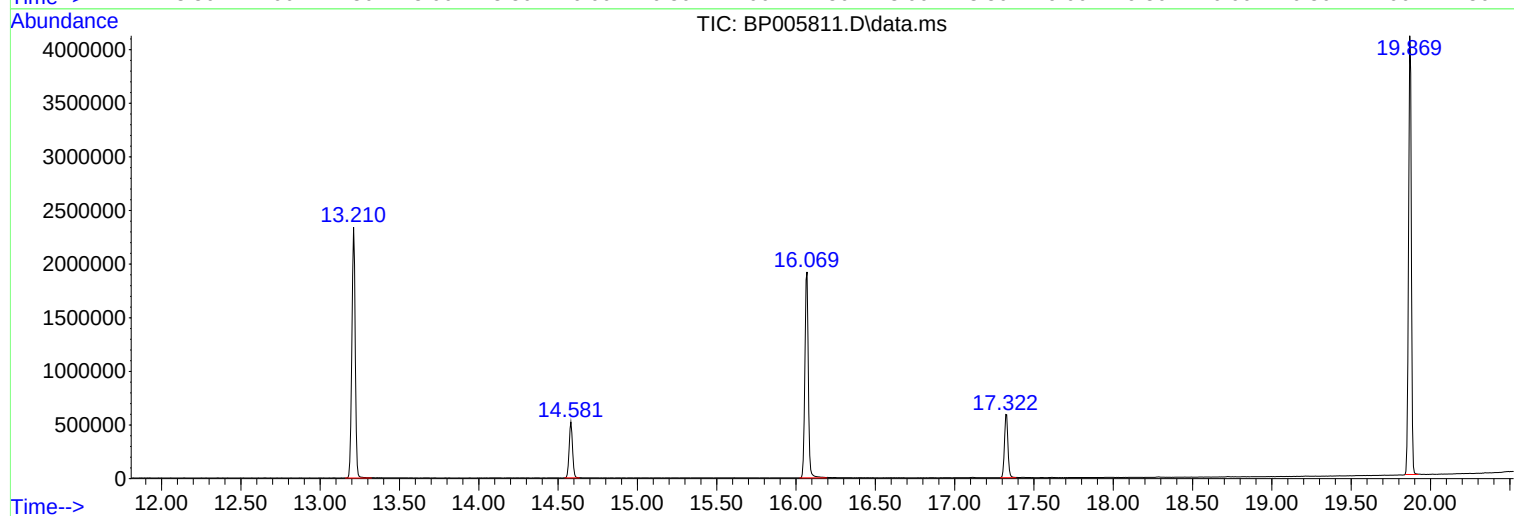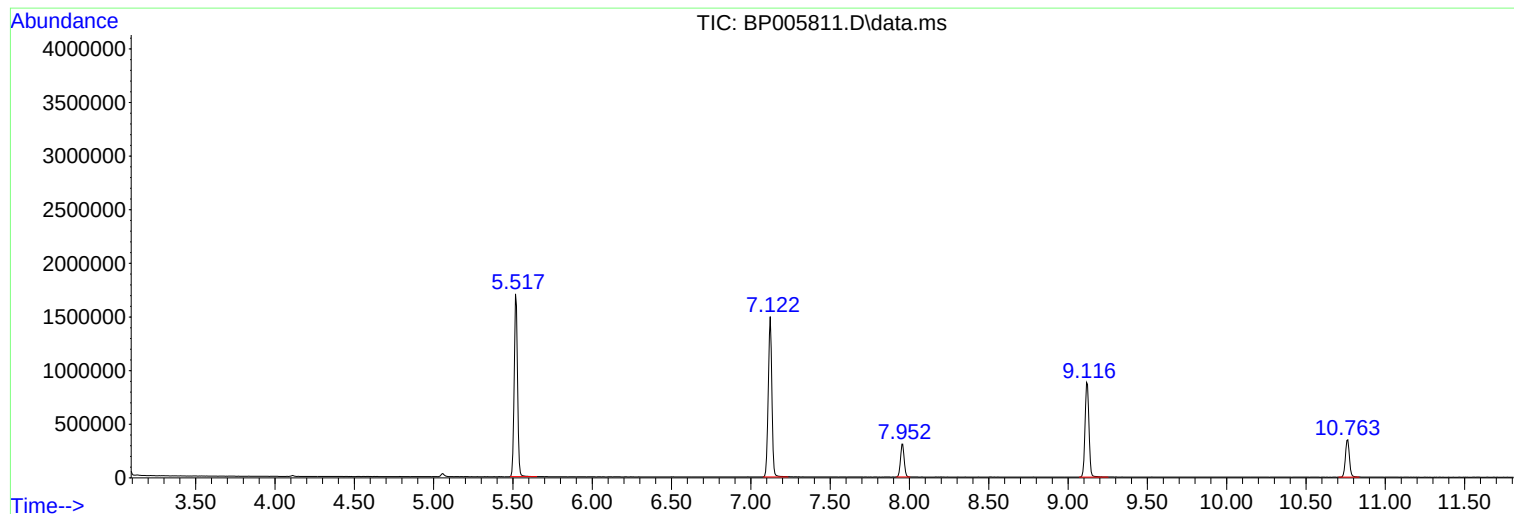

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060921\
Data File : BP005811.D
Acq On : 09 Jun 2021 16:15
Operator : CG/JU
Sample : PB136947BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136947BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060921\
Data File : BP005811.D
Acq On : 09 Jun 2021 16:15
Operator : CG/JU
Sample : PB136947BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136947BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------