
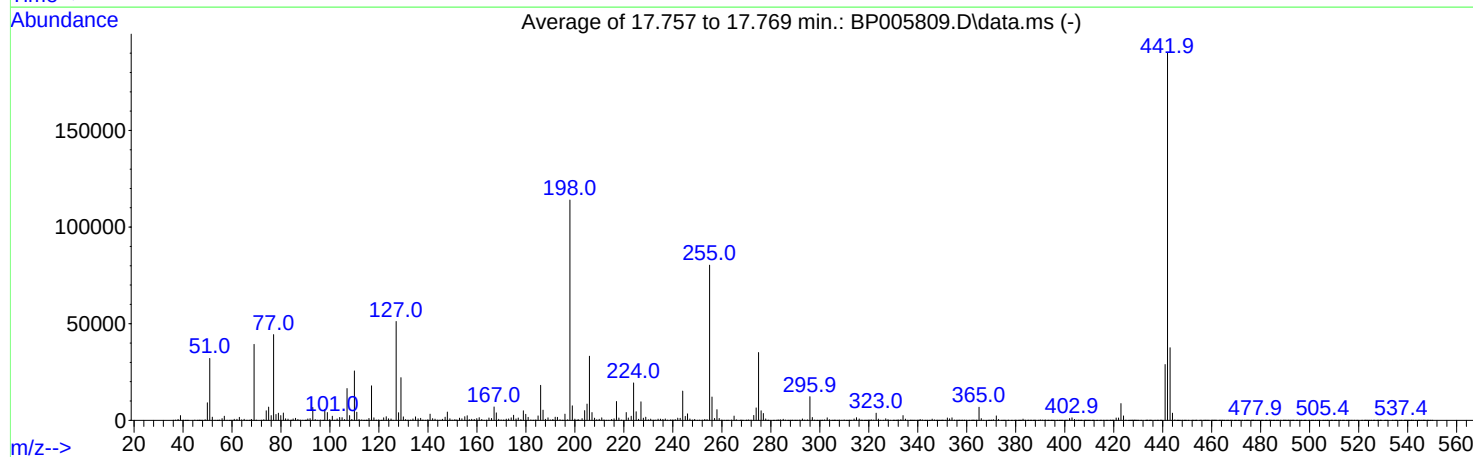


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060921\
 Data File : BP005809.D
 Acq On : 09 Jun 2021 14:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 09 11:54:55 2021

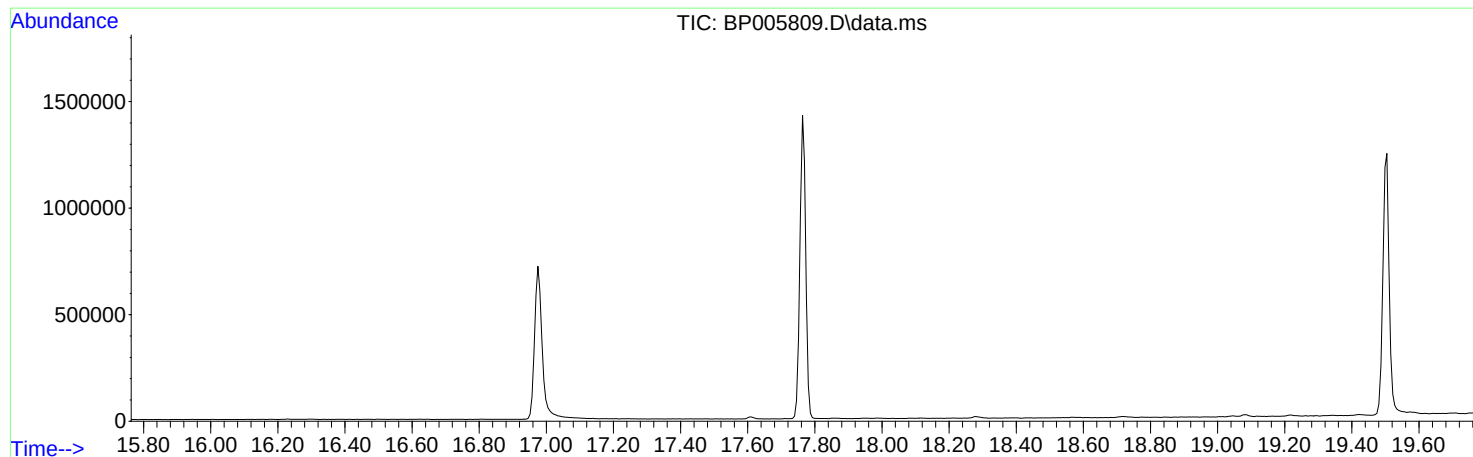




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	32050	PASS
68	69	0.00	2	1.4	542	PASS
69	198	0.00	100	34.5	39339	PASS
70	69	0.00	2	0.5	215	PASS
127	198	10	80	44.9	51197	PASS
197	198	0.00	2	0.3	300	PASS
198	198	100	100	100.0	114011	PASS
199	198	5	9	6.6	7558	PASS
275	198	10	60	30.8	35149	PASS
365	198	1	100	5.9	6766	PASS
441	198	0.01	100	25.4	28933	PASS
442	442	100	100	100.0	190334	PASS
443	442	15	24	19.8	37591	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060921\
 Data File : BP005809.D
 Acq On : 09 Jun 2021 14:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 09 16:37:43 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 09 11:54:55 2021
 Response via : Initial Calibration

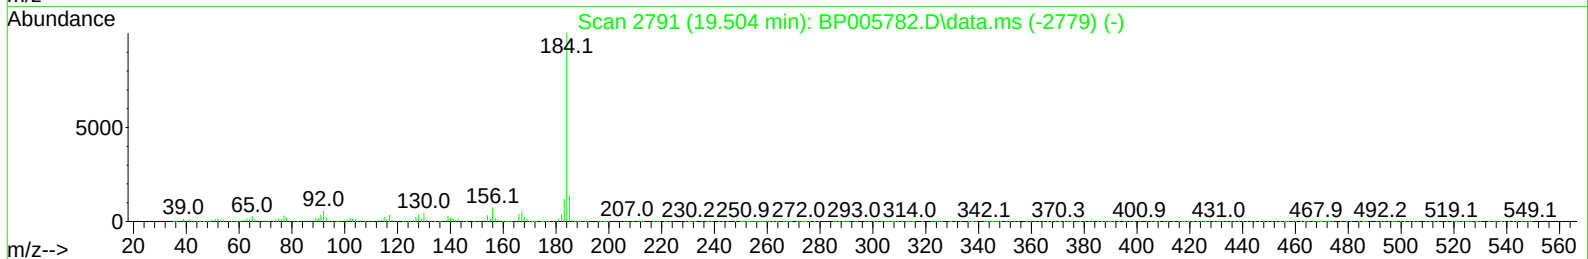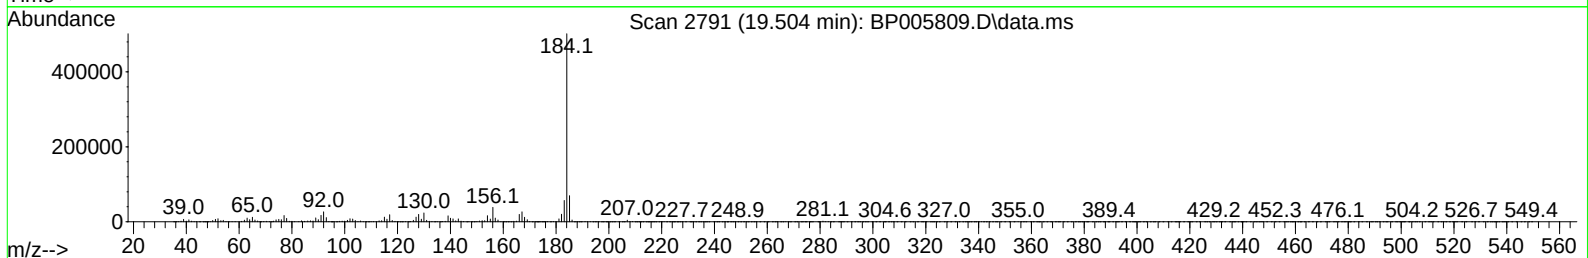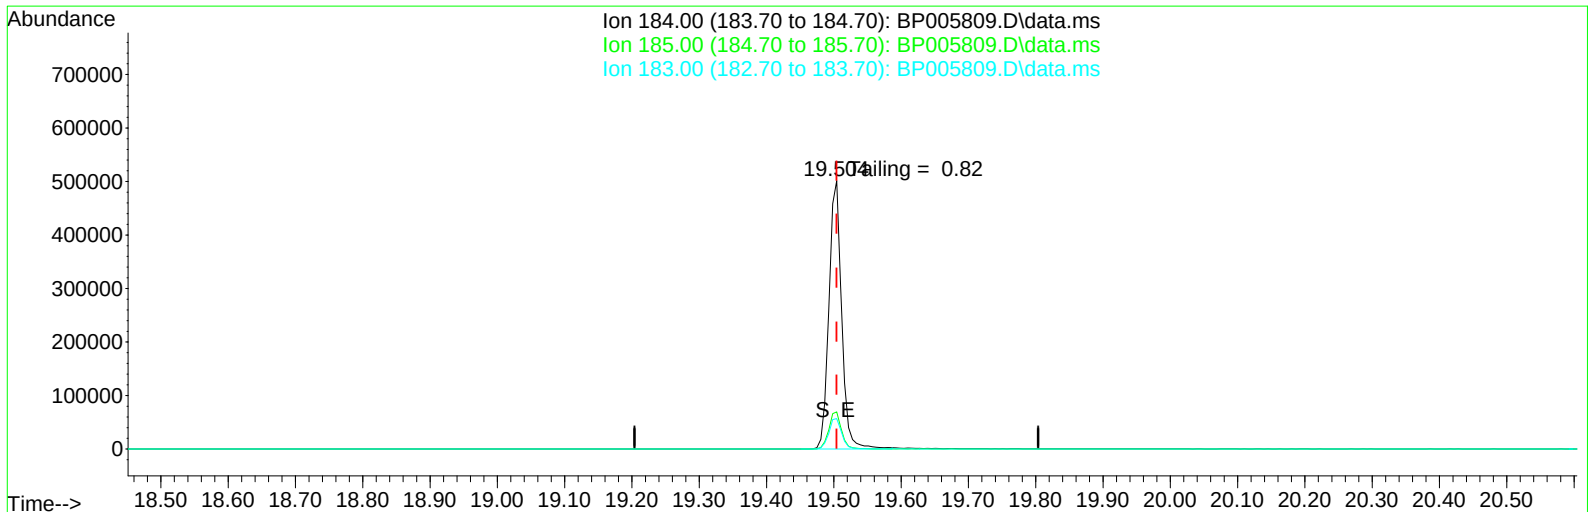

TIC: BP005809.D\data.ms

(77) Benzidine

19.504min (+ 0.000) 1507519.89 ng




response 658738

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.86
183.00	11.90	11.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060921\
 Data File : BP005809.D
 Acq On : 09 Jun 2021 14:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 09 16:37:43 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 09 11:54:55 2021
 Response via : Initial Calibration

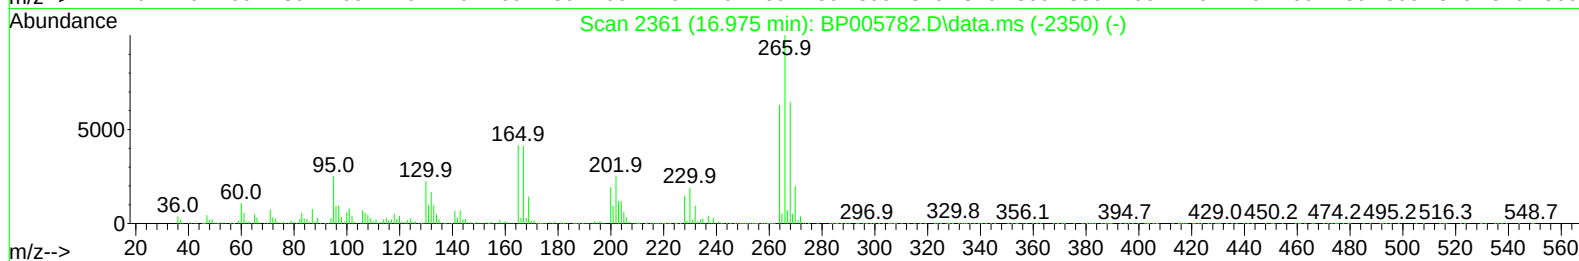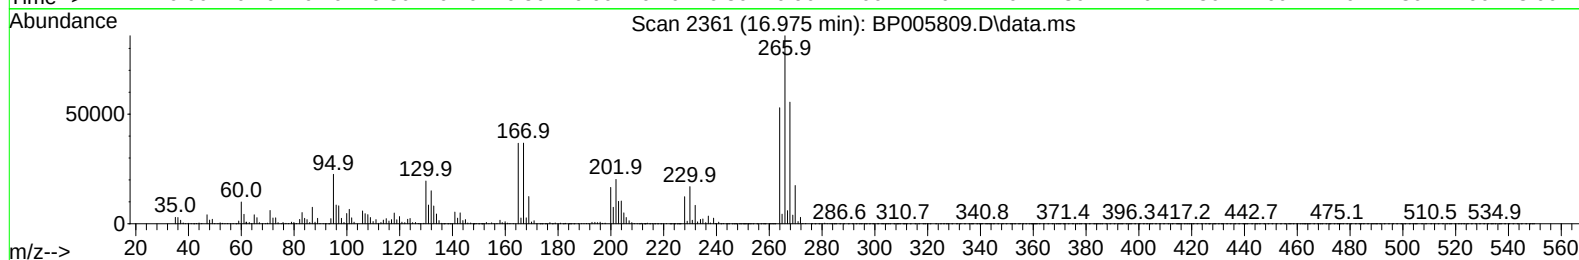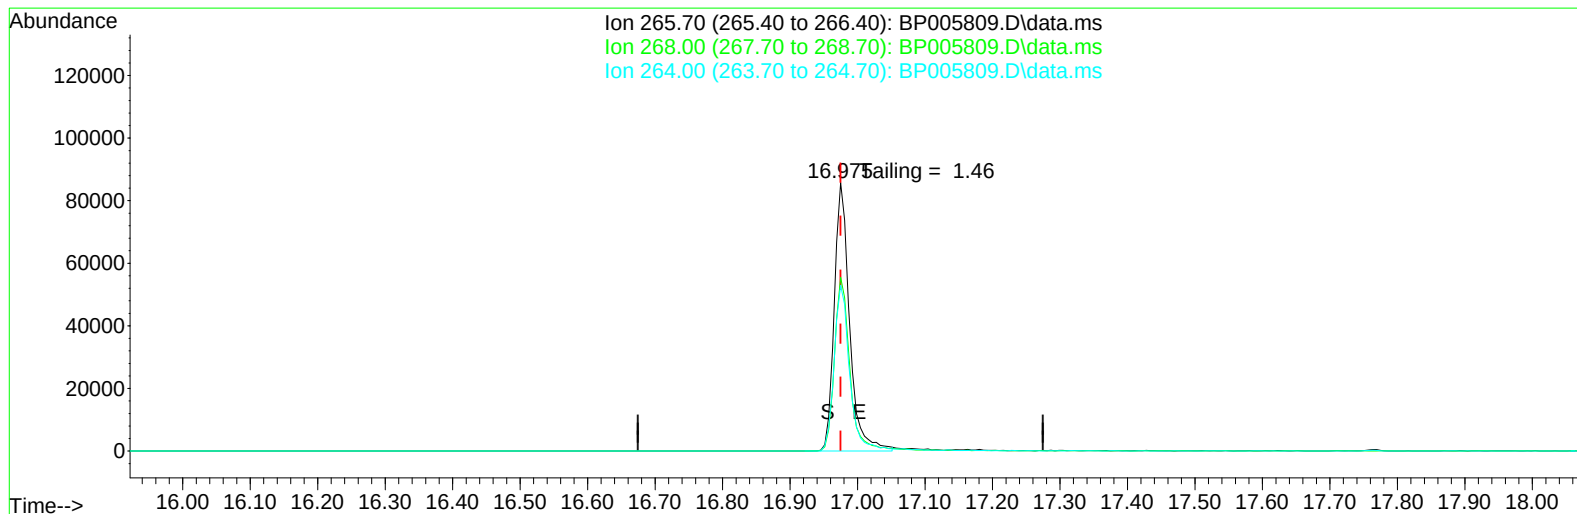

TIC: BP005809.D\data.ms

(70) Pentachlorophenol (C)

16.975min (+ 0.000) 139648.05 ng

response 136185

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.67
264.00	62.90	61.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/9/2021	BNA_P	<u>BP005809.D</u>
Compound Name	Response	Retention Time
DDT	372404	20.69
DDD	1299	20.27
DDE	751	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2050	374454	0.55