
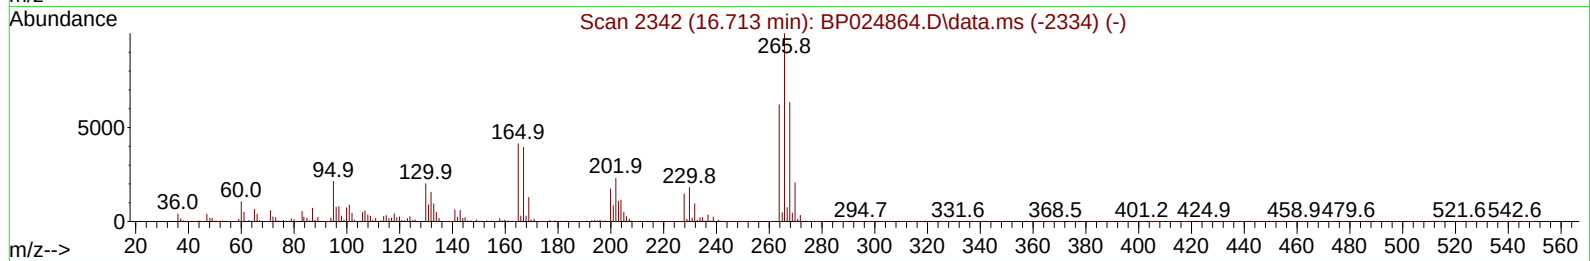
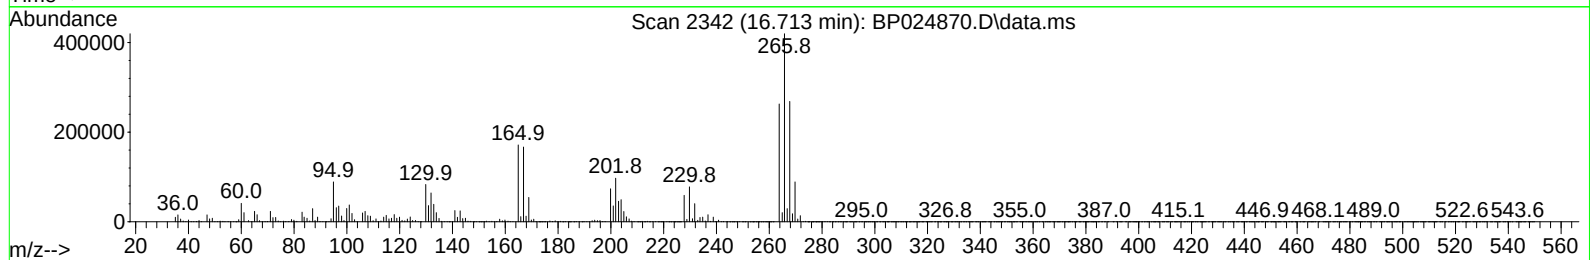


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP060925\  
Data File : BP024870.D  
Acq On : 09 Jun 2025 10:03  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 10:53:38 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP060625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jun 06 16:20:27 2025  
Response via : Initial Calibration

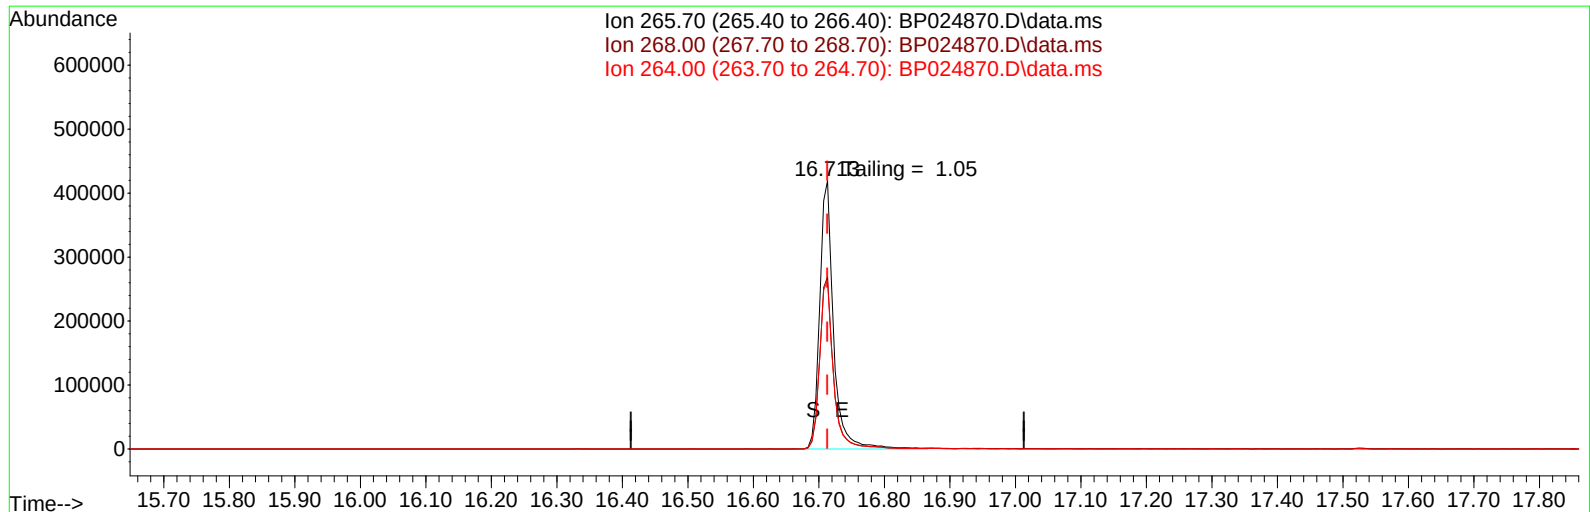

TIC: BP024870.D\data.ms

**(70) Pentachlorophenol (C)**




**16.713min (-0.000) 92926.84 ng**

**response 615758**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.30  | 64.02  |
| 264.00 | 62.10  | 62.65  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP060925\  
Data File : BP024870.D  
Acq On : 09 Jun 2025 10:03  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 10:53:38 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP060625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jun 06 16:20:27 2025  
Response via : Initial Calibration

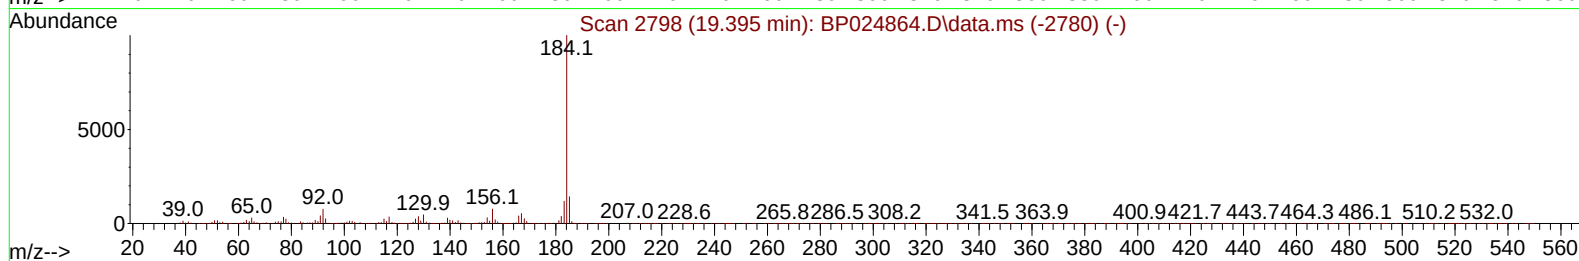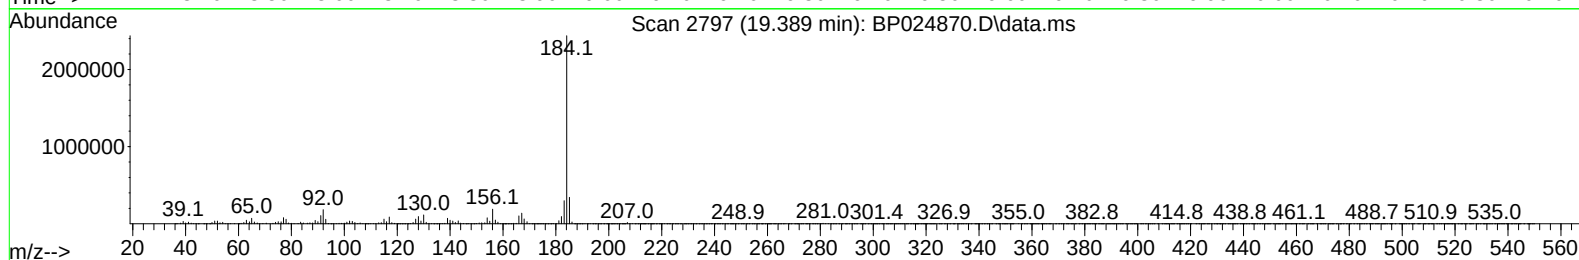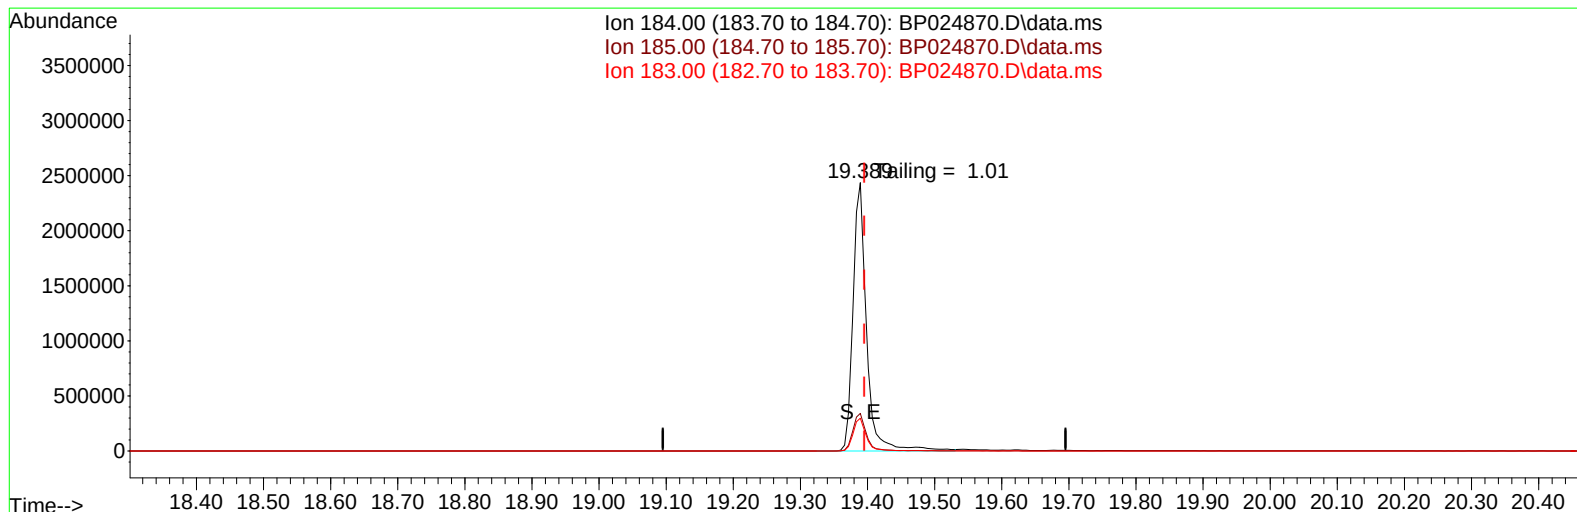

TIC: BP024870.D\data.ms

**(77) Benzidine****19.389min (-0.006) 1294.06 ng****response 3322112**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.20  | 14.01  |
| 183.00 | 11.90  | 12.23  |
| 0.00   | 0.00   | 0.00   |