
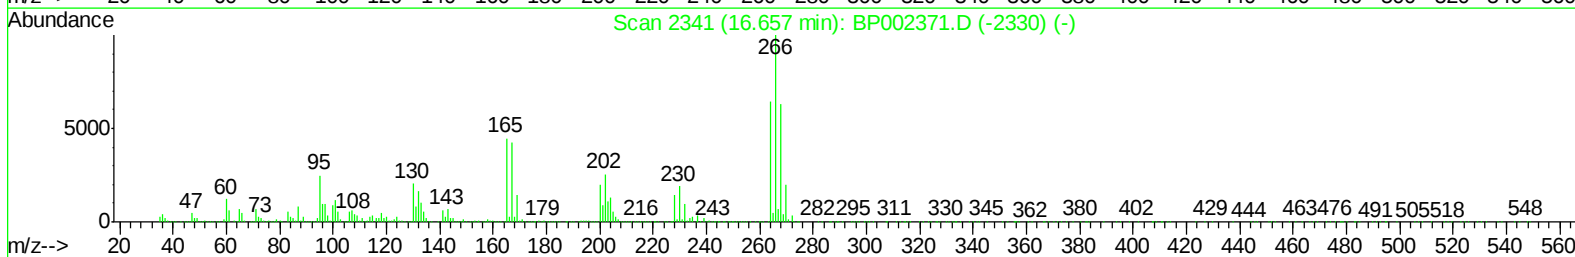
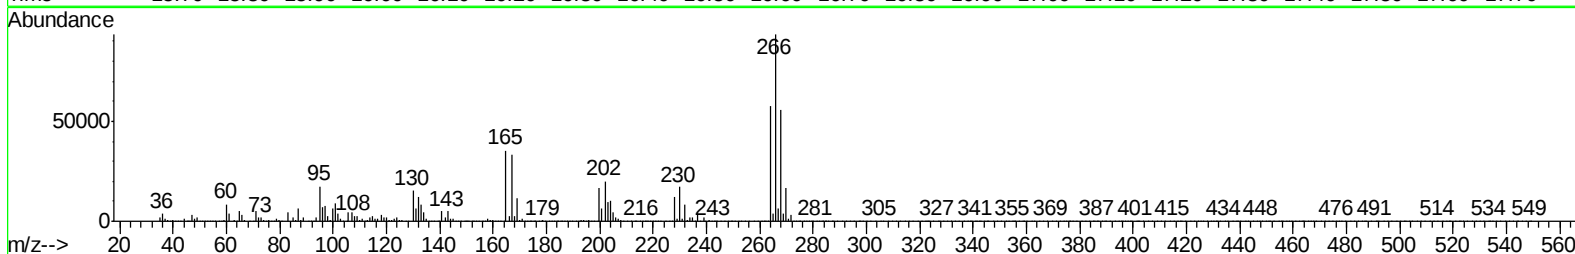


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP061020\
 Data File : BP002378.D
 Acq On : 10 Jun 2020 14:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 02:25:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 15:08:53 2020
 Response via : Initial Calibration

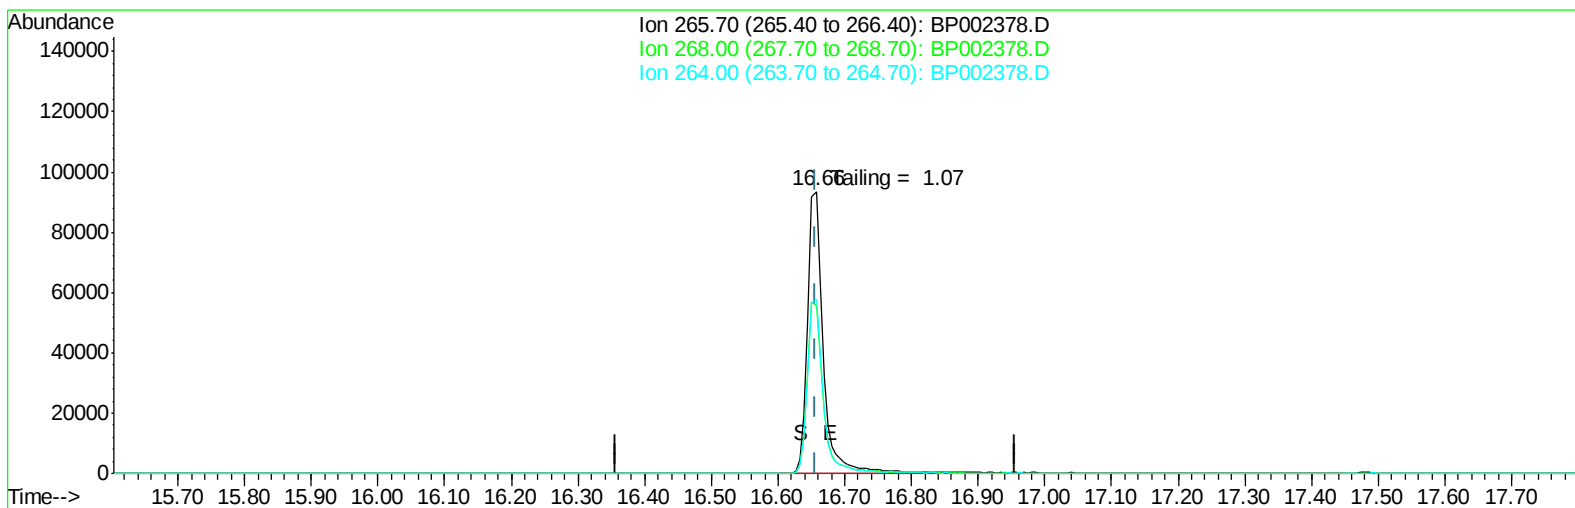

TIC: BP002378.D

(70) Pentachlorophenol (C)




16.657min (+0.000) 720305.06ng

response 147287

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	59.78
264.00	64.20	61.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP061020\
 Data File : BP002378.D
 Acq On : 10 Jun 2020 14:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 02:25:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 15:08:53 2020
 Response via : Initial Calibration

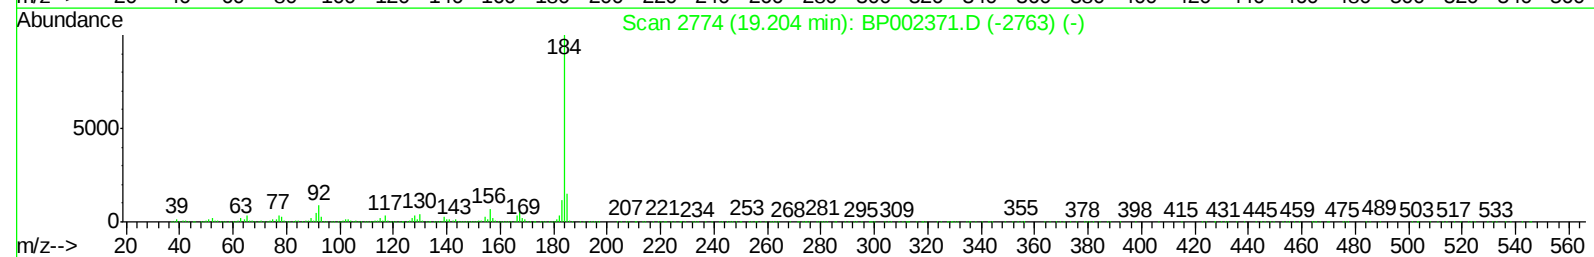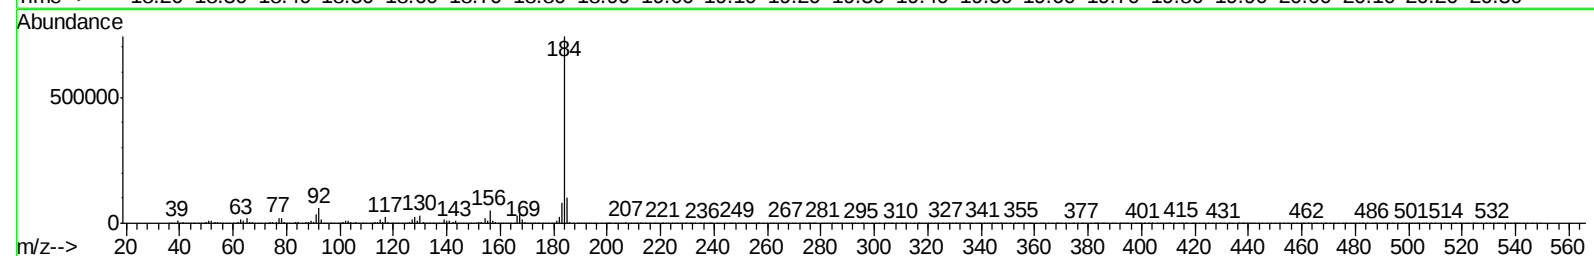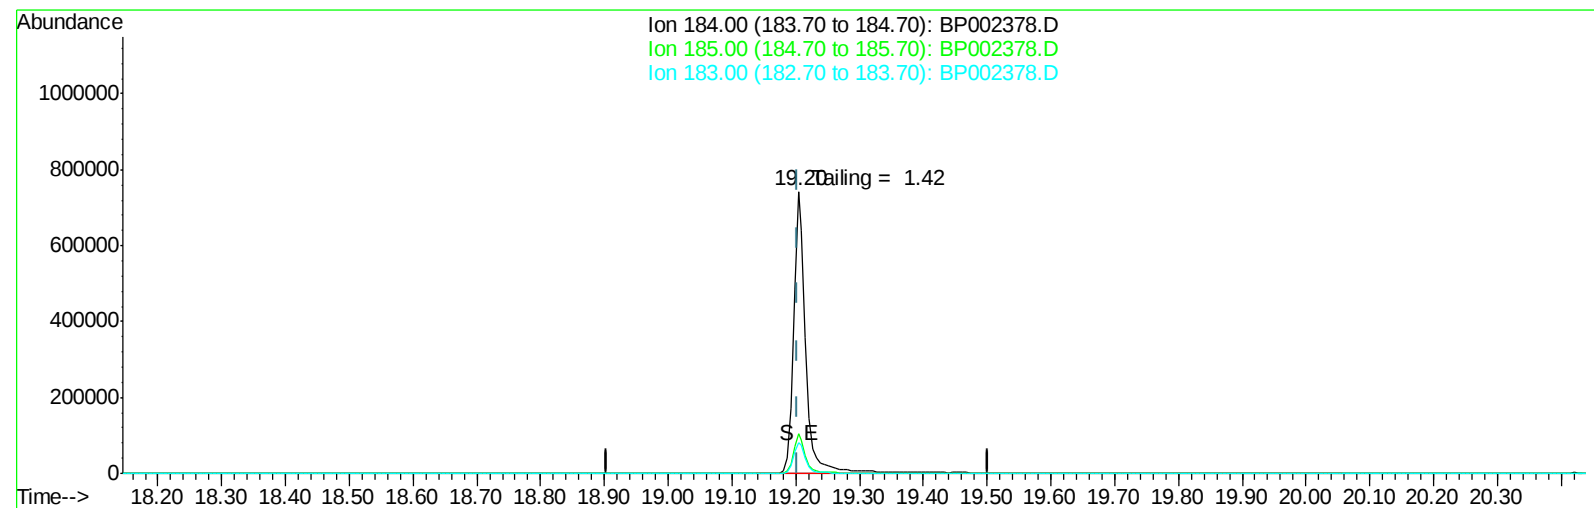

TIC: BP002378.D

(77) Benzidine

19.204min (+0.000) 515325.71ng

response 1036347

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.05
183.00	11.50	11.05
0.00	0.00	0.00