

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061020\
 Data File : BP002380.D
 Acq On : 10 Jun 2020 18:16
 Operator : CG/JU
 Sample : PB129455BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB129455BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.211	388	395	409	rBV	3012578	4516041	38.65%	8.324%
2	6.781	654	662	681	rBV	2855257	4627017	39.60%	8.528%
3	7.593	793	800	809	rBV	619326	987506	8.45%	1.820%
4	7.910	846	854	874	rBV	2608661	4195690	35.91%	7.733%
5	8.734	985	994	1015	rBV	1929375	3225859	27.61%	5.946%
6	10.363	1262	1271	1289	rBV	776096	1346687	11.53%	2.482%
7	12.857	1686	1695	1720	rBV	4778819	7447331	63.74%	13.727%
8	14.234	1920	1929	1942	rBV	1209118	1906637	16.32%	3.514%
9	15.734	2176	2184	2206	rBV	4056617	6005100	51.39%	11.068%
10	16.992	2391	2398	2411	rBV	1660173	2400444	20.54%	4.424%
11	19.586	2833	2839	2855	rBV	8945949	11684814	100.00%	21.537%
12	21.098	3091	3096	3107	rBV	2300522	2897995	24.80%	5.342%
13	23.292	3463	3469	3480	rVB	1648613	3012976	25.79%	5.553%




Sum of corrected areas: 54254097

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061020\
Data File : BP002380.D
Acq On : 10 Jun 2020 18:16
Operator : CG/JU
Sample : PB129455BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129455BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

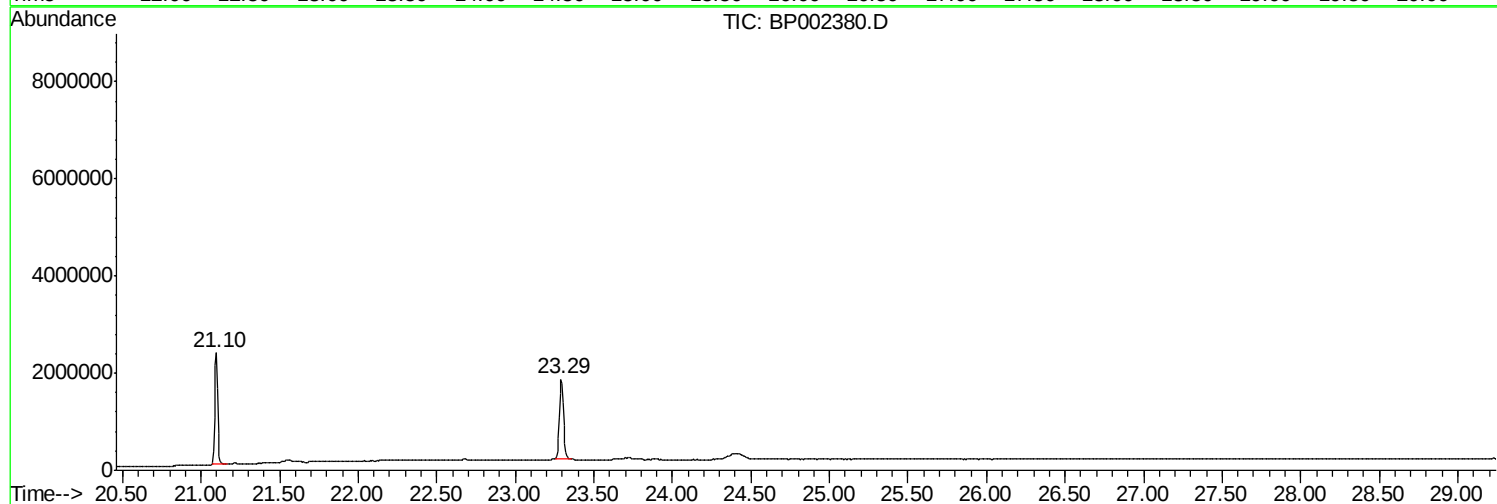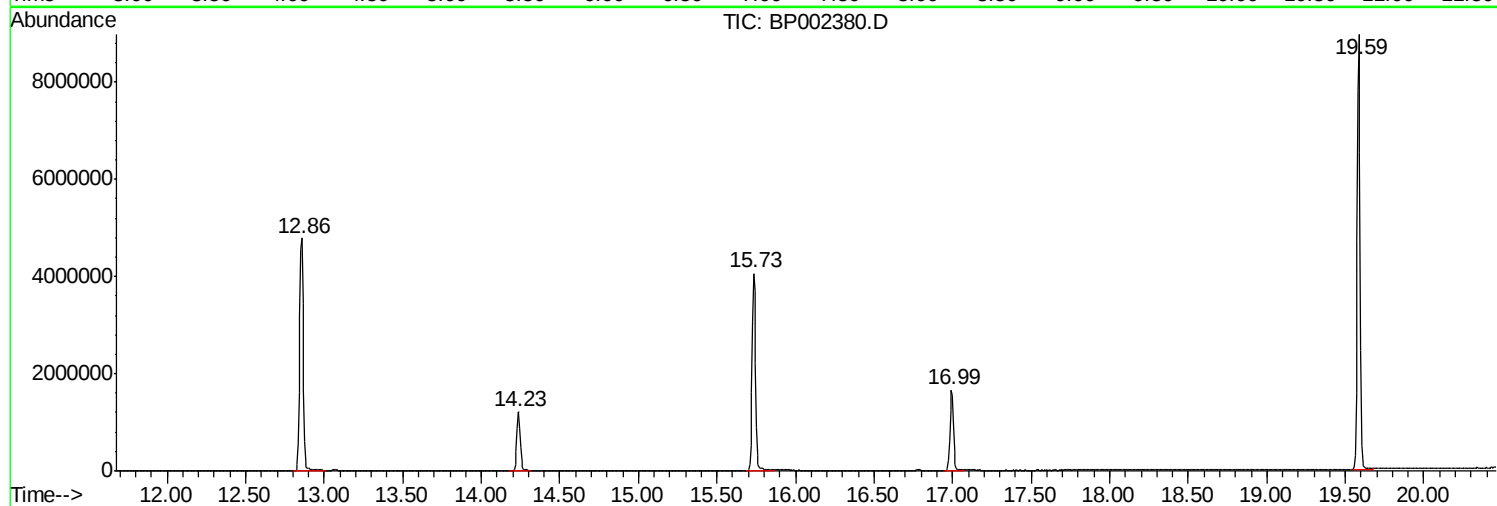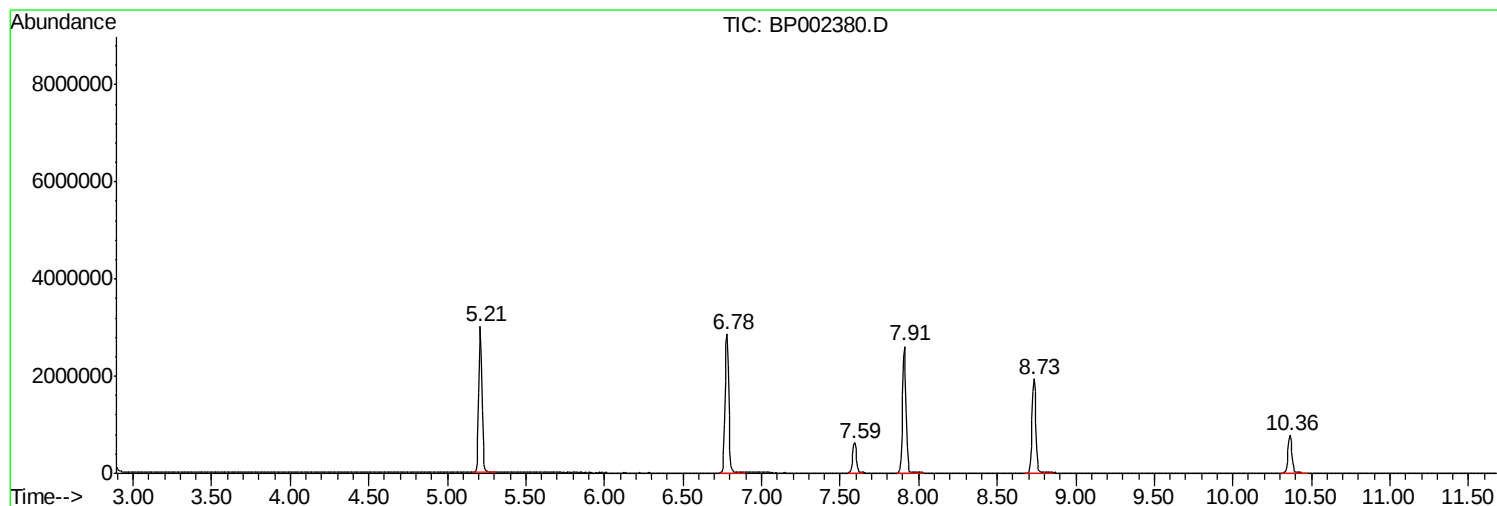

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP061020\
Data File : BP002380.D
Acq On : 10 Jun 2020 18:16
Operator : CG/JU
Sample : PB129455BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129455BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP061020\
Data File : BP002380.D
Acq On : 10 Jun 2020 18:16
Operator : CG/JU
Sample : PB129455BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129455BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc