

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP061020\
 Data File : BP002381.D
 Acq On : 10 Jun 2020 18:50
 Operator : CG/JU
 Sample : PB129457BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB129457BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.211	388	395	415	rBV	2732552	4151395	36.23%	7.516%
2	6.781	654	662	681	rBV	2619444	4303395	37.55%	7.791%
3	7.593	793	800	810	rBV	724565	1158251	10.11%	2.097%
4	7.911	843	854	865	rBV	2435418	3927014	34.27%	7.109%
5	8.734	985	994	1012	rBV	1854873	3019830	26.35%	5.467%
6	10.363	1263	1271	1287	rBV	938297	1609412	14.04%	2.914%
7	12.857	1687	1695	1719	rBV	4469368	7184842	62.70%	13.007%
8	14.240	1921	1930	1942	rBV	1521690	2338498	20.41%	4.234%
9	15.734	2173	2184	2205	rBV	3891417	5866107	51.19%	10.620%
10	16.992	2391	2398	2412	rBV	2042996	2959497	25.83%	5.358%
11	19.586	2833	2839	2854	rBV	8521195	11459530	100.00%	20.746%
12	21.098	3091	3096	3108	rBV	2821944	3573069	31.18%	6.469%
13	23.298	3463	3470	3483	rVB	1949104	3685976	32.17%	6.673%




Sum of corrected areas: 55236816

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061020\
Data File : BP002381.D
Acq On : 10 Jun 2020 18:50
Operator : CG/JU
Sample : PB129457BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129457BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

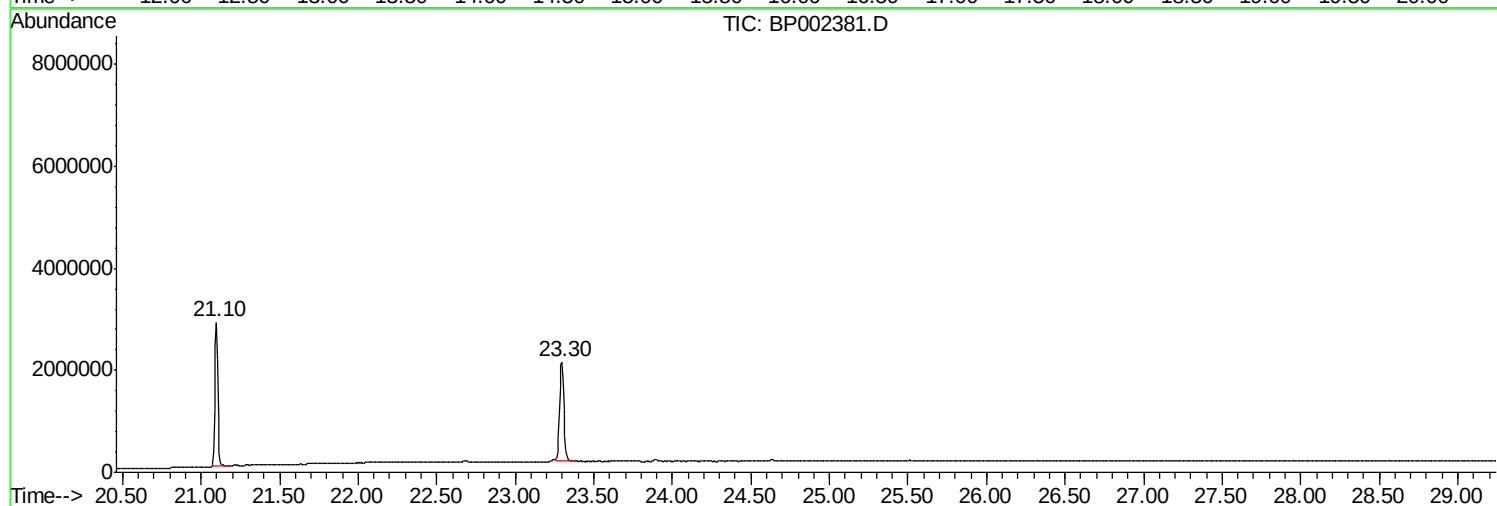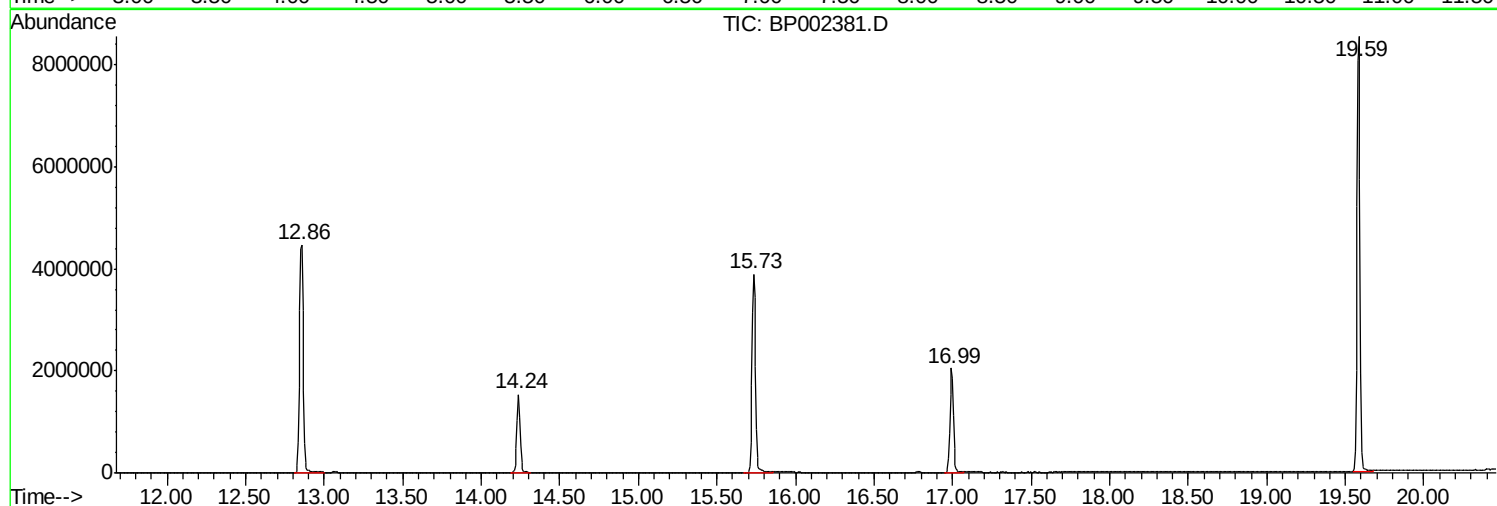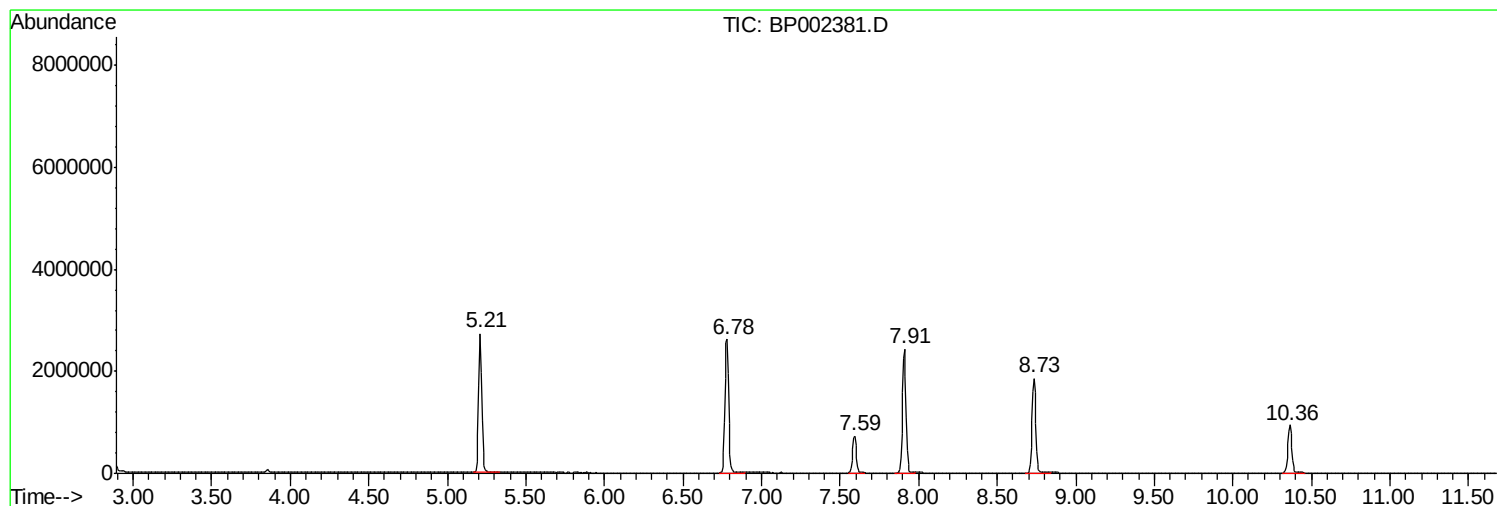

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP061020\
Data File : BP002381.D
Acq On : 10 Jun 2020 18:50
Operator : CG/JU
Sample : PB129457BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129457BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP061020\
Data File : BP002381.D
Acq On : 10 Jun 2020 18:50
Operator : CG/JU
Sample : PB129457BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129457BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc