


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061020\
 Data File : BP002378.D
 Acq On : 10 Jun 2020 14:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 05 15:08:53 2020

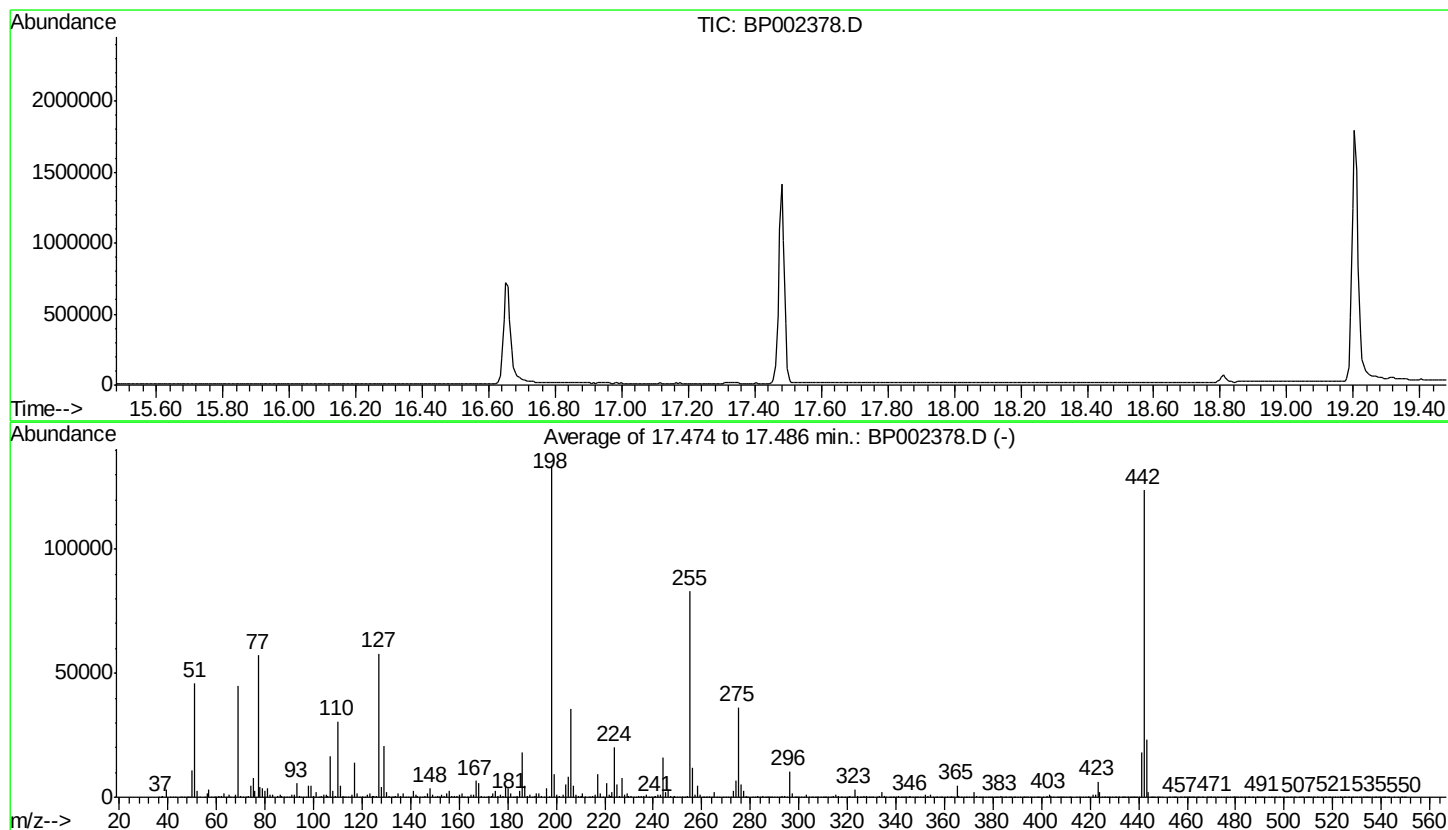

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	45958	PASS
68	69	0.00	2	2.0	886	PASS
69	198	0.00	100	33.7	45026	PASS
70	69	0.00	2	0.6	286	PASS
127	198	10	80	43.3	57848	PASS
197	198	0.00	2	0.2	212	PASS
198	198	100	100	100.0	133746	PASS
199	198	5	9	7.0	9355	PASS
275	198	10	60	27.2	36341	PASS
365	198	1	100	3.5	4685	PASS
441	198	0.01	100	13.7	18326	PASS
442	198	50	100	92.7	123954	PASS
443	442	15	24	18.8	23282	PASS