
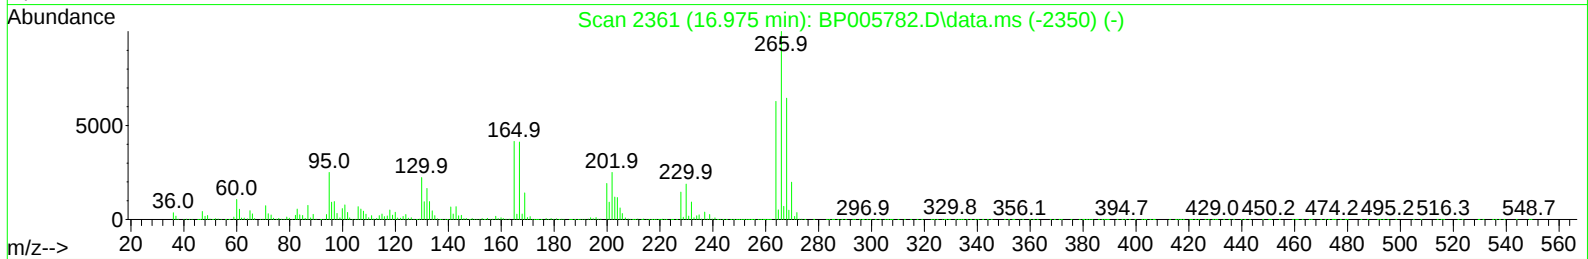
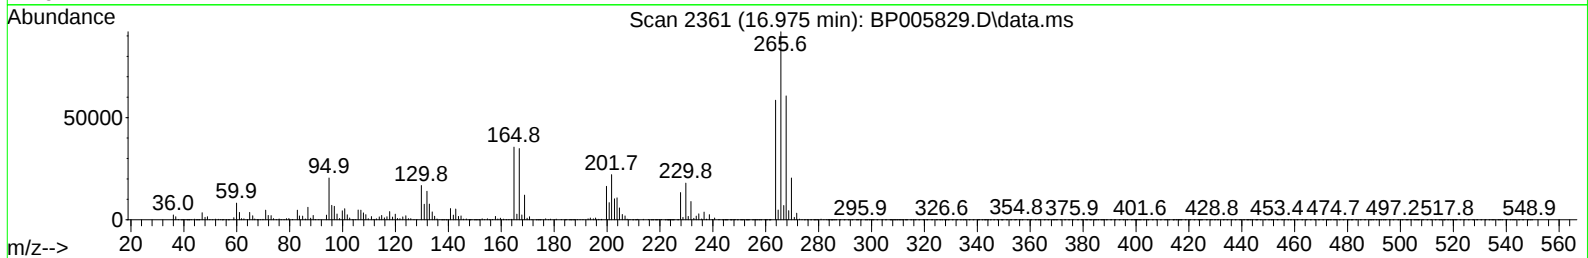


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061021\
 Data File : BP005829.D
 Acq On : 10 Jun 2021 10:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 11:49:26 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 09 11:54:55 2021
 Response via : Initial Calibration

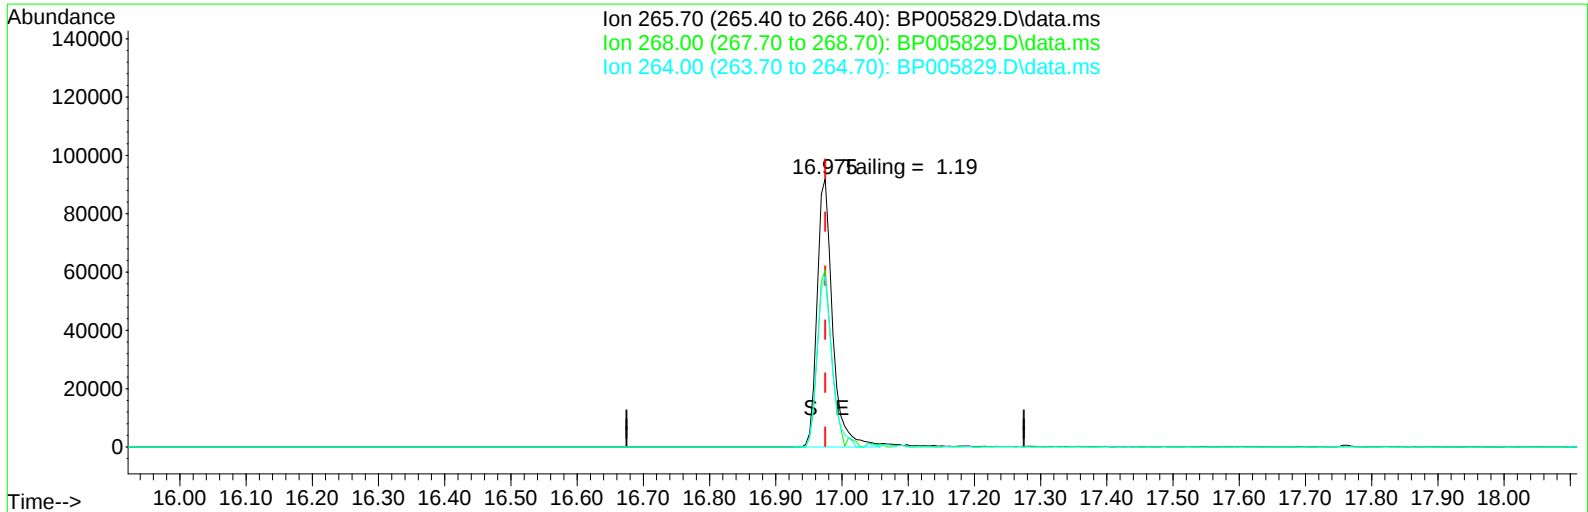

TIC: BP005829.D\data.ms

(70) Pentachlorophenol (C)




16.975min (-0.000) 1614841.51 ng

response 151954

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	70.71
264.00	62.90	68.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061021\
 Data File : BP005829.D
 Acq On : 10 Jun 2021 10:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 11:49:26 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 09 11:54:55 2021
 Response via : Initial Calibration

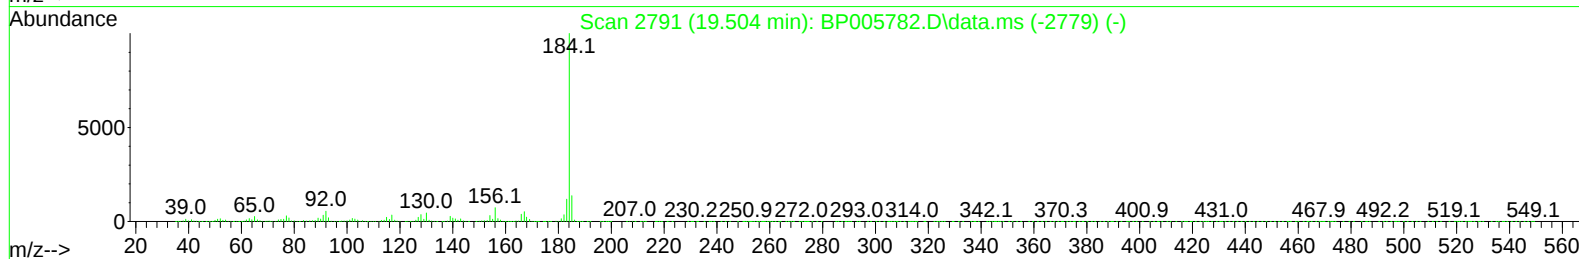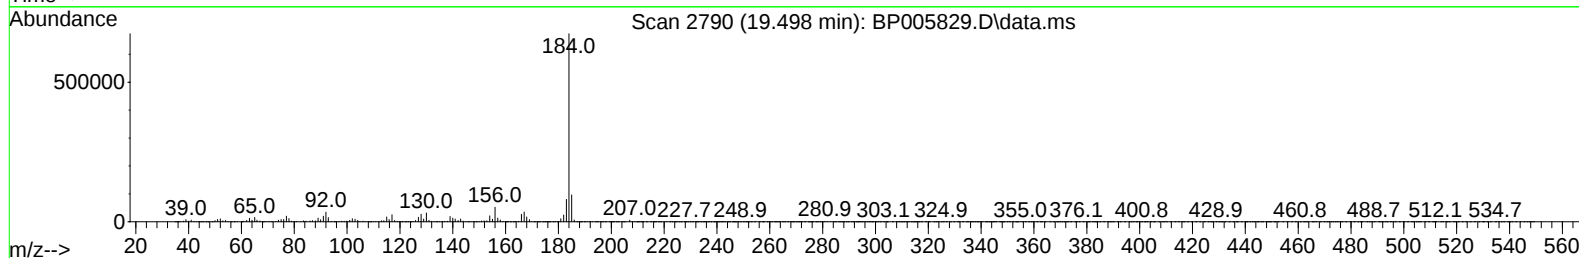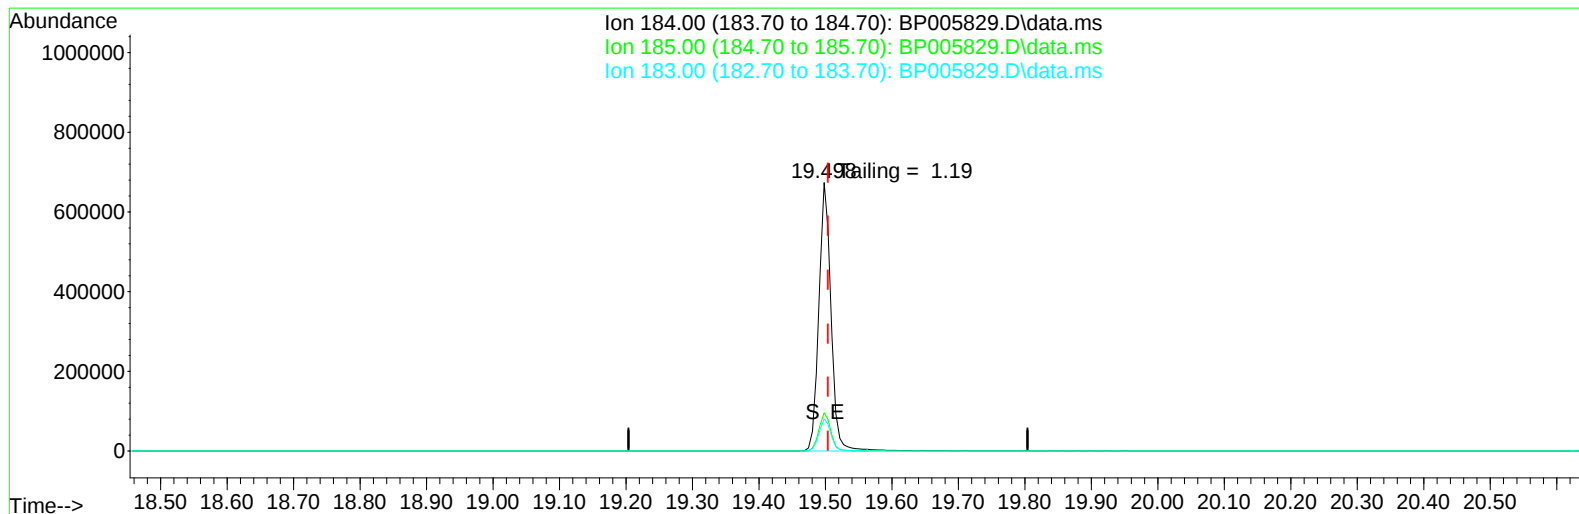

TIC: BP005829.D\data.ms

(77) Benzidine**19.498min (-0.006) 207698.85 ng****response 855716**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.27
183.00	11.90	11.96
0.00	0.00	0.00