
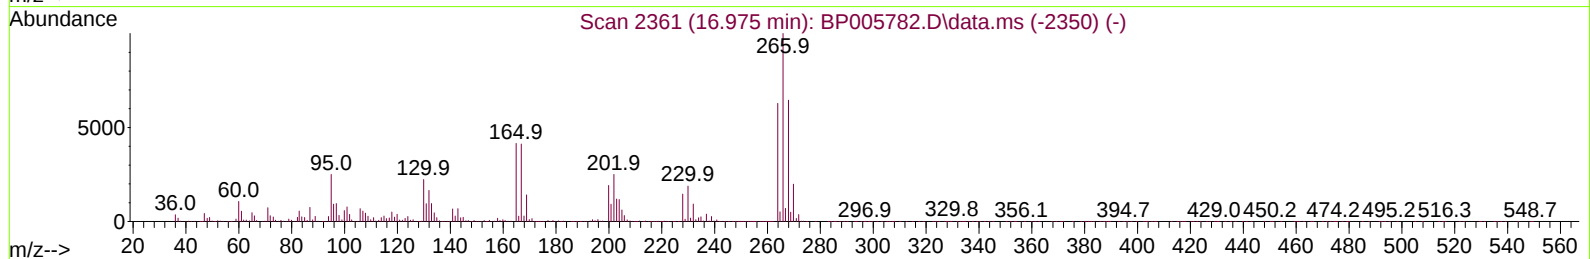
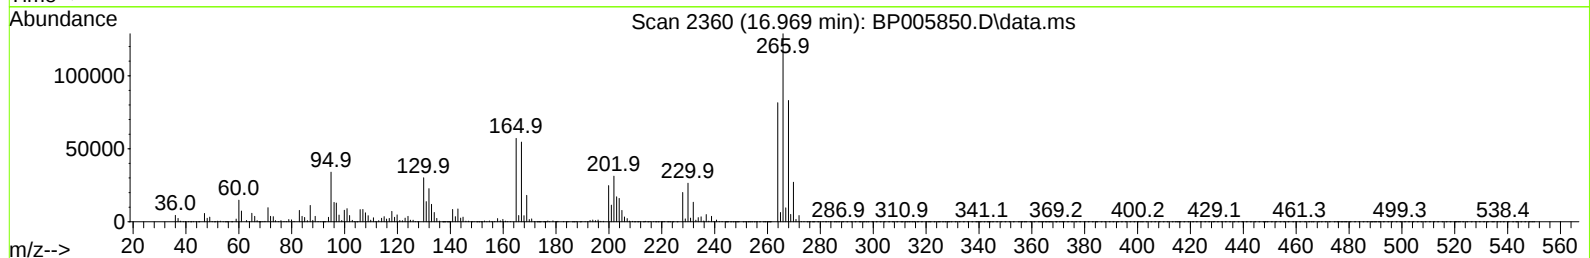


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP061021\  
Data File : BP005850.D  
Acq On : 10 Jun 2021 23:16  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 07:25:51 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP060821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jun 09 11:54:55 2021  
Response via : Initial Calibration

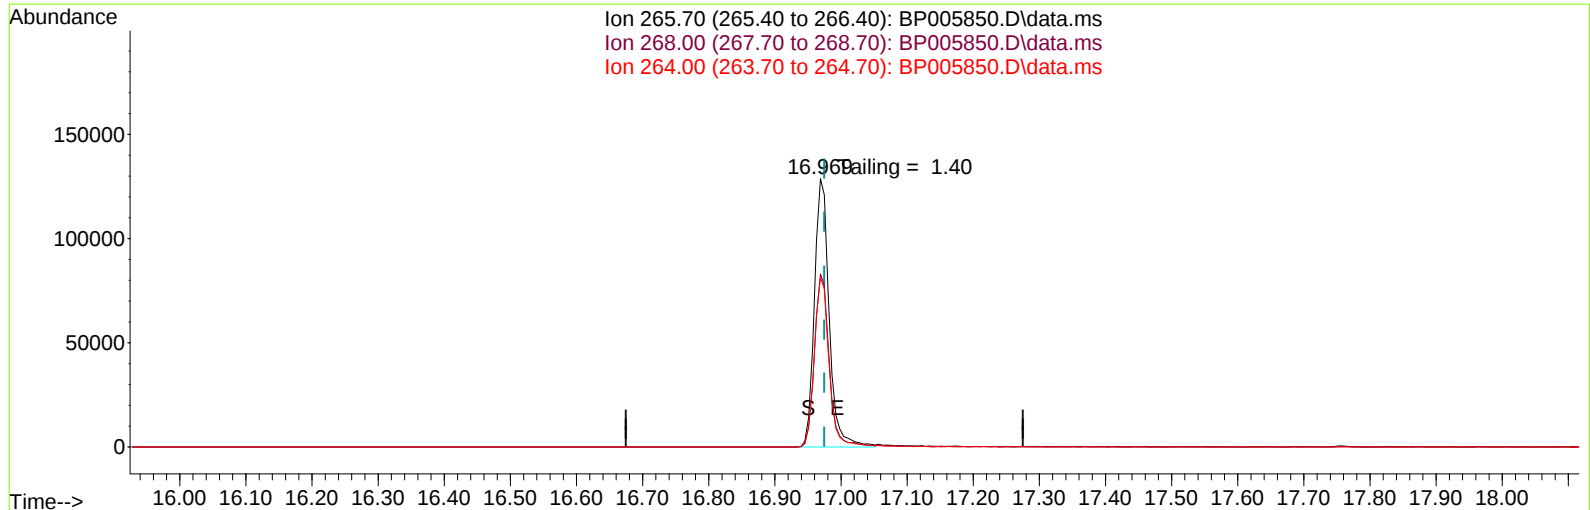

TIC: BP005850.D\data.ms

**(70) Pentachlorophenol (C)**




16.969min (-0.006) 643983.09 ng

response 198320

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.50  | 64.49  |
| 264.00 | 62.90  | 63.32  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP061021\  
 Data File : BP005850.D  
 Acq On : 10 Jun 2021 23:16  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 07:25:51 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP060821.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Jun 09 11:54:55 2021  
 Response via : Initial Calibration

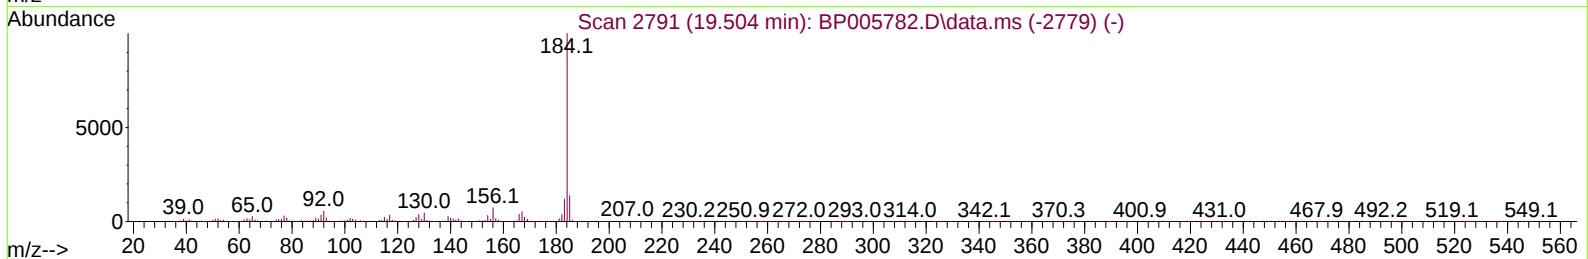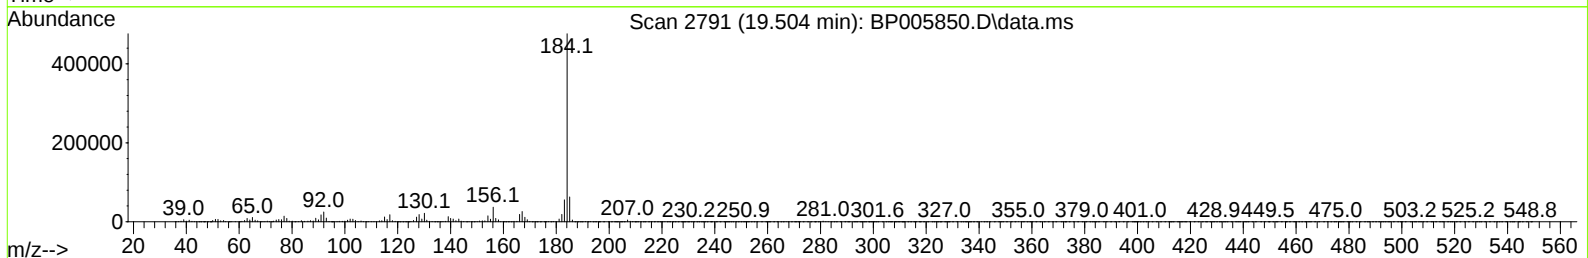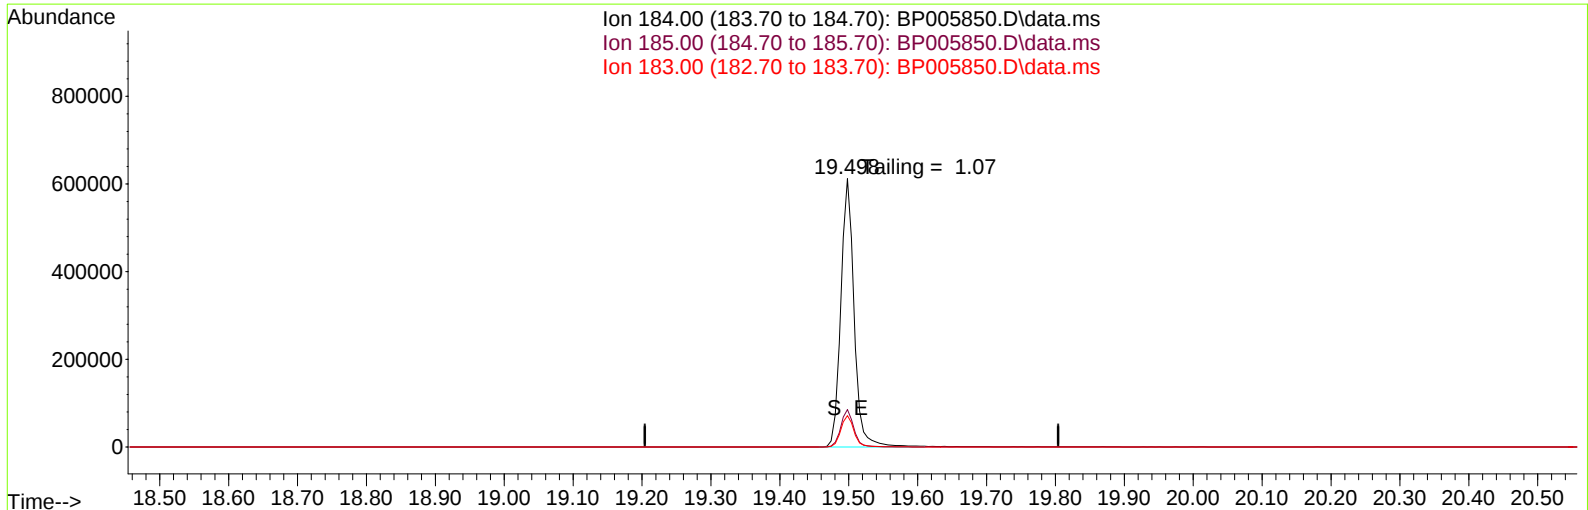

TIC: BP005850.D\data.ms

**(77) Benzidine****19.504min (-19.504) 0.00 ng****response 0**

| Ion    | Exp%   | Act%  |
|--------|--------|-------|
| 184.00 | 100.00 | 0.00  |
| 185.00 | 13.70  | 0.00# |
| 183.00 | 11.90  | 0.00# |
| 0.00   | 0.00   | 0.00  |