

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061021\
 Data File : BP005854.D
 Acq On : 11 Jun 2021 02:40
 Operator : CG/JU
 Sample : M2612-26
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 18-B12(26-30)

Quant Time: Jun 11 07:03:01 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 09 11:54:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	70134	20.000	ng	-0.01
21) Naphthalene-d8	10.751	136	253749	20.000	ng	-0.01
39) Acenaphthene-d10	14.575	164	158179	20.000	ng	0.00
64) Phenanthrene-d10	17.316	188	338150	20.000	ng	-0.01
76) Chrysene-d12	21.386	240	389727	20.000	ng	0.00
86) Perylene-d12	23.804	264	462219	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.510	112	494911	113.233	ng	0.00
7) Phenol-d6	7.110	99	533254	94.130	ng	-0.01
23) Nitrobenzene-d5	9.110	82	382194	73.844	ng	-0.01
42) 2,4,6-Tribromophenol	16.063	330	318427	117.307	ng	0.00
45) 2-Fluorobiphenyl	13.204	172	885961	73.549	ng	-0.01
79) Terphenyl-d14	19.863	244	1592023	76.491	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061021\
Data File : BP005854.D
Acq On : 11 Jun 2021 02:40
Operator : CG/JU
Sample : M2612-26
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
18-B12(26-30)

Quant Time: Jun 11 07:03:01 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 09 11:54:55 2021
Response via : Initial Calibration




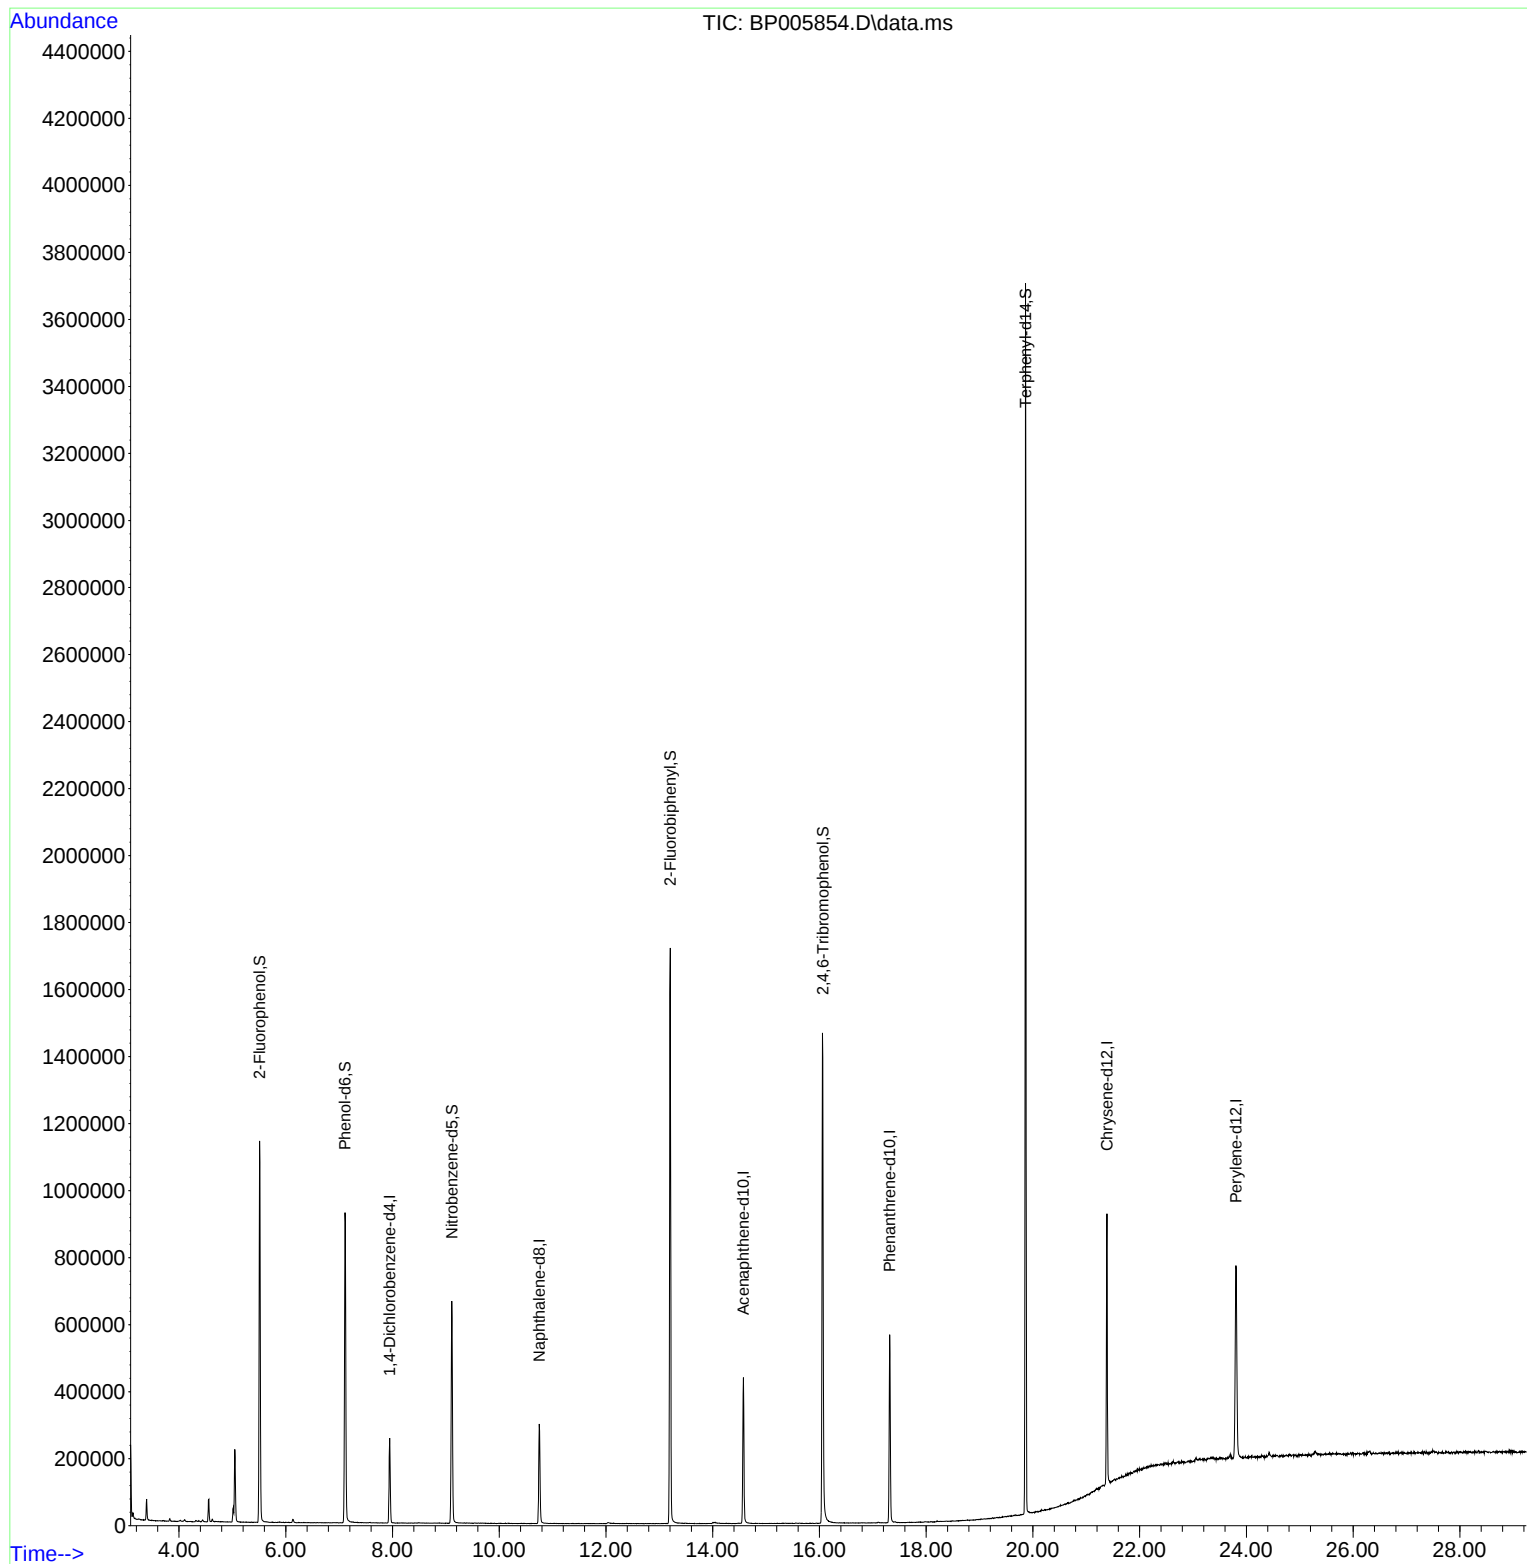


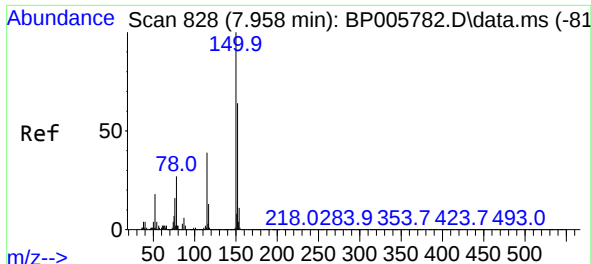

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.946 min Scan# 826
Delta R.T. -0.012 min
Lab File: BP005854.D
Acq: 11 Jun 2021 02:40




Instrument :
BNA_P
ClientSampleId :
18-B12(26-30)


Tgt Ion:152 Resp: 70134
Ion Ratio Lower Upper
152 100
150 159.0 125.6 188.4
115 61.4 48.5 72.7

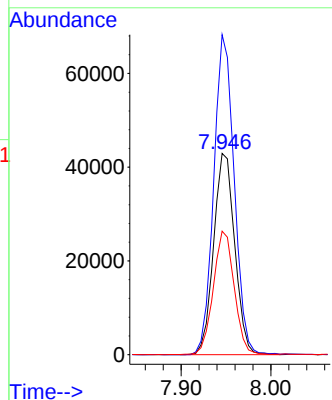

#5
2-Fluorophenol
Concen: 113.233 ng
RT: 5.510 min Scan# 412
Delta R.T. -0.007 min
Lab File: BP005854.D
Acq: 11 Jun 2021 02:40

Tgt Ion:112 Resp: 494911
Ion Ratio Lower Upper
112 100
64 51.0 41.4 62.2
63 29.1 23.8 35.8


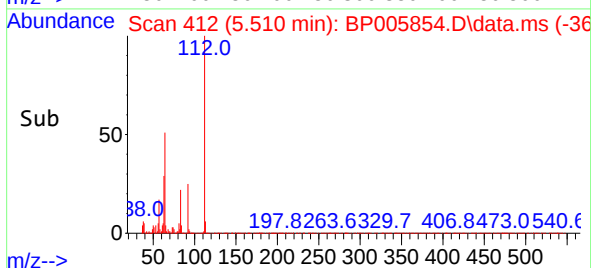
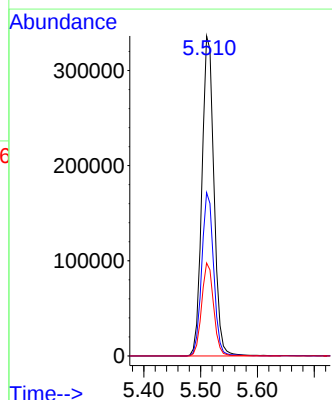
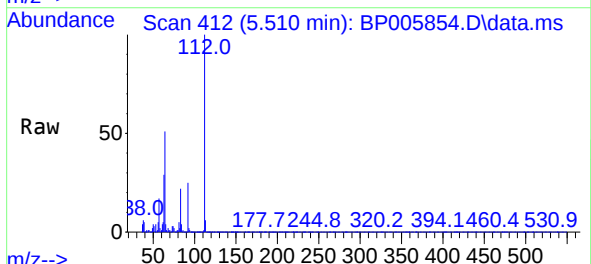


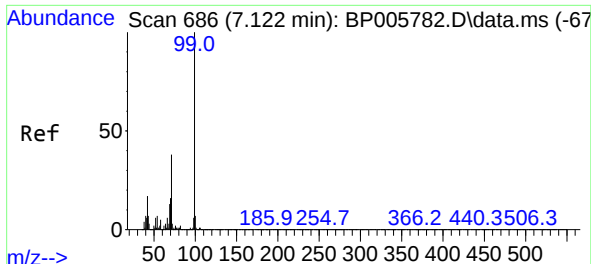

#7
Phenol-d6
Concen: 94.130 ng
RT: 7.110 min Scan# 684
Delta R.T. -0.012 min
Lab File: BP005854.D
Acq: 11 Jun 2021 02:40




Instrument :
BNA_P
ClientSampleId :
18-B12(26-30)


Tgt Ion: 99 Resp: 533254
Ion Ratio Lower Upper
99 100
42 16.4 13.4 20.0
71 39.7 30.6 46.0

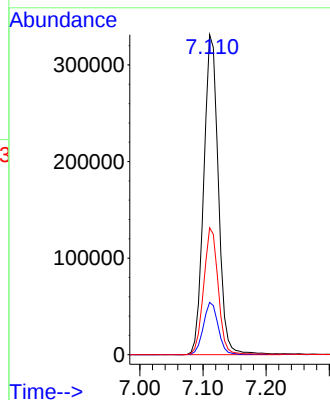

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.751 min Scan# 1303
Delta R.T. -0.012 min
Lab File: BP005854.D
Acq: 11 Jun 2021 02:40

Tgt Ion: 136 Resp: 253749
Ion Ratio Lower Upper
136 100
137 11.2 8.6 12.8
54 5.7 4.6 6.8
68 4.3 3.6 5.4


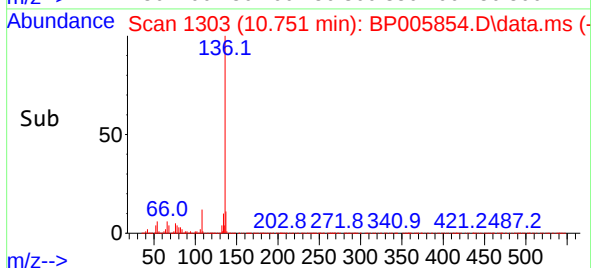
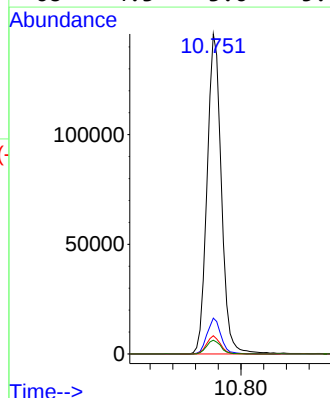
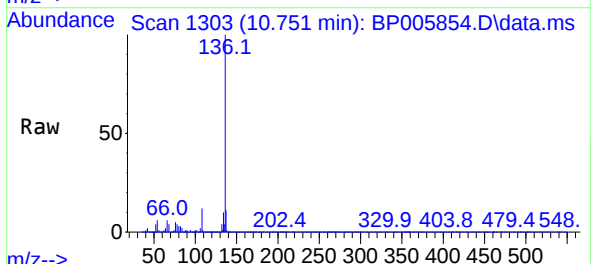


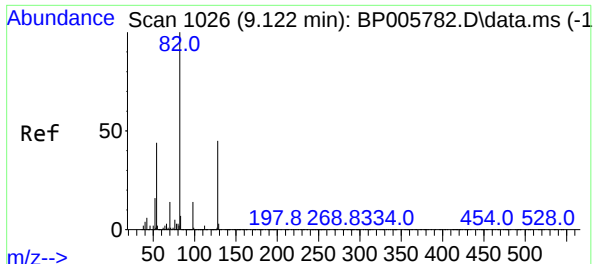

#23
Nitrobenzene-d5
Concen: 73.844 ng
RT: 9.110 min Scan# 1024
Delta R.T. -0.012 min
Lab File: BP005854.D
Acq: 11 Jun 2021 02:40




Instrument :
BNA_P
ClientSampleId :
18-B12(26-30)

Tgt Ion: 82 Resp: 382194
Ion Ratio Lower Upper
82 100
128 44.3 35.7 53.5
54 43.6 35.0 52.4

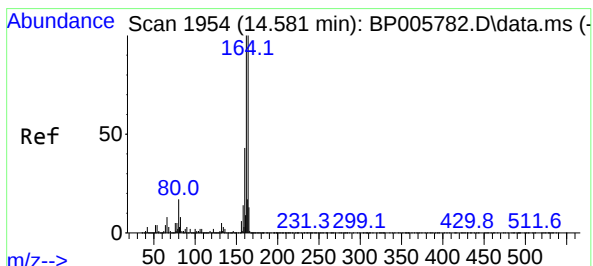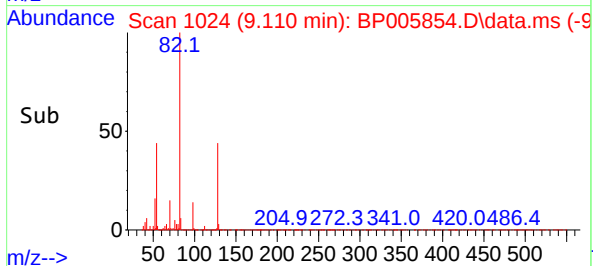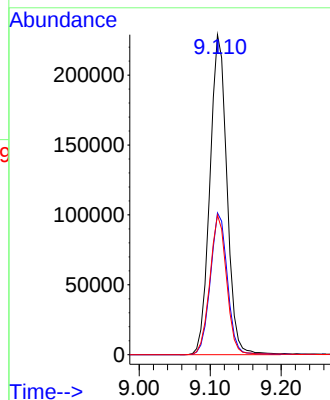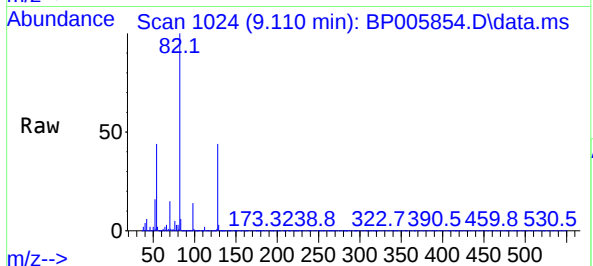

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.575 min Scan# 1953
Delta R.T. -0.006 min
Lab File: BP005854.D
Acq: 11 Jun 2021 02:40

Tgt Ion: 164 Resp: 158179
Ion Ratio Lower Upper
164 100
162 102.7 80.2 120.2
160 44.5 34.5 51.7


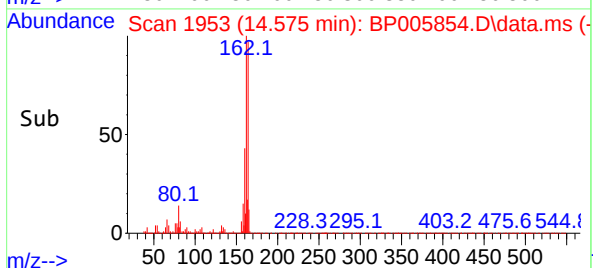
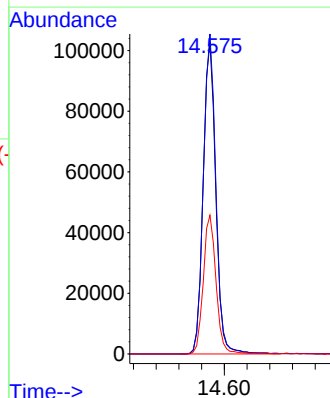
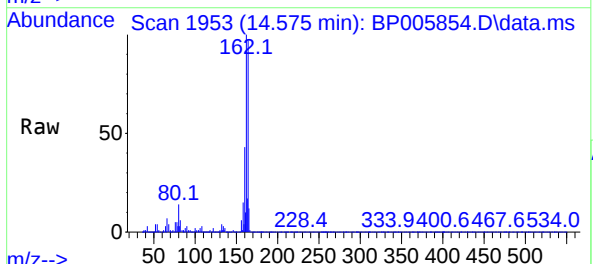




#42
2,4,6-Tribromophenol
Concen: 117.307 ng
RT: 16.063 min Scan# 2206
Delta R.T. -0.006 min
Lab File: BP005854.D
Acq: 11 Jun 2021 02:40




Instrument :
BNA_P
ClientSampleId :
18-B12(26-30)


Tgt Ion: 330 Resp: 318427
Ion Ratio Lower Upper
330 100
332 97.5 77.8 116.8
141 33.1 25.4 38.2

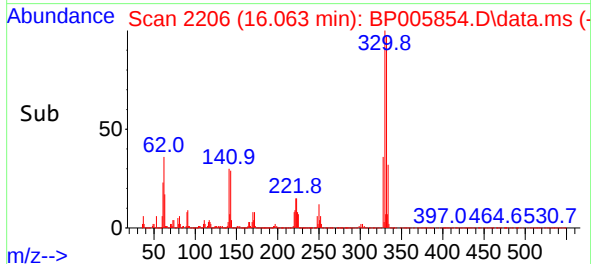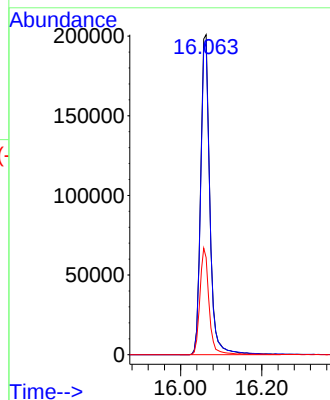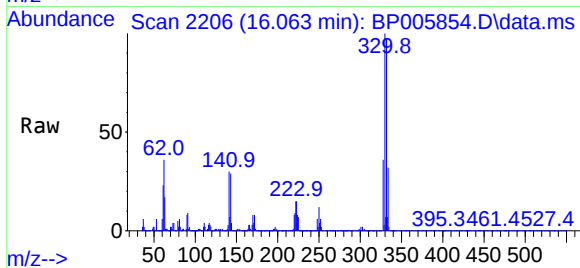

#45
2-Fluorobiphenyl
Concen: 73.549 ng
RT: 13.204 min Scan# 1720
Delta R.T. -0.012 min
Lab File: BP005854.D
Acq: 11 Jun 2021 02:40

Tgt Ion: 172 Resp: 885961
Ion Ratio Lower Upper
172 100
171 35.8 27.9 41.9
170 23.2 18.6 27.8


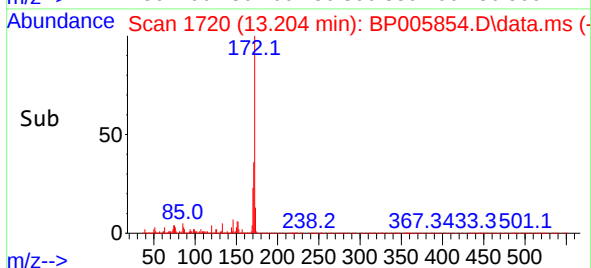
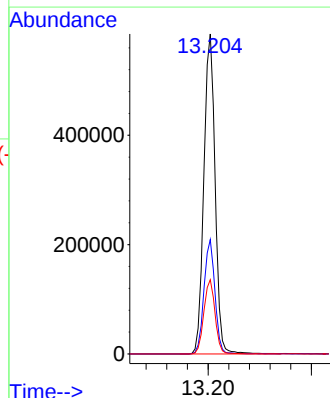
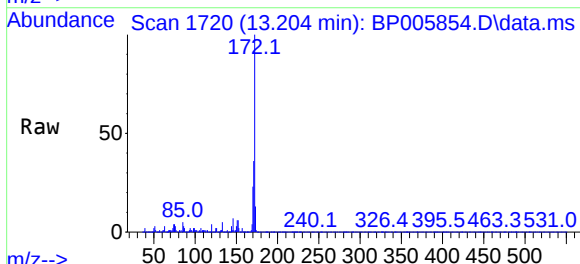




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.316 min Scan# 2419
Delta R.T. -0.012 min
Lab File: BP005854.D
Acq: 11 Jun 2021 02:40




Instrument :
BNA_P
ClientSampleId :
18-B12(26-30)


Tgt Ion:188 Resp: 338150
Ion Ratio Lower Upper
188 100
94 6.9 5.6 8.4
80 7.5 6.3 9.5

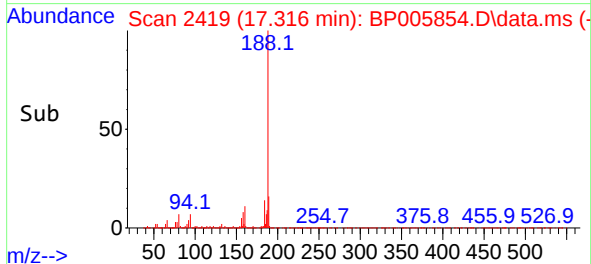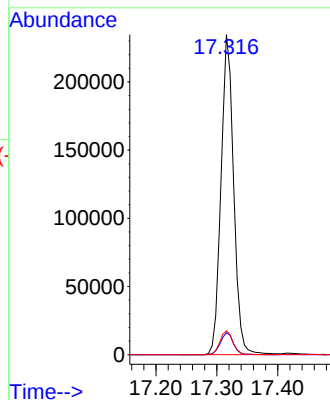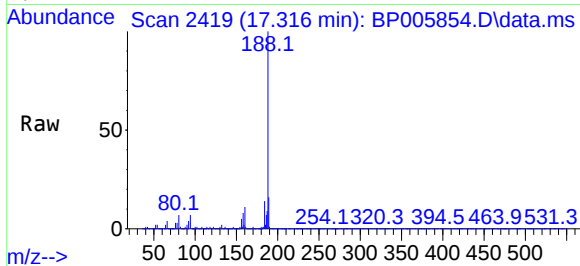

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.386 min Scan# 3111
Delta R.T. -0.006 min
Lab File: BP005854.D
Acq: 11 Jun 2021 02:40

Tgt Ion:240 Resp: 389727
Ion Ratio Lower Upper
240 100
120 7.9 6.5 9.7
236 24.9 20.6 31.0


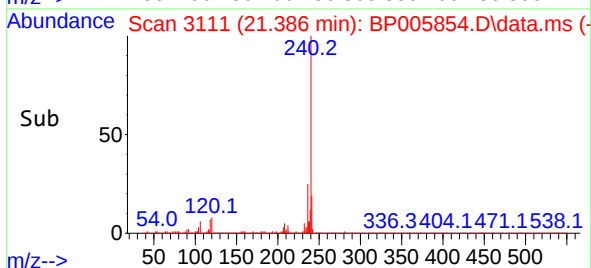
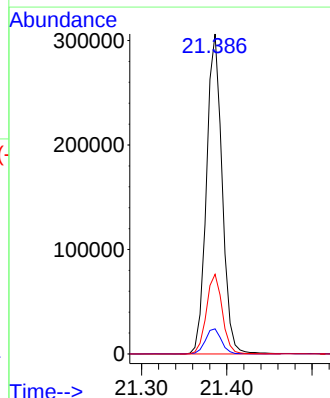
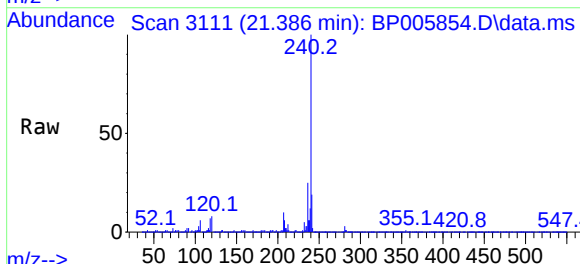


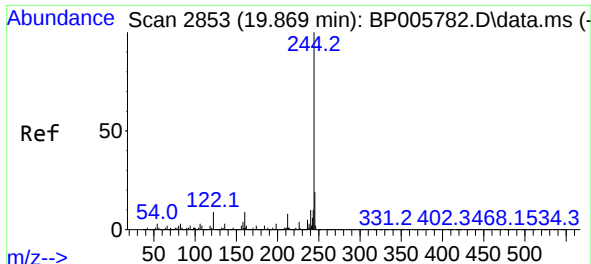

#79
Terphenyl-d14
Concen: 76.491 ng
RT: 19.863 min Scan# 2852
Delta R.T. -0.006 min
Lab File: BP005854.D
Acq: 11 Jun 2021 02:40

Instrument :
BNA_P
ClientSampleId :
18-B12(26-30)

Tgt Ion:244 Resp: 1592023
Ion Ratio Lower Upper
244 100
212 7.9 6.0 9.0
122 8.6 7.1 10.7

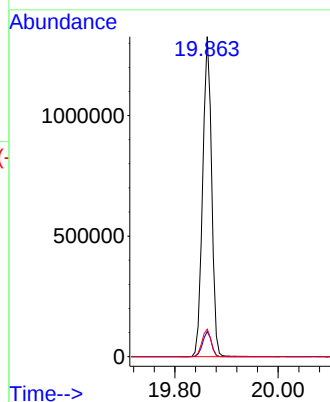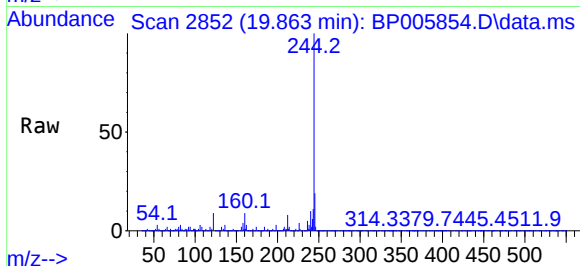

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.804 min Scan# 3522
Delta R.T. -0.012 min
Lab File: BP005854.D
Acq: 11 Jun 2021 02:40

Tgt Ion:264 Resp: 462219
Ion Ratio Lower Upper
264 100
260 23.4 18.6 28.0
265 22.2 17.6 26.4

