


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061021\
 Data File : BP005829.D
 Acq On : 10 Jun 2021 10:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 11 13:53:36 2021

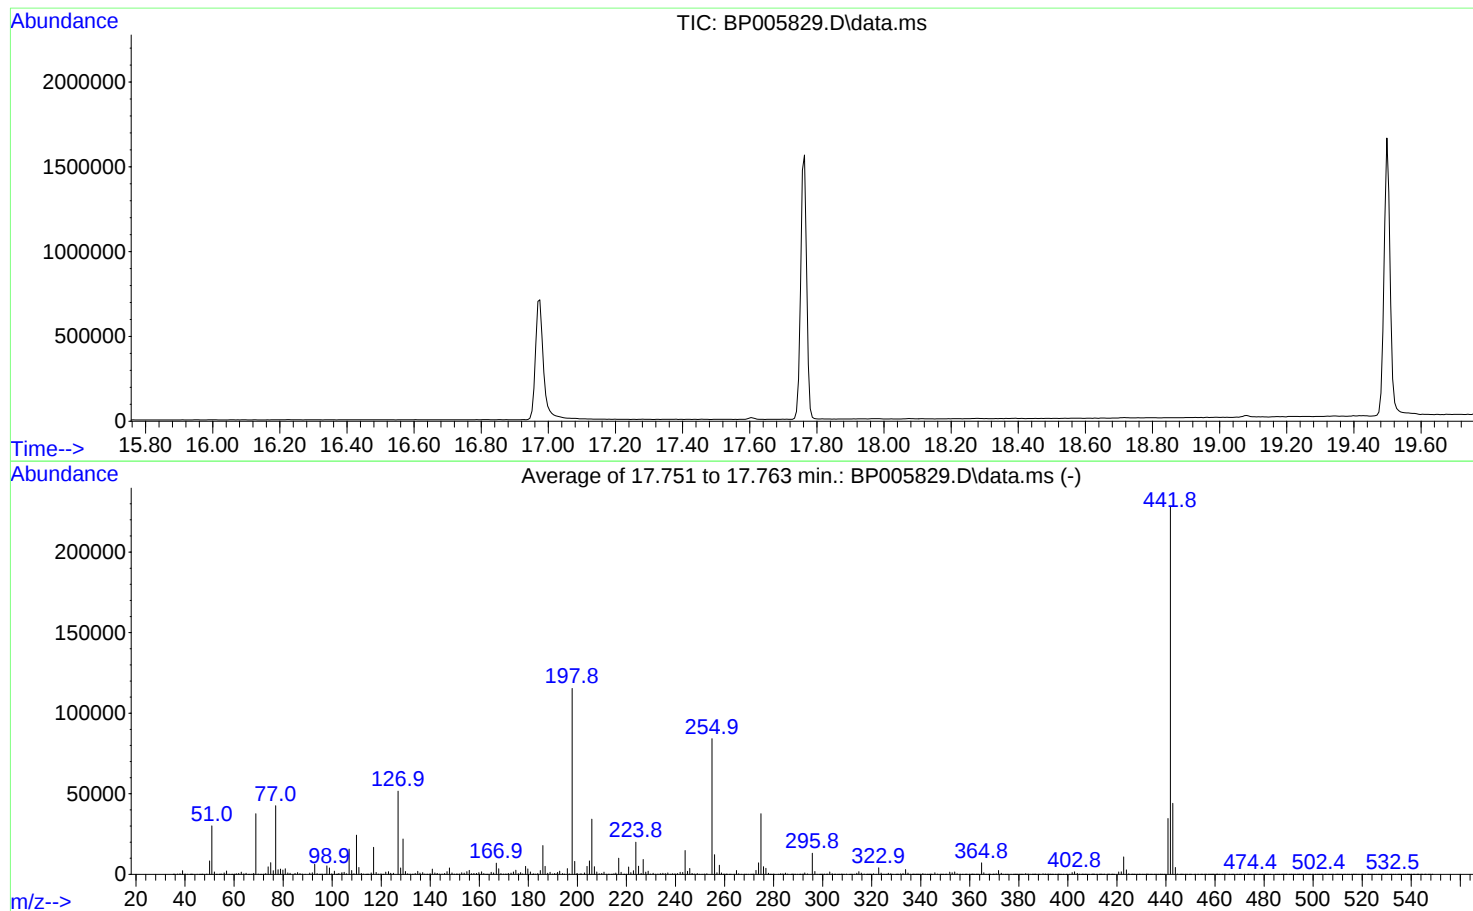




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.0	30056	PASS
68	69	0.00	2	1.5	573	PASS
69	198	0.00	100	32.6	37636	PASS
70	69	0.00	2	0.6	215	PASS
127	198	10	80	44.8	51672	PASS
197	198	0.00	2	0.3	323	PASS
198	198	100	100	100.0	115395	PASS
199	198	5	9	7.0	8027	PASS
275	198	10	60	32.6	37676	PASS
365	198	1	100	6.2	7149	PASS
441	198	0.01	100	30.0	34645	PASS
442	442	100	100	100.0	228291	PASS
443	442	15	24	19.3	44130	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061021\
Data File : BP005829.D
Acq On : 10 Jun 2021 10:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 10 11:49:26 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 09 11:54:55 2021
Response via : Initial Calibration

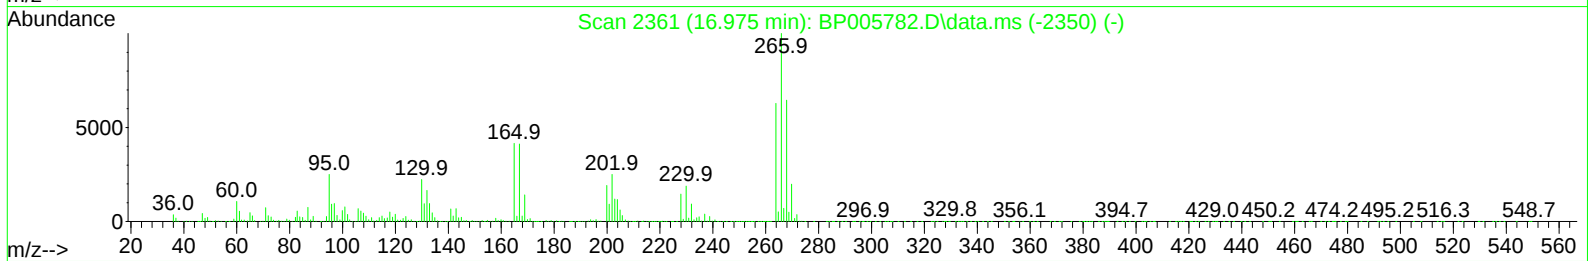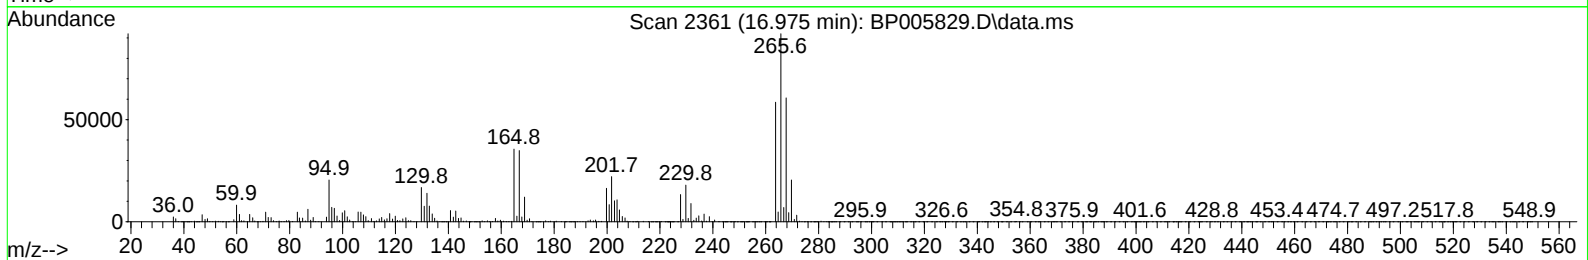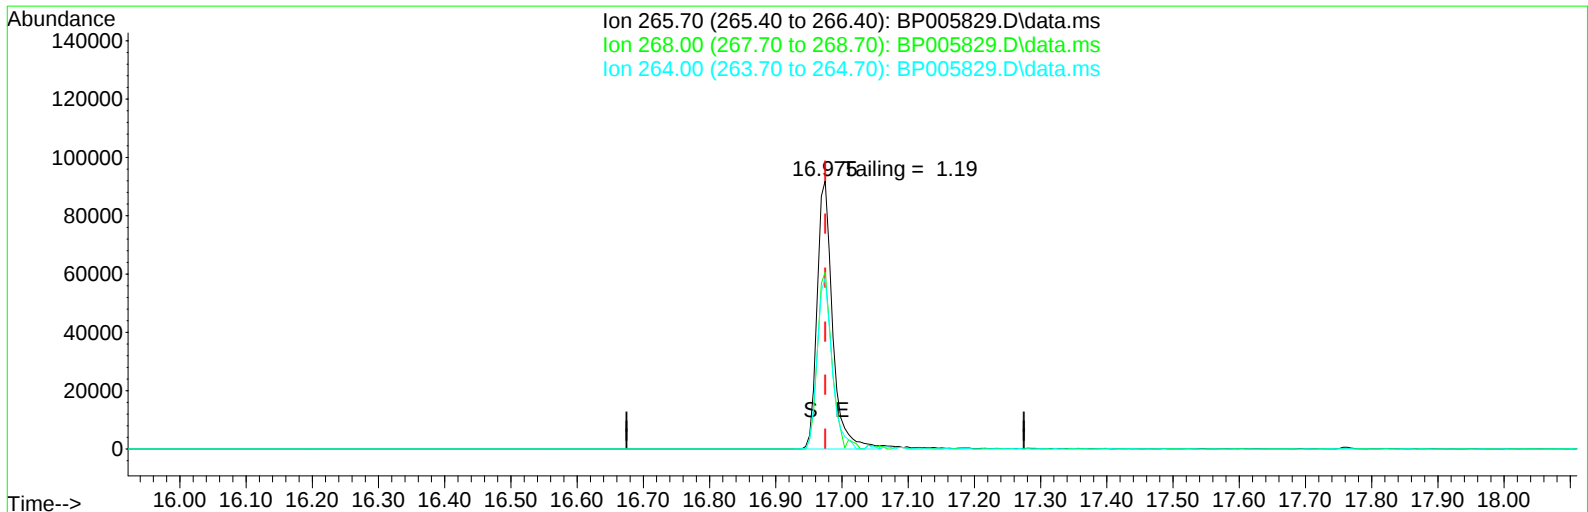

TIC: BP005829.D\data.ms

(70) Pentachlorophenol (C)

16.975min (-0.000) 1614841.51 ng




response 151954

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	70.71
264.00	62.90	68.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061021\
 Data File : BP005829.D
 Acq On : 10 Jun 2021 10:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 10 11:49:26 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 09 11:54:55 2021
 Response via : Initial Calibration

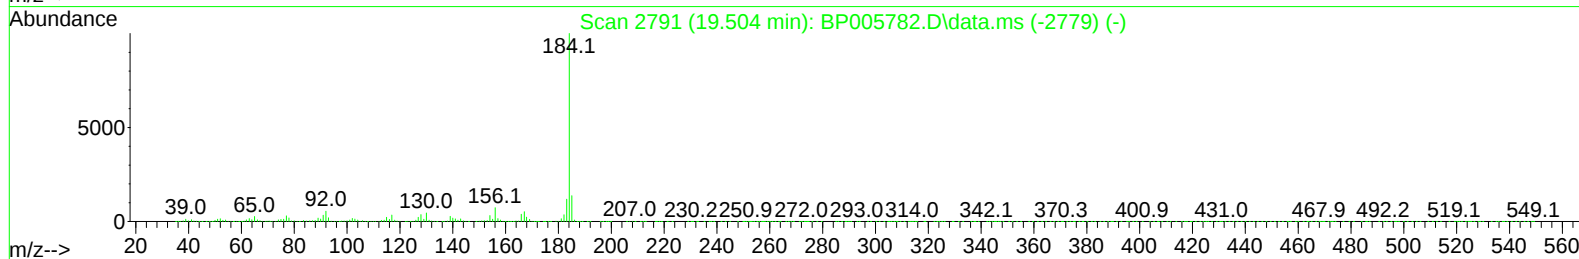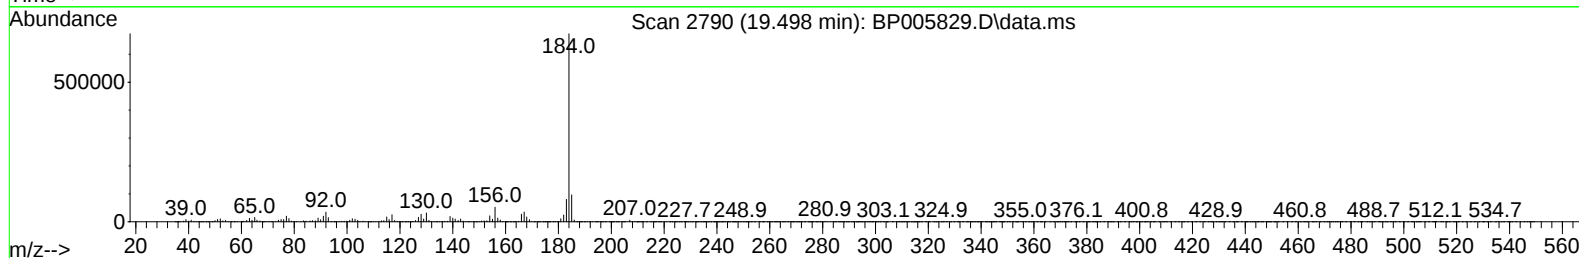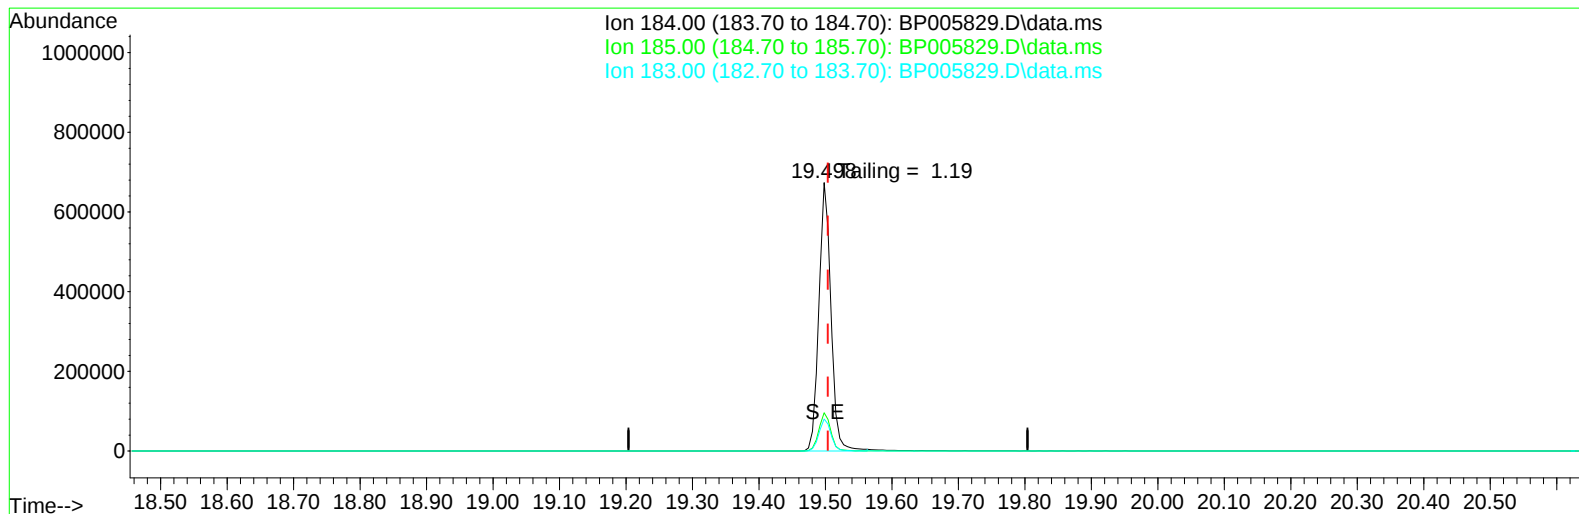

TIC: BP005829.D\data.ms

(77) Benzidine

19.498min (-0.006) 207698.85 ng

response 855716

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.27
183.00	11.90	11.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/10/2021	BNA_P	<u>BP005829.D</u>
Compound Name	Response	Retention Time
DDT	471174	20.69
DDD	2390	20.26
DDE	1166	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3556	474730	0.75

Instrument :
BNA_P
ClientSampleId :
DFTPP