

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061025\
 Data File : BP024892.D
 Acq On : 10 Jun 2025 13:43
 Operator : RC/JU
 Sample : Q2265-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TP11-MHL-WC

Quant Time: Jun 10 14:10:34 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 06 16:20:27 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.608	152	209510	20.000	ng	0.00
21) Naphthalene-d8	10.372	136	824081	20.000	ng	0.00
39) Acenaphthene-d10	14.248	164	530605	20.000	ng	0.00
64) Phenanthrene-d10	17.060	188	1084172	20.000	ng	0.00
76) Chrysene-d12	21.483	240	1201133	20.000	ng	0.00
86) Perylene-d12	24.730	264	1427181	20.000	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.237	112	1197486	95.406	ng	0.00
7) Phenol-d6	6.814	99	1508721	90.849	ng	0.00
23) Nitrobenzene-d5	8.761	82	950157	56.027	ng	0.00
42) 2,4,6-Tribromophenol	15.778	330	742068	101.156	ng	0.00
45) 2-Fluorobiphenyl	12.849	172	2210917	56.132	ng	-0.01
79) Terphenyl-d14	19.783	244	3779952	56.402	ng	-0.01
Target Compounds						
60) Diethylphthalate	15.095	149	118256	3.031	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061025\
Data File : BP024892.D
Acq On : 10 Jun 2025 13:43
Operator : RC/JU
Sample : Q2265-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP11-MHL-WC

Quant Time: Jun 10 14:10:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration




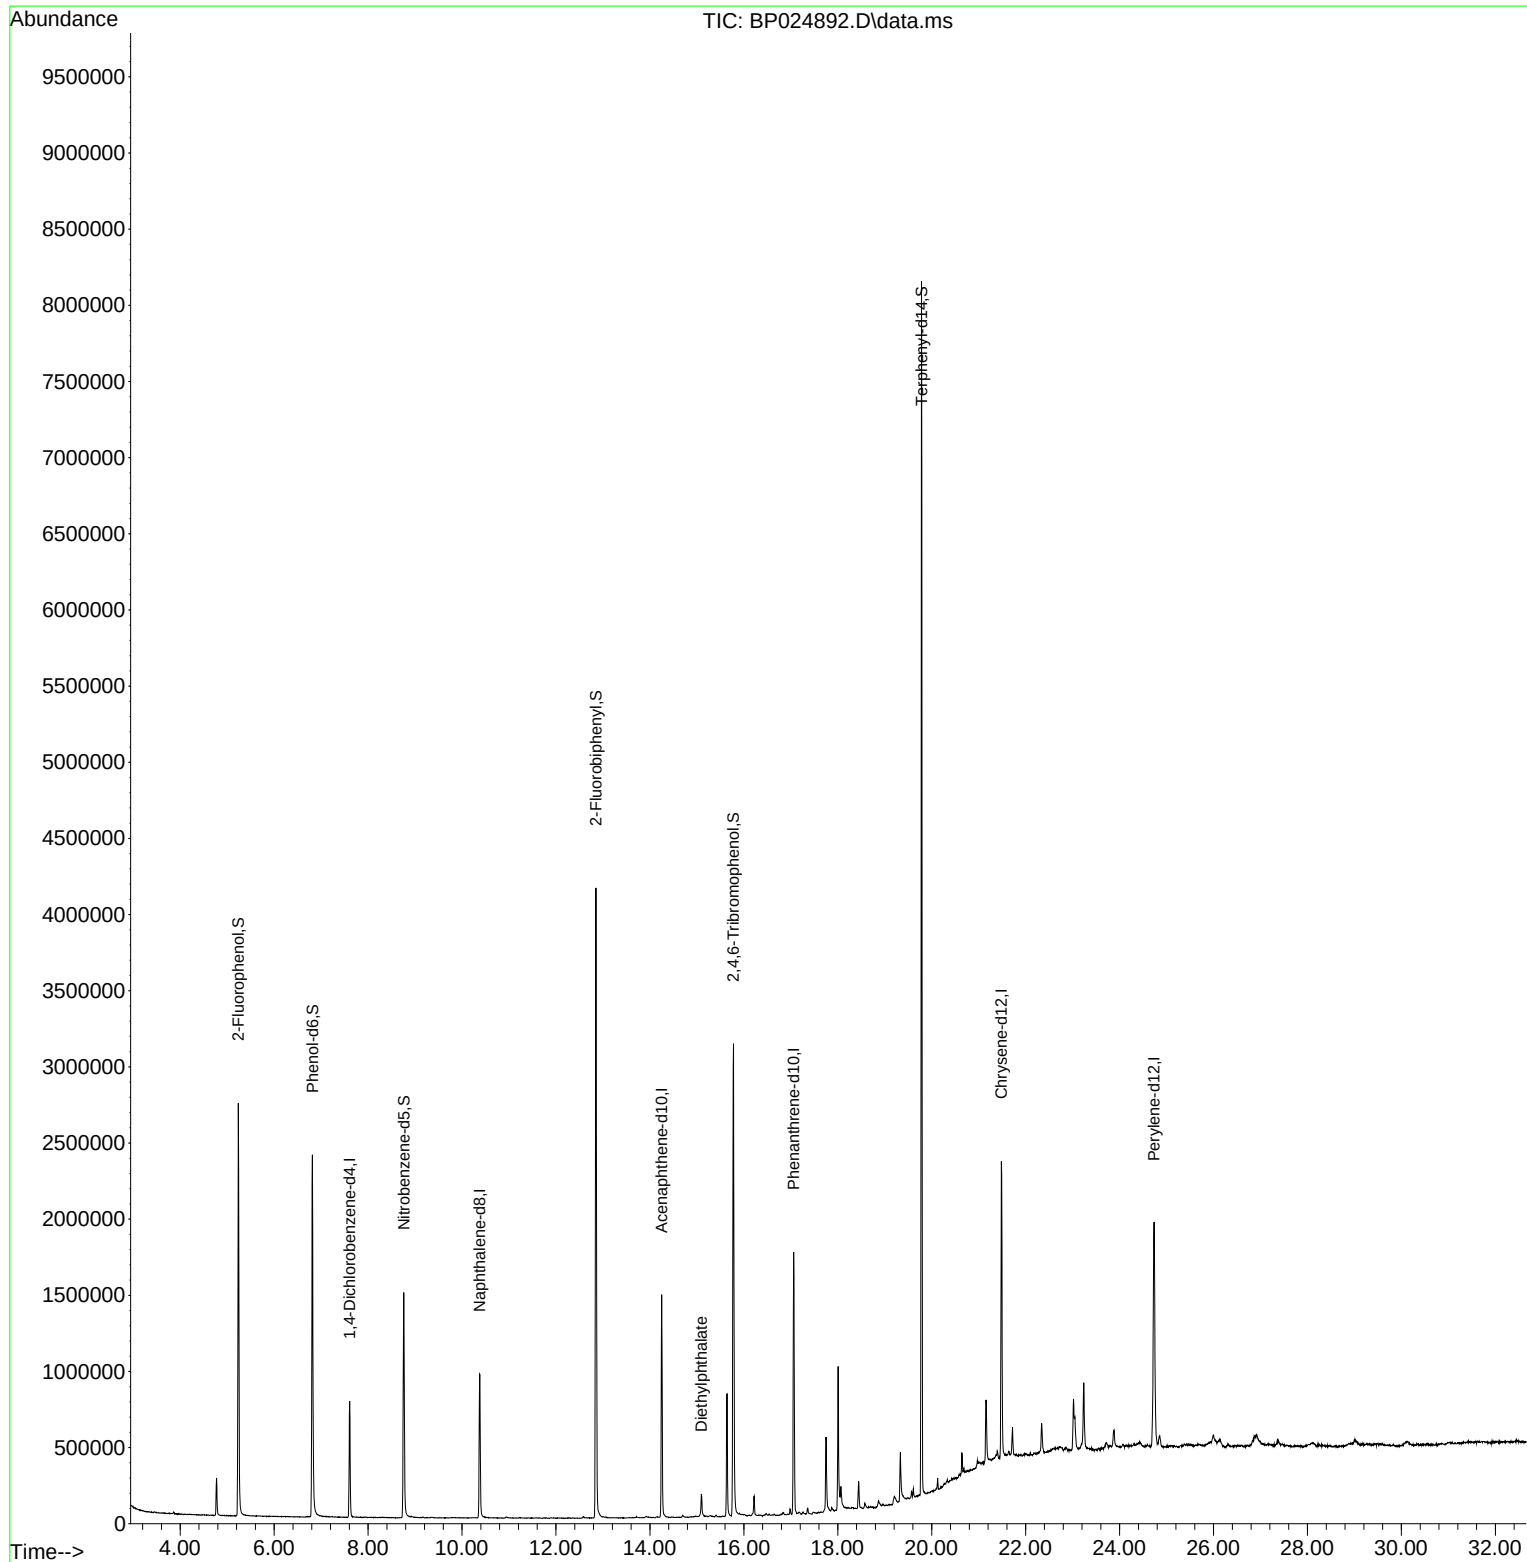


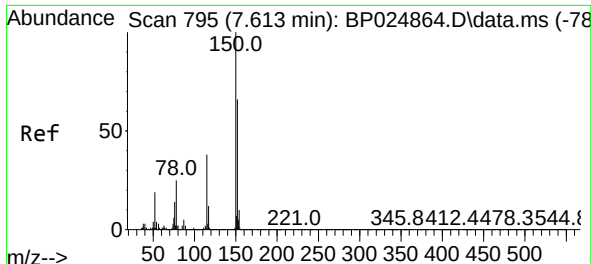

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.608 min Scan# 795
Delta R.T. -0.005 min
Lab File: BP024892.D
Acq: 10 Jun 2025 13:43




Instrument :
BNA_P
ClientSampleId :
TP11-MHL-WC


Tgt Ion:152 Resp: 209510
Ion Ratio Lower Upper
152 100
150 157.6 122.1 183.1
115 61.3 46.4 69.6

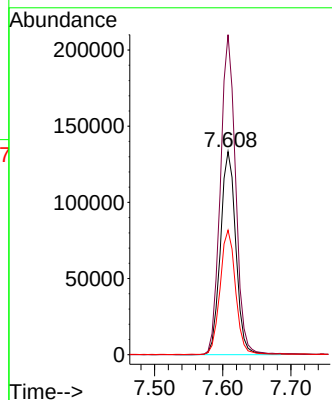

#5
2-Fluorophenol
Concen: 95.406 ng
RT: 5.237 min Scan# 391
Delta R.T. -0.006 min
Lab File: BP024892.D
Acq: 10 Jun 2025 13:43

Tgt Ion:112 Resp: 1197486
Ion Ratio Lower Upper
112 100
64 55.8 44.7 67.1
63 29.1 23.5 35.3


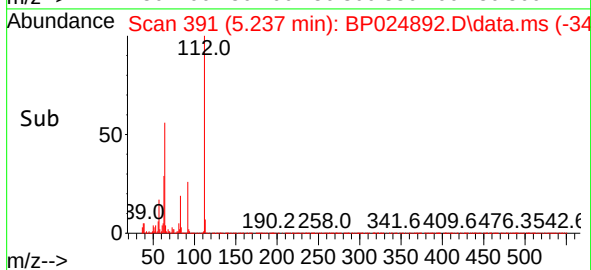
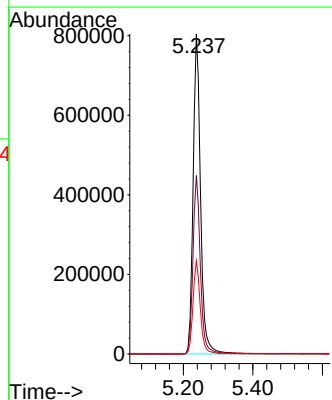
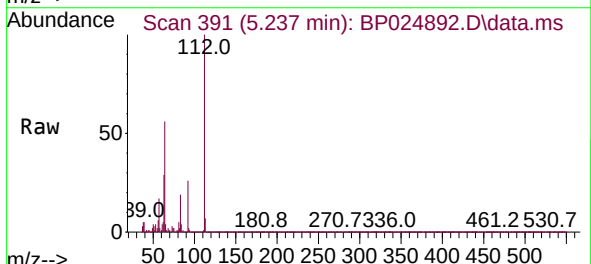




#7
Phenol-d6
Concen: 90.849 ng
RT: 6.814 min Scan# 61
Delta R.T. 0.000 min
Lab File: BP024892.D
Acq: 10 Jun 2025 13:43




Instrument :
BNA_P
ClientSampleId :
TP11-MHL-WC


Tgt Ion: 99 Resp: 1508721
Ion Ratio Lower Upper
99 100
42 16.2 13.4 20.2
71 34.2 27.6 41.4

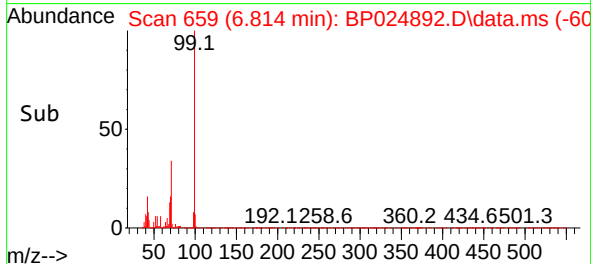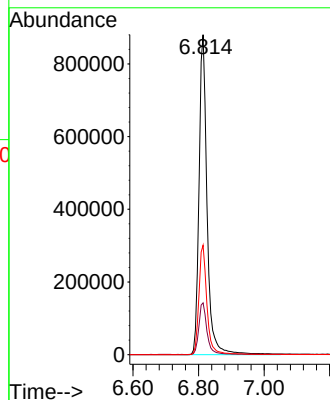

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.372 min Scan# 1264
Delta R.T. -0.006 min
Lab File: BP024892.D
Acq: 10 Jun 2025 13:43

Tgt Ion: 136 Resp: 824081
Ion Ratio Lower Upper
136 100
137 10.9 8.9 13.3
54 7.6 6.1 9.1
68 5.9 4.6 7.0


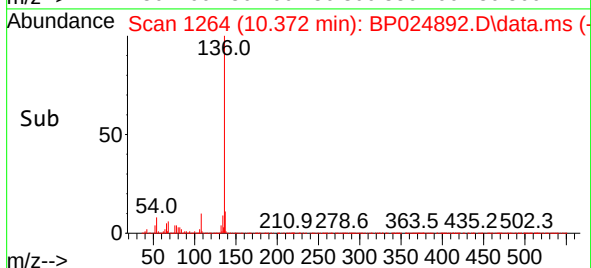
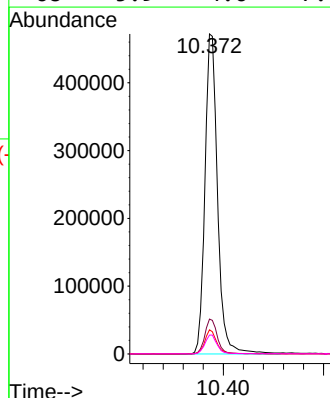
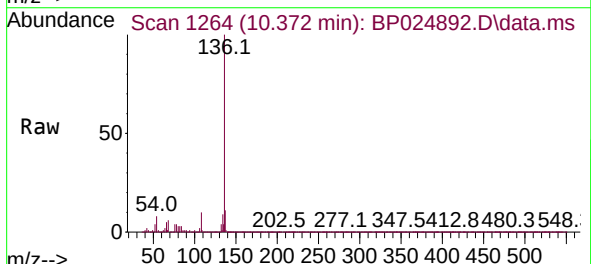




#23
Nitrobenzene-d5
Concen: 56.027 ng
RT: 8.761 min Scan# 990
Delta R.T. 0.000 min
Lab File: BP024892.D
Acq: 10 Jun 2025 13:43




Instrument :
BNA_P
ClientSampleId :
TP11-MHL-WC


Tgt Ion: 82 Resp: 950157
Ion Ratio Lower Upper
82 100
128 45.0 35.3 52.9
54 45.3 37.4 56.0

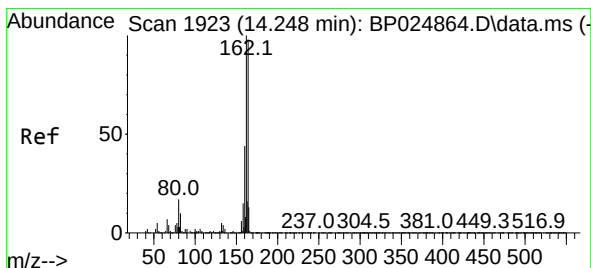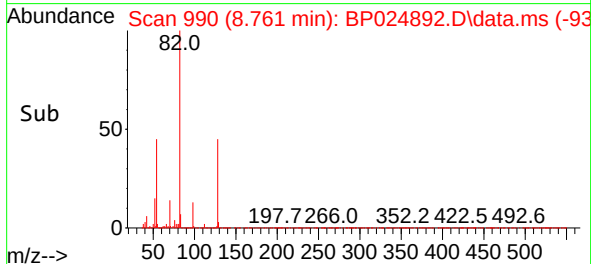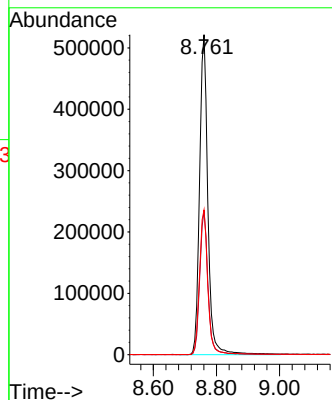

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.248 min Scan# 1923
Delta R.T. 0.000 min
Lab File: BP024892.D
Acq: 10 Jun 2025 13:43

Tgt Ion:164 Resp: 530605
Ion Ratio Lower Upper
164 100
162 101.9 81.6 122.4
160 44.4 36.2 54.2


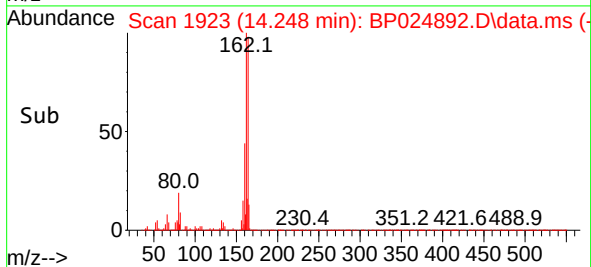
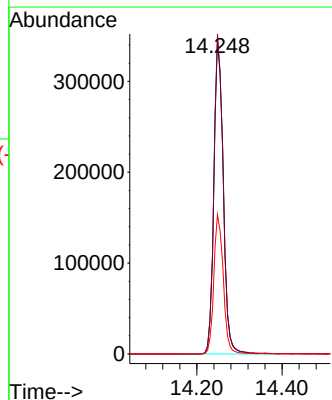
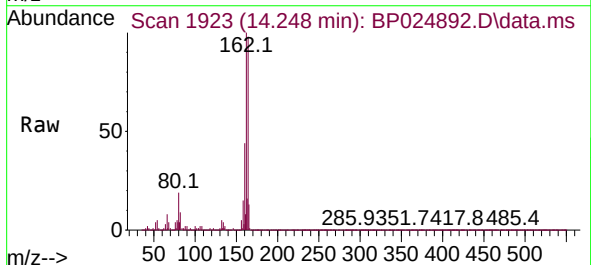




#42
2,4,6-Tribromophenol
Concen: 101.156 ng
RT: 15.778 min Scan# 2184
Delta R.T. -0.006 min
Lab File: BP024892.D
Acq: 10 Jun 2025 13:43




Instrument :
BNA_P
ClientSampleId :
TP11-MHL-WC


Tgt Ion:330 Resp: 742068
Ion Ratio Lower Upper
330 100
332 97.0 77.7 116.5
141 32.1 26.4 39.6

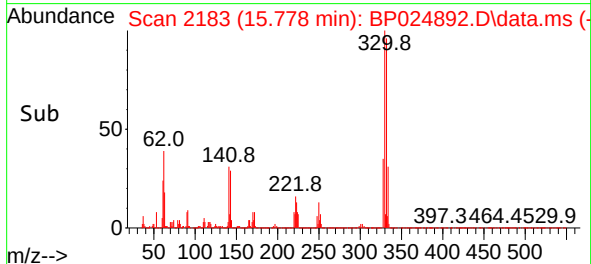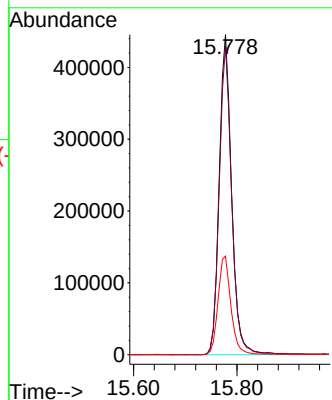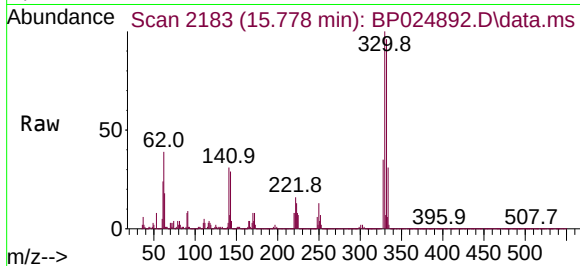

#45
2-Fluorobiphenyl
Concen: 56.132 ng
RT: 12.849 min Scan# 1685
Delta R.T. -0.012 min
Lab File: BP024892.D
Acq: 10 Jun 2025 13:43

Tgt Ion:172 Resp: 2210917
Ion Ratio Lower Upper
172 100
171 35.1 28.3 42.5
170 23.5 19.0 28.4


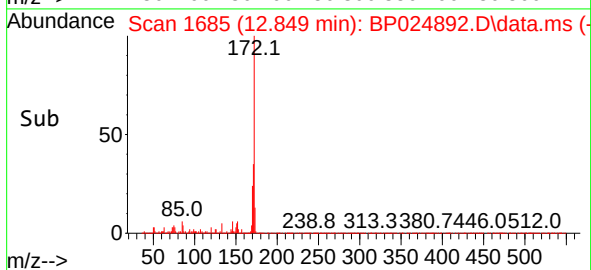
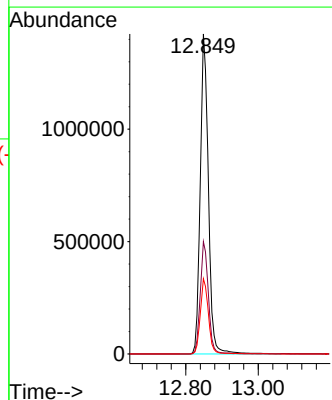
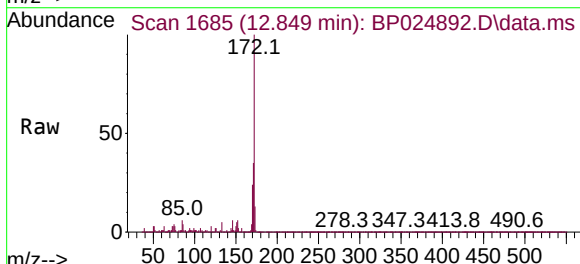




#60
Diethylphthalate
Concen: 3.031 ng
RT: 15.095 min Scan# 2067
Delta R.T. -0.006 min
Lab File: BP024892.D
Acq: 10 Jun 2025 13:43




Instrument :
BNA_P
ClientSampleId :
TP11-MHL-WC


Tgt Ion:149 Resp: 118256
Ion Ratio Lower Upper
149 100
177 22.4 17.9 26.9
150 13.4 9.8 14.6

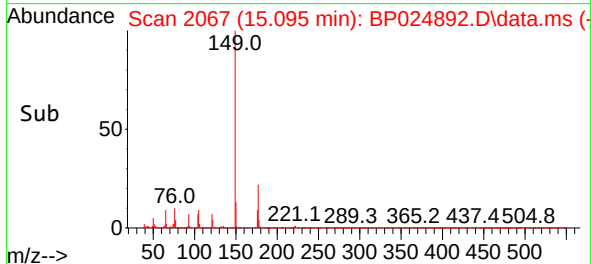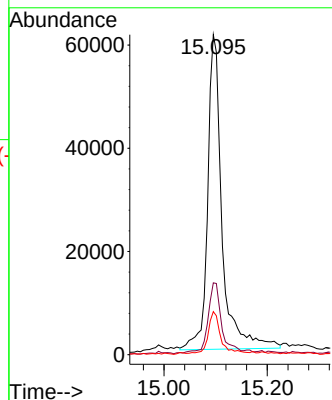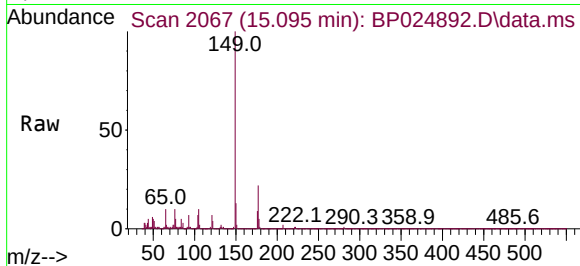

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.060 min Scan# 2401
Delta R.T. 0.000 min
Lab File: BP024892.D
Acq: 10 Jun 2025 13:43

Tgt Ion:188 Resp: 1084172
Ion Ratio Lower Upper
188 100
94 9.3 7.3 10.9
80 10.2 8.5 12.7

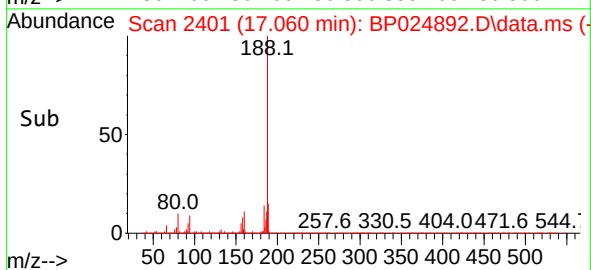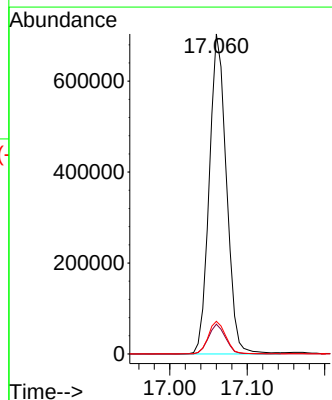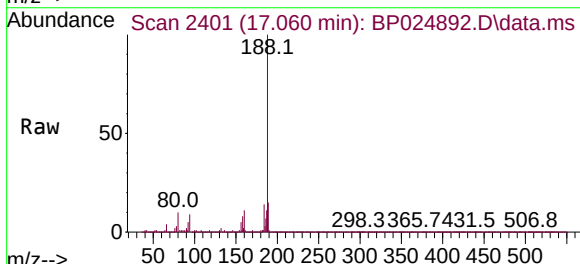

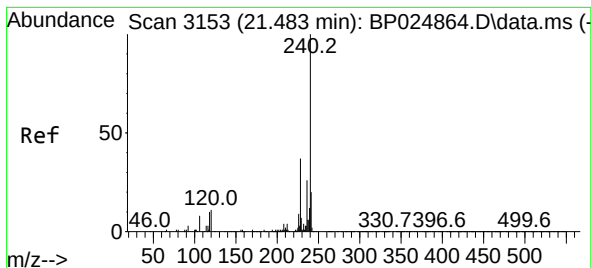

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.483 min Scan# 3153

Delta R.T. 0.000 min

Lab File: BP024892.D

Acq: 10 Jun 2025 13:43

Instrument :

BNA_P

ClientSampleId :

TP11-MHL-WC





Tgt Ion:240 Resp: 1201133

Ion Ratio Lower Upper

240 100

120 10.9 8.9 13.3

236 25.7 20.9 31.3

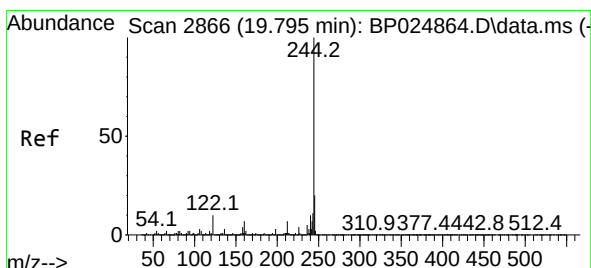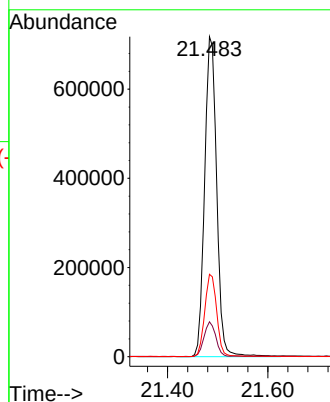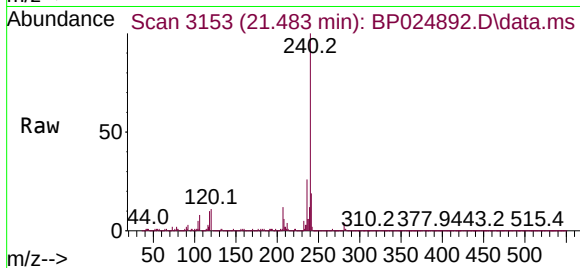

#79

Terphenyl-d14

Concen: 56.402 ng

RT: 19.783 min Scan# 2864

Delta R.T. -0.012 min

Lab File: BP024892.D

Acq: 10 Jun 2025 13:43




Tgt Ion:244 Resp: 3779952


Ion Ratio Lower Upper

244 100

212 7.1 5.6 8.4

122 10.7 7.7 11.5

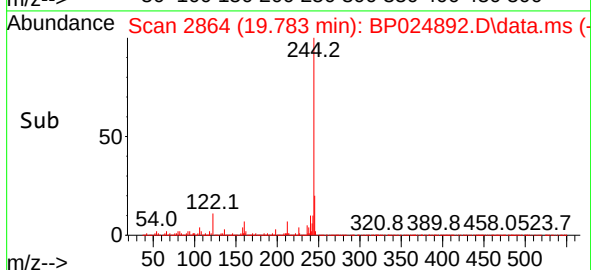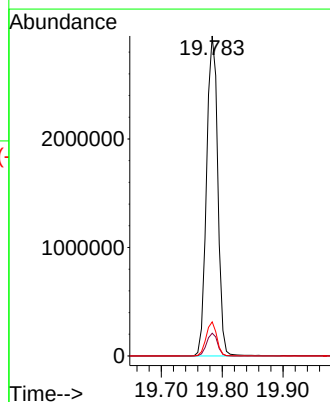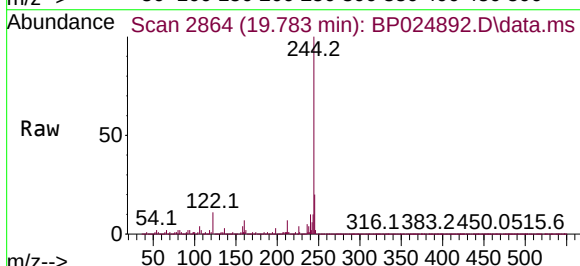

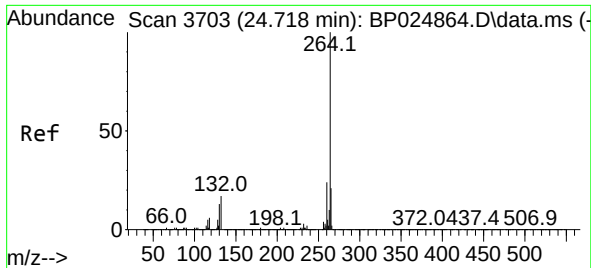

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.730 min Scan# 31
 Delta R.T. 0.012 min
 Lab File: BP024892.D
 Acq: 10 Jun 2025 13:43

Instrument :
 BNA_P
 ClientSampleId :
 TP11-MHL-WC

Tgt Ion:264 Resp: 1427181
 Ion Ratio Lower Upper
 264 100
 260 23.5 19.0 28.4
 265 22.0 17.4 26.0

