
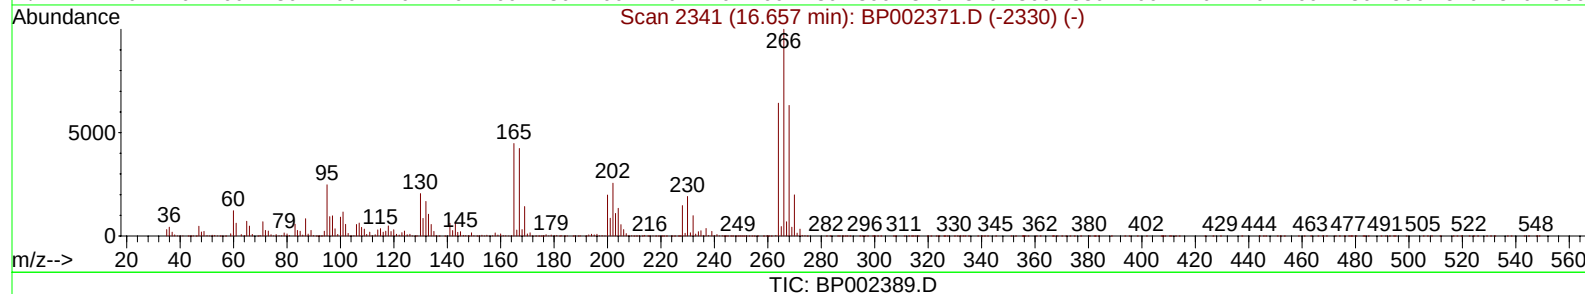
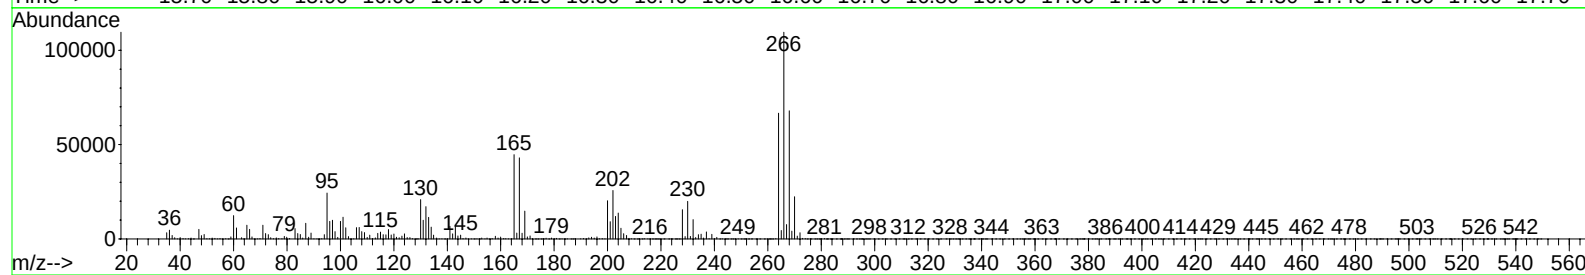


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061120\
Data File : BP002389.D
Acq On : 11 Jun 2020 08:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 17:51:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 15:08:53 2020
Response via : Initial Calibration

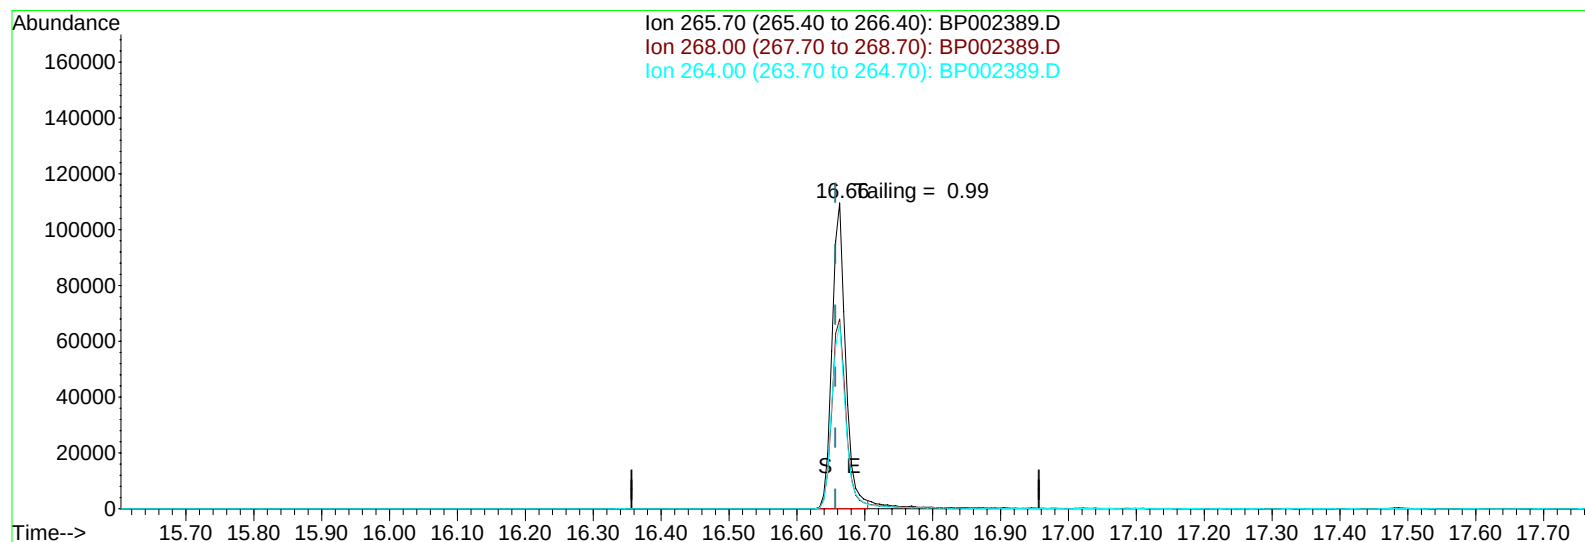

TIC: BP002389.D

(70) Pentachlorophenol (C)




16.663min (+0.006) 29804.64ng

response 155766

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	62.03
264.00	64.20	60.84
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061120\
 Data File : BP002389.D
 Acq On : 11 Jun 2020 08:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 17:51:59 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 15:08:53 2020
 Response via : Initial Calibration

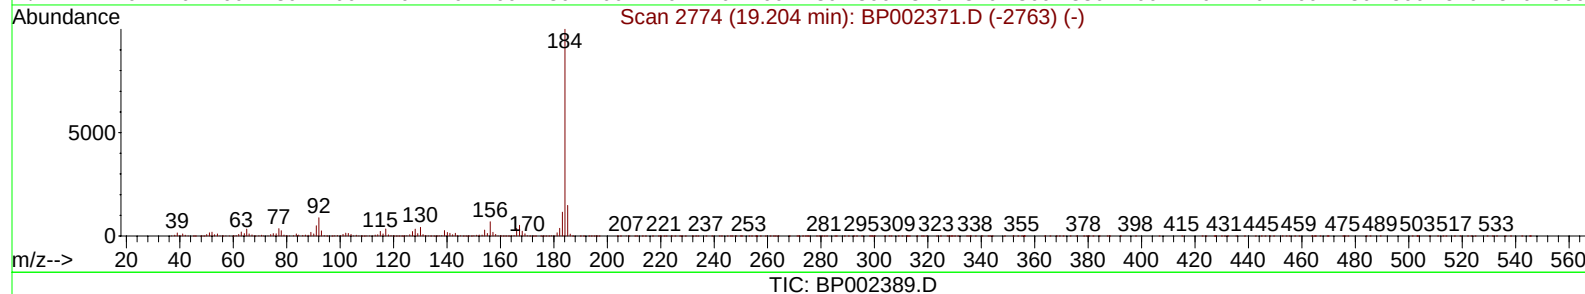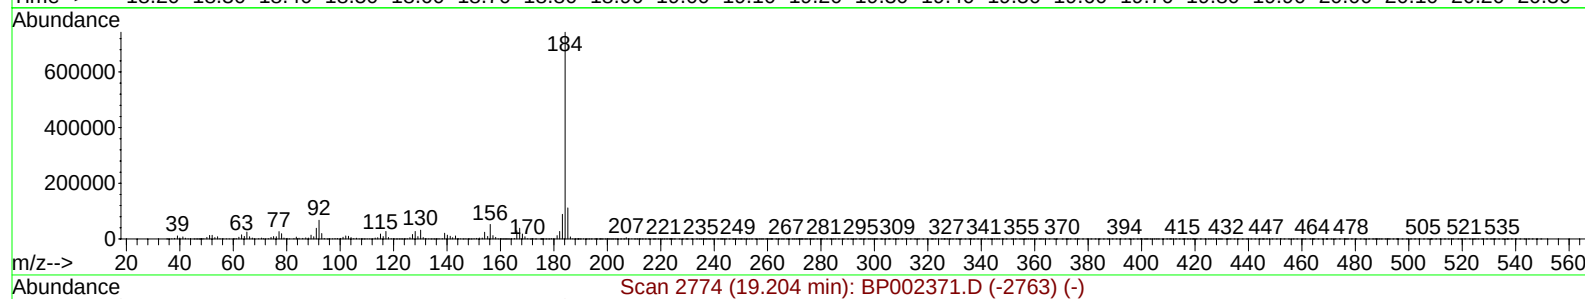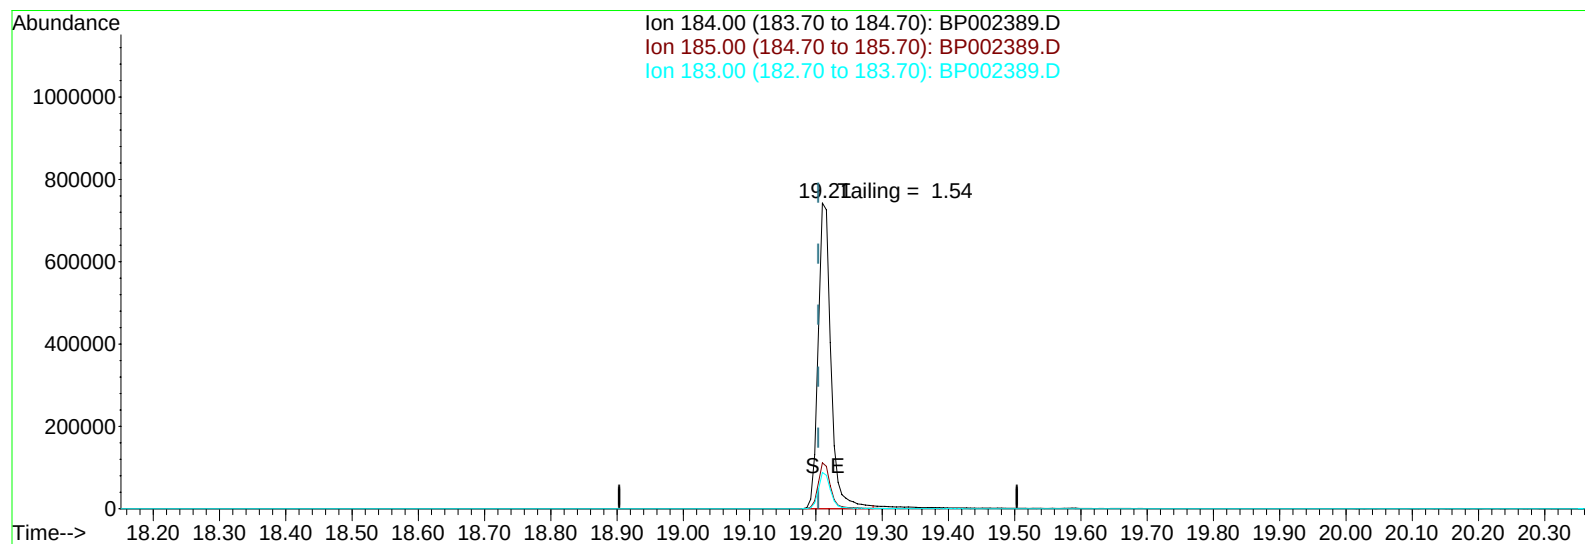

(77) Benzidine

19.210min (+0.006) 7633.85ng

response 1018525

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.99
183.00	11.50	11.89
0.00	0.00	0.00