


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP061120\
 Data File : BP002389.D
 Acq On : 11 Jun 2020 08:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 05 15:08:53 2020

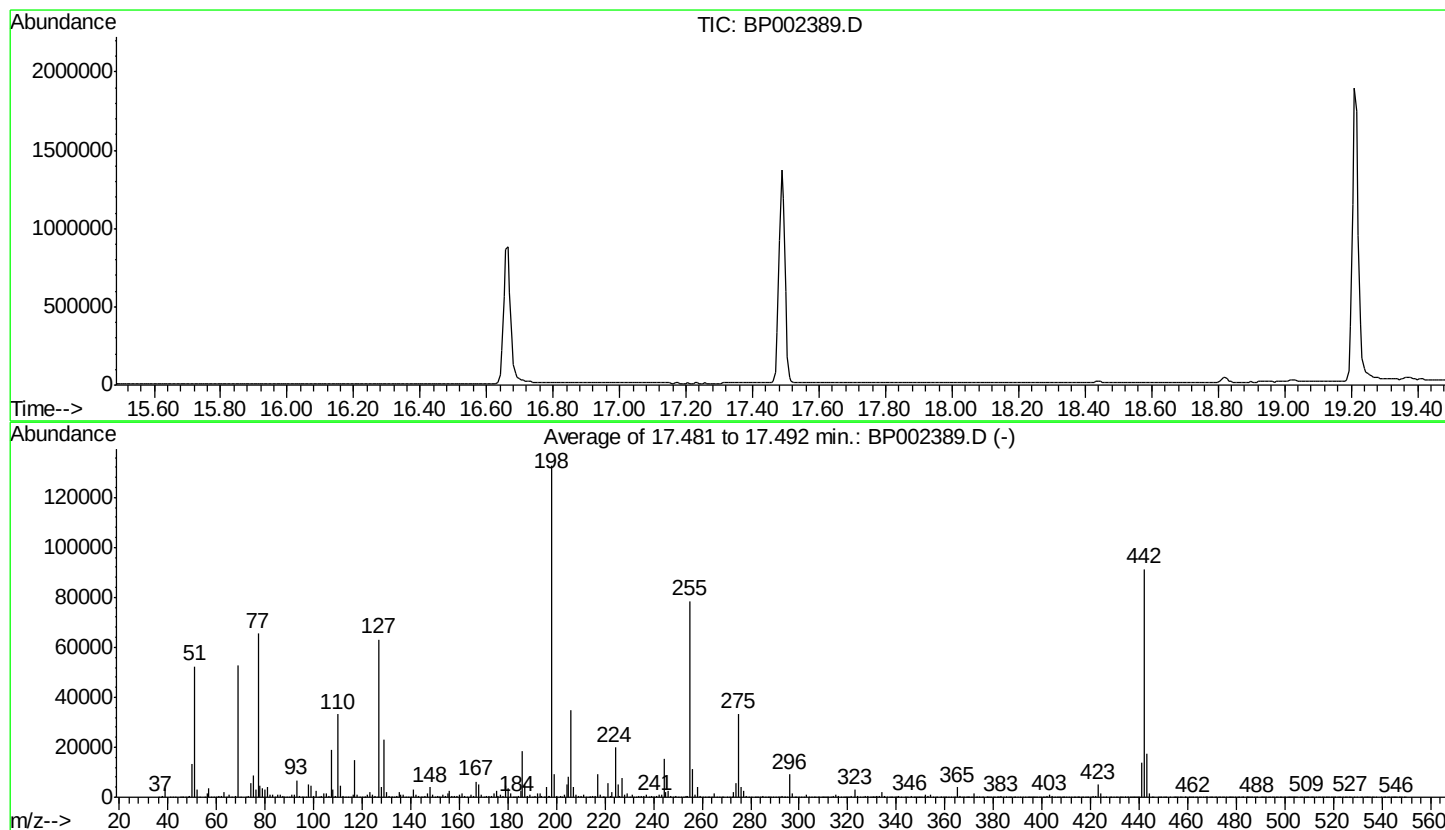

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	52464	PASS
68	69	0.00	2	1.4	763	PASS
69	198	0.00	100	39.8	52823	PASS
70	69	0.00	2	0.5	260	PASS
127	198	10	80	47.6	63212	PASS
197	198	0.00	2	0.3	418	PASS
198	198	100	100	100.0	132688	PASS
199	198	5	9	6.8	9030	PASS
275	198	10	60	25.3	33530	PASS
365	198	1	100	3.0	3950	PASS
441	198	0.01	100	10.3	13703	PASS
442	198	50	100	68.9	91365	PASS
443	442	15	24	19.1	17494	PASS