
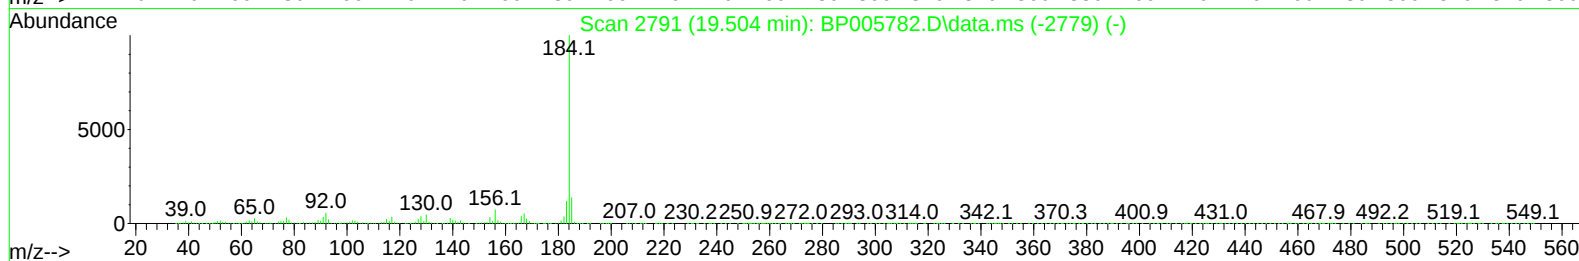
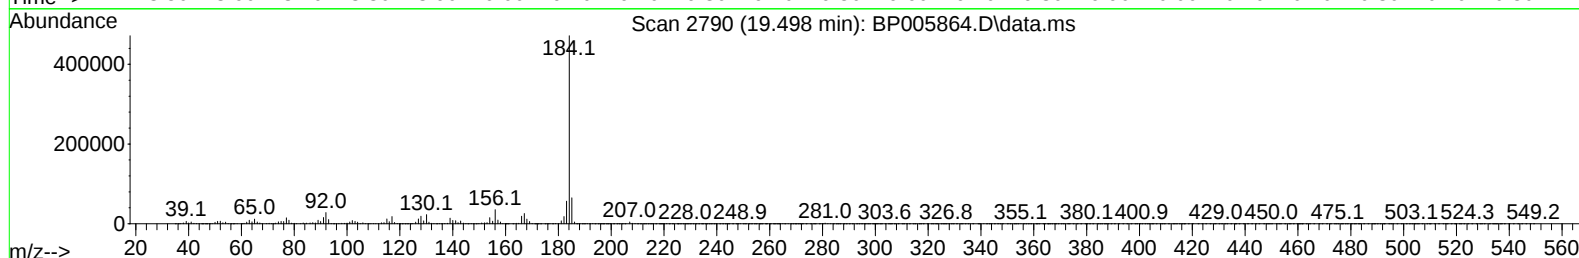


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061121\
 Data File : BP005864.D
 Acq On : 11 Jun 2021 11:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 12:23:43 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 09 11:54:55 2021
 Response via : Initial Calibration

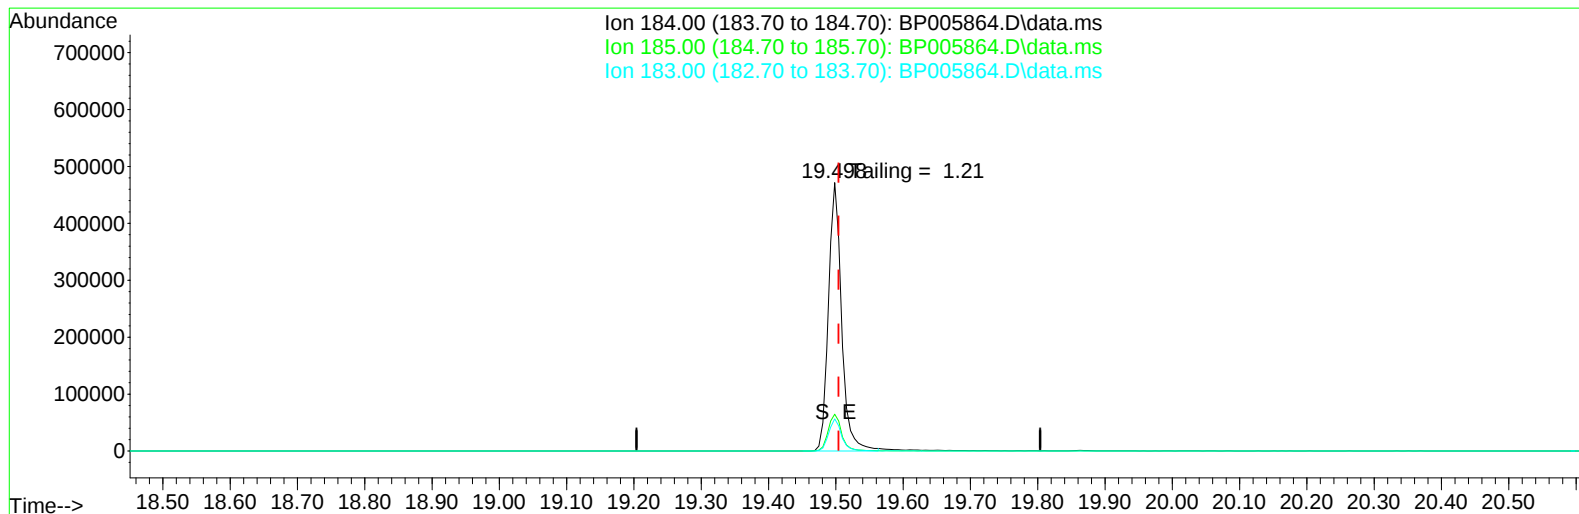




TIC: BP005864.D\data.ms

(77) Benzidine**19.498min (-0.006) 281569.13 ng****response 644478**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.76
183.00	11.90	12.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061121\
Data File : BP005864.D
Acq On : 11 Jun 2021 11:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 12:23:43 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 09 11:54:55 2021
Response via : Initial Calibration

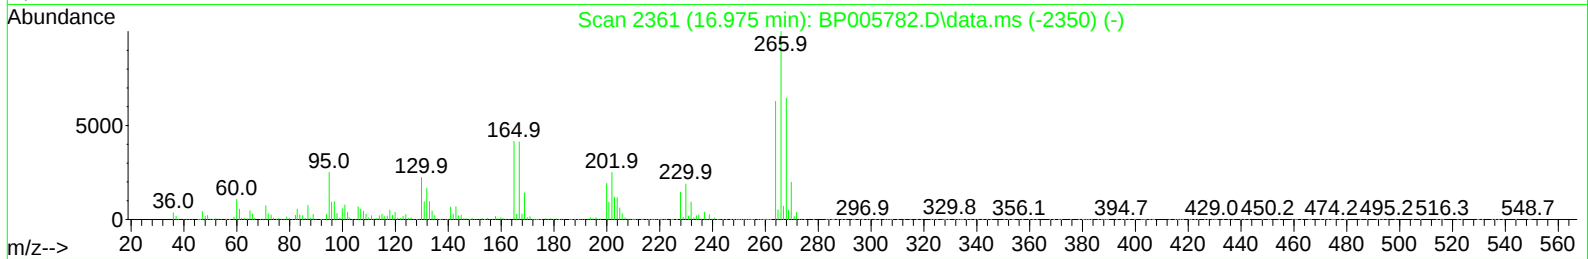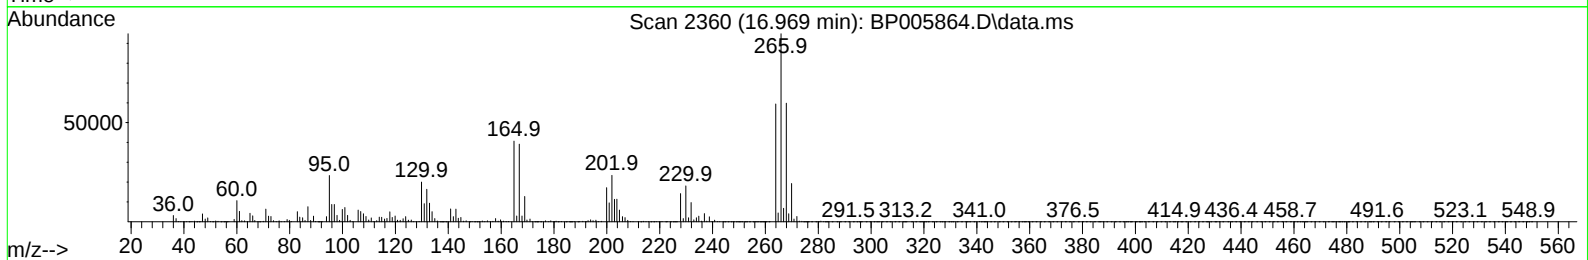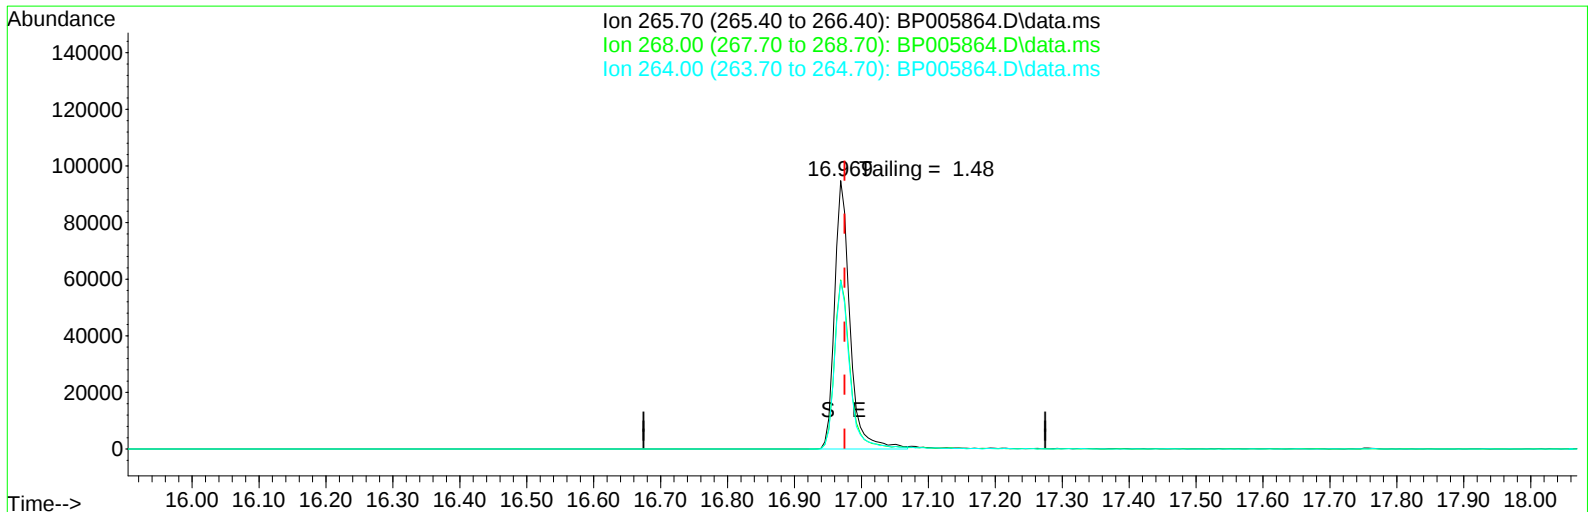

TIC: BP005864.D\data.ms

(70) Pentachlorophenol (C)

16.969min (-0.006) 1111927.80 ng

response 152190

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.03
264.00	62.90	62.66
0.00	0.00	0.00