
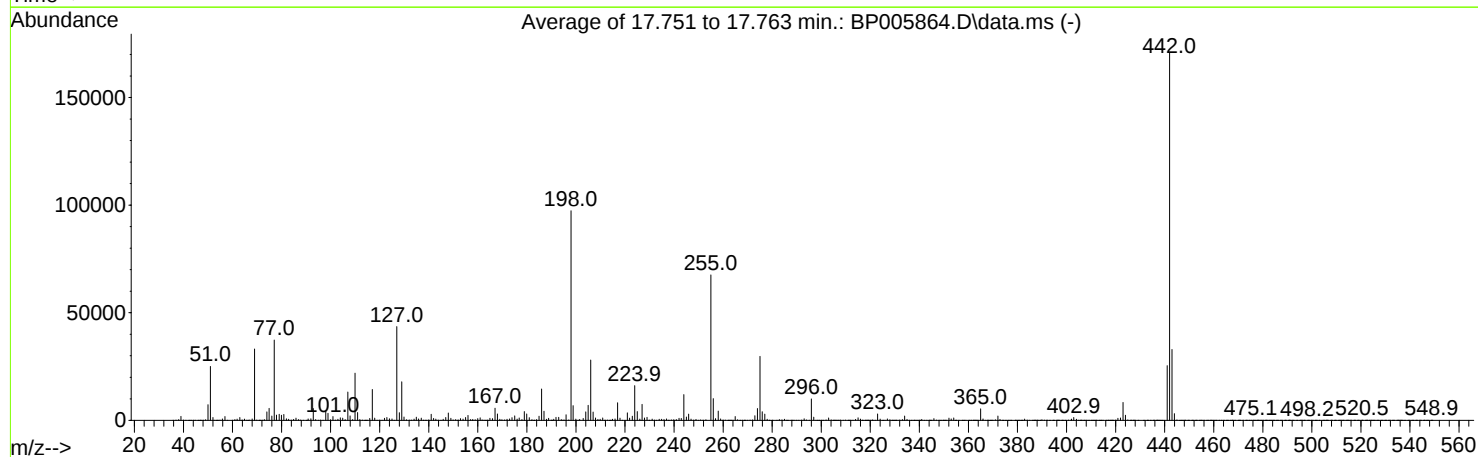


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061121\
 Data File : BP005864.D
 Acq On : 11 Jun 2021 11:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 11 13:53:36 2021

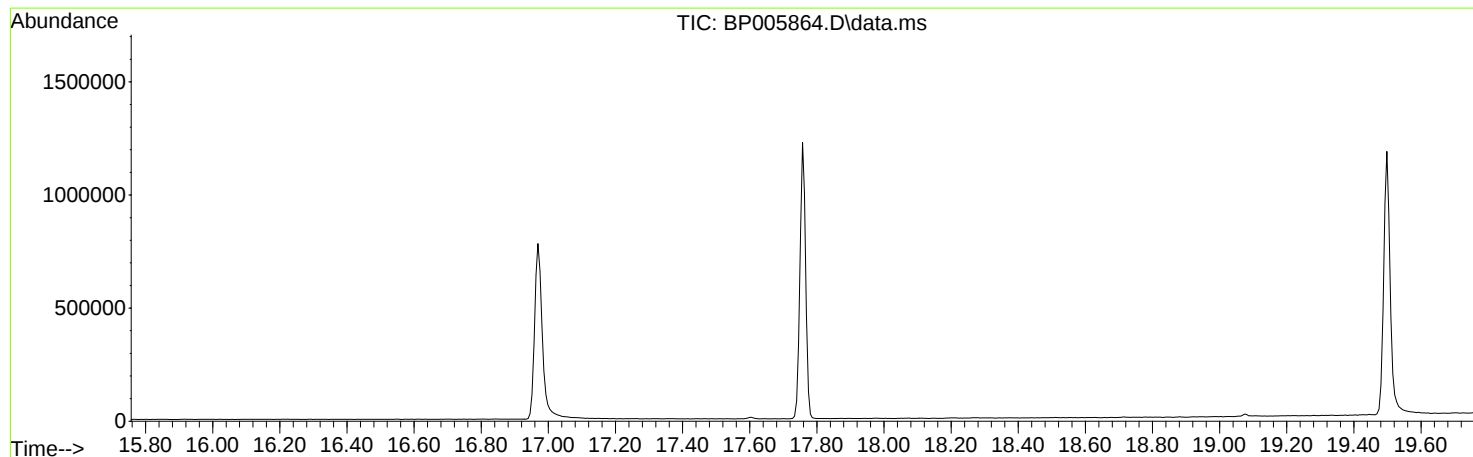

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.7	25073	PASS
68	69	0.00	2	2.0	651	PASS
69	198	0.00	100	34.1	33198	PASS
70	69	0.00	2	0.5	152	PASS
127	198	10	80	44.7	43586	PASS
197	198	0.00	2	0.2	207	PASS
198	198	100	100	100.0	97427	PASS
199	198	5	9	7.0	6835	PASS
275	198	10	60	30.5	29763	PASS
365	198	1	100	5.5	5388	PASS
441	198	0.01	100	26.1	25469	PASS
442	442	100	100	100.0	170923	PASS
443	442	15	24	19.3	32968	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/11/2021	BNA_P	<u>BP005864.D</u>
Compound Name	Response	Retention Time
DDT	374381	20.69
DDD	2835	20.26
DDE	795	19.77
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3630	378011	0.96

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061121\
 Data File : BP005864.D
 Acq On : 11 Jun 2021 11:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 11 12:23:43 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 09 11:54:55 2021
 Response via : Initial Calibration

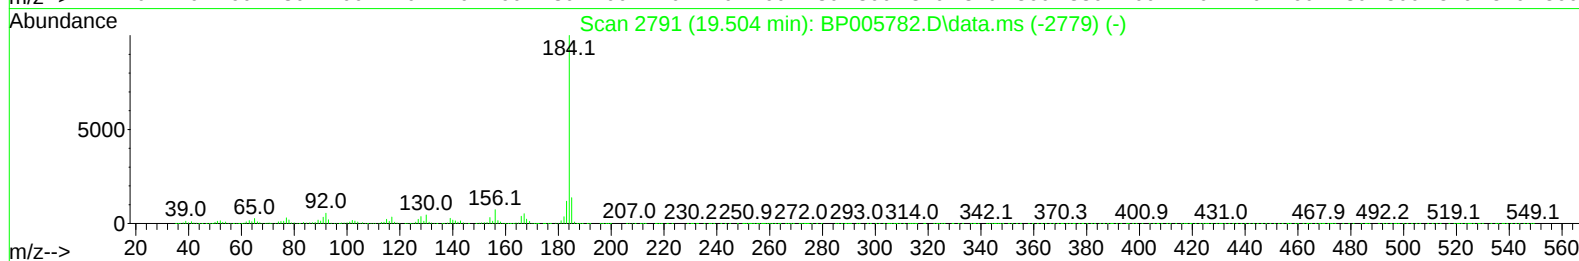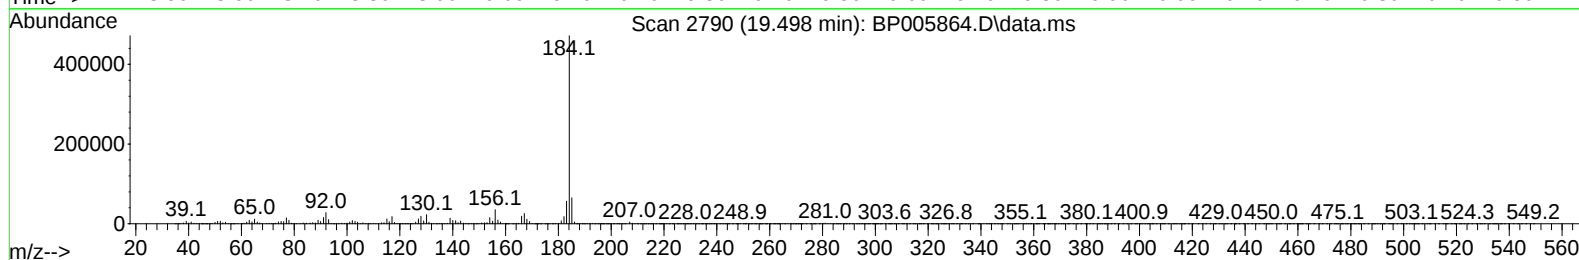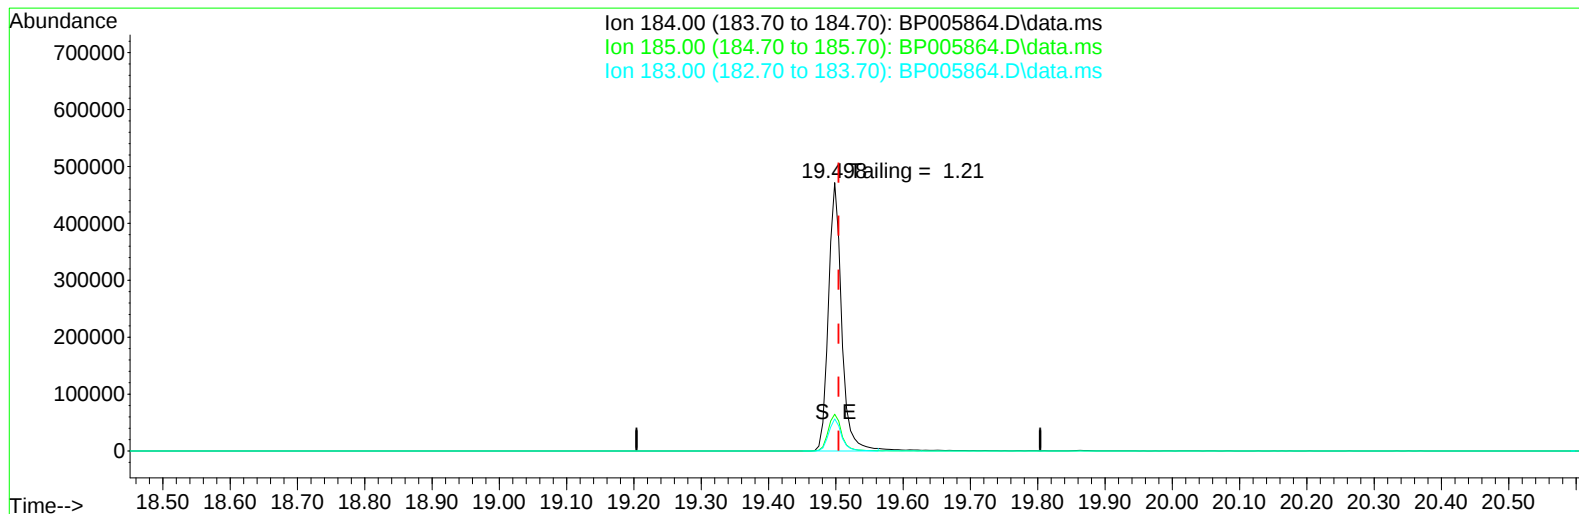

TIC: BP005864.D\data.ms

(77) Benzidine

19.498min (-0.006) 281569.13 ng




response 644478

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.76
183.00	11.90	12.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061121\
 Data File : BP005864.D
 Acq On : 11 Jun 2021 11:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 11 12:23:43 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 09 11:54:55 2021
 Response via : Initial Calibration

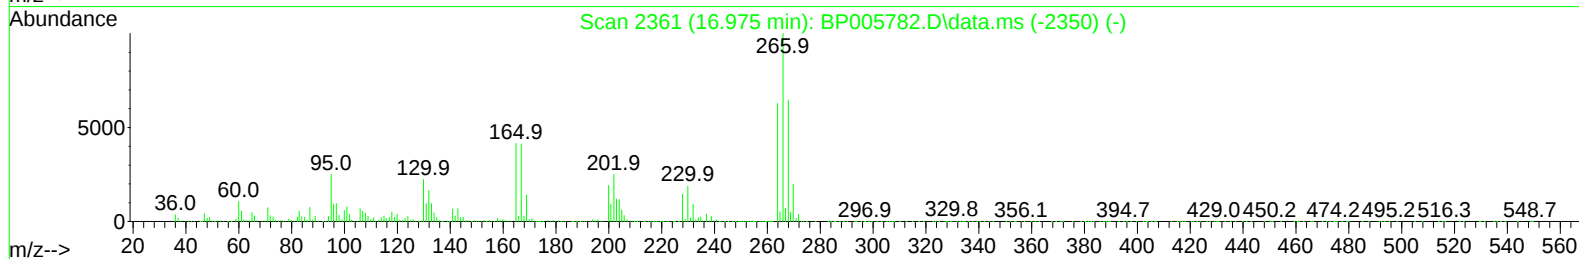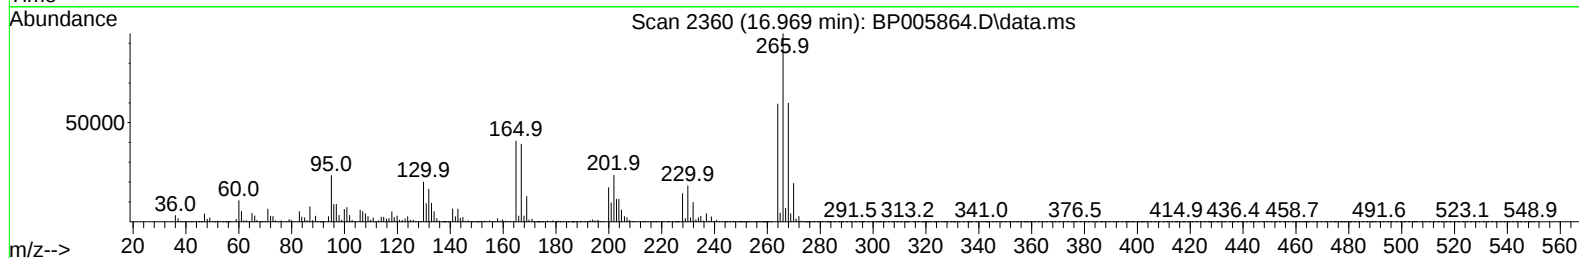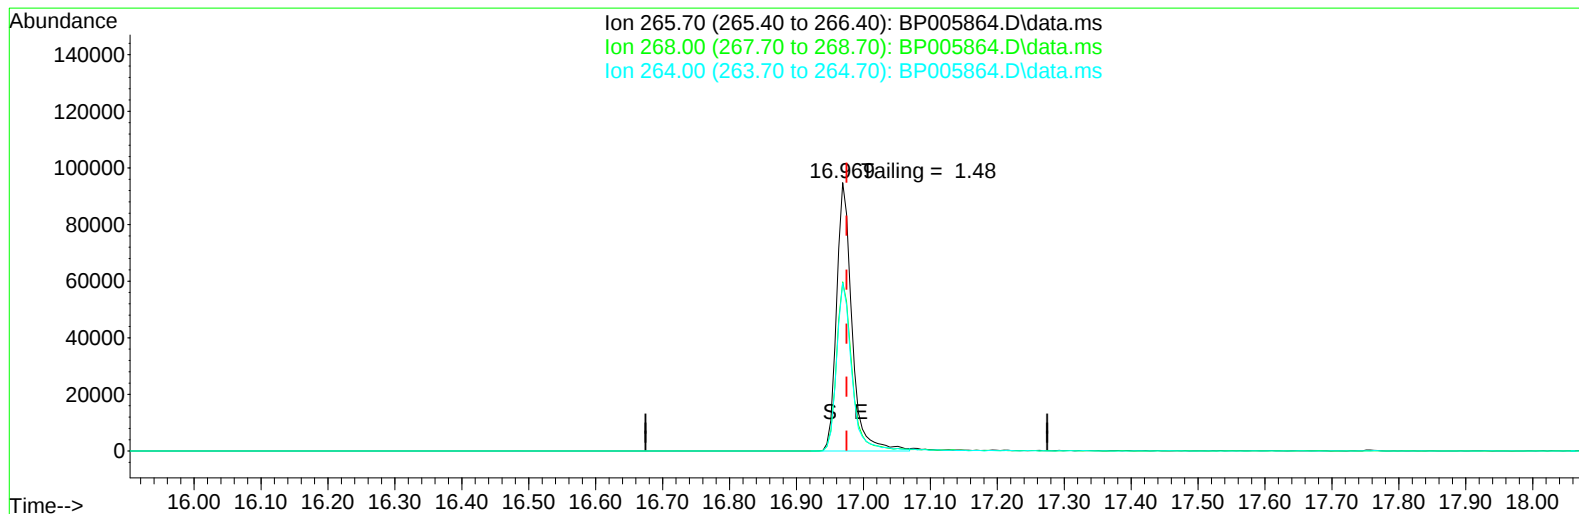

TIC: BP005864.D\data.ms

(70) Pentachlorophenol (C)

16.969min (-0.006) 1111927.80 ng

response 152190

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.03
264.00	62.90	62.66
0.00	0.00	0.00