
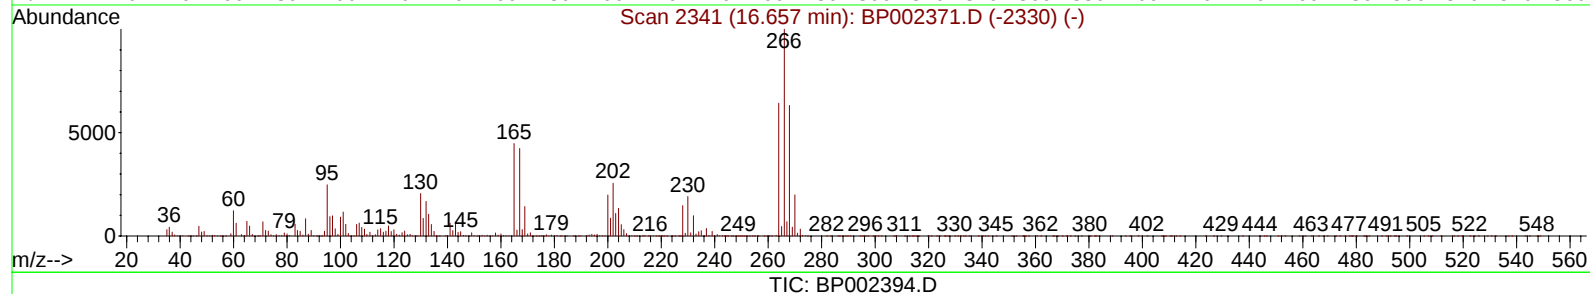
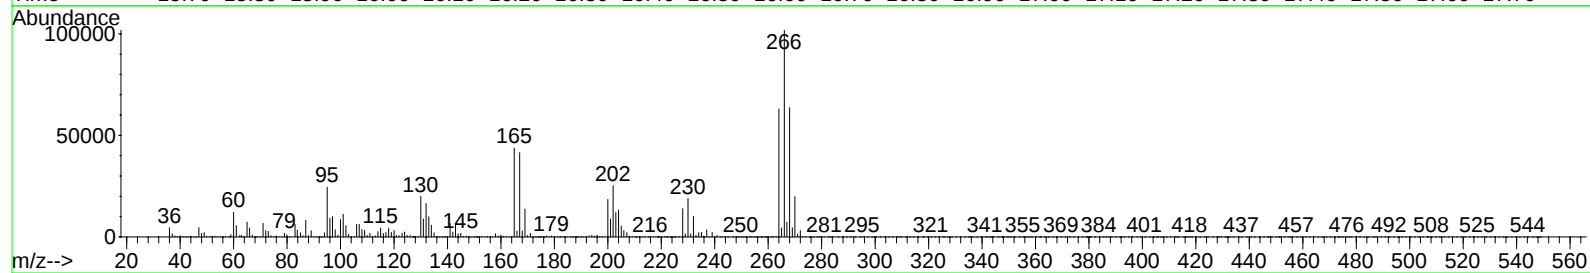


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061220\
Data File : BP002394.D
Acq On : 12 Jun 2020 08:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 12 19:10:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 15:08:53 2020
Response via : Initial Calibration

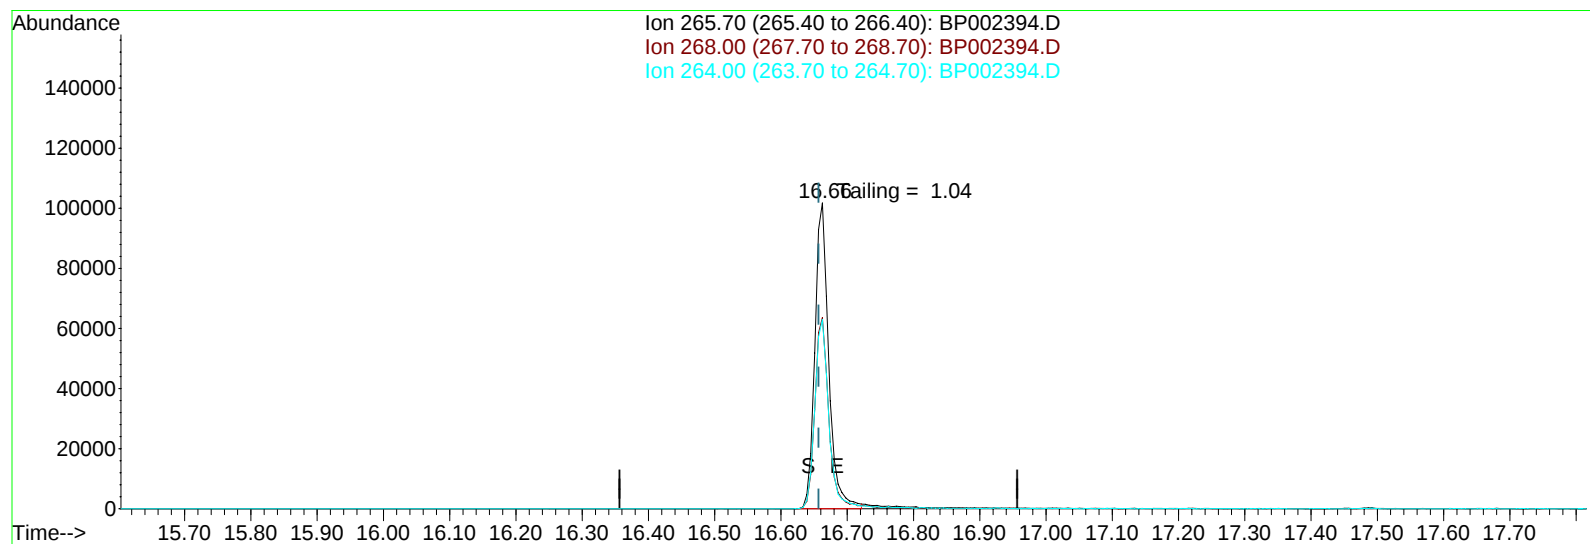

TIC: BP002394.D

(70) Pentachlorophenol (C)




16.663min (+0.006) 163301.80ng

response 152227

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	62.55
264.00	64.20	61.92
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061220\
 Data File : BP002394.D
 Acq On : 12 Jun 2020 08:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 12 19:10:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 15:08:53 2020
 Response via : Initial Calibration

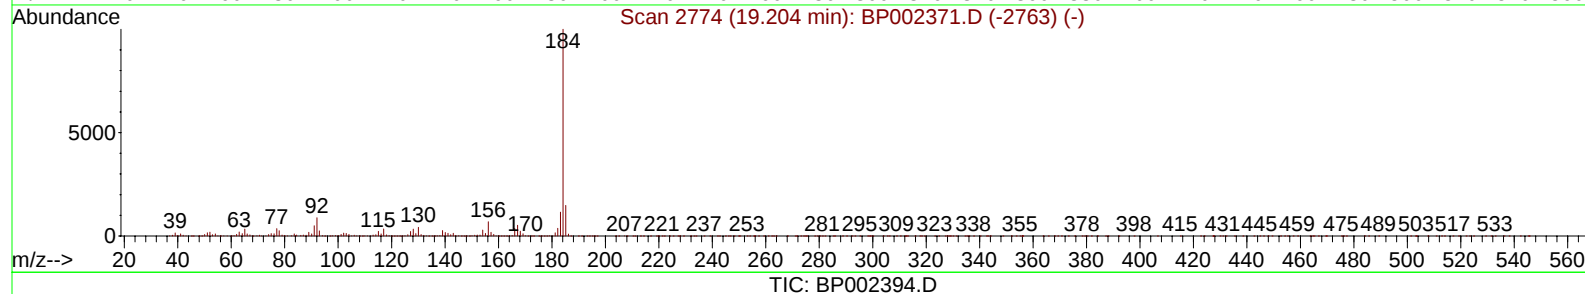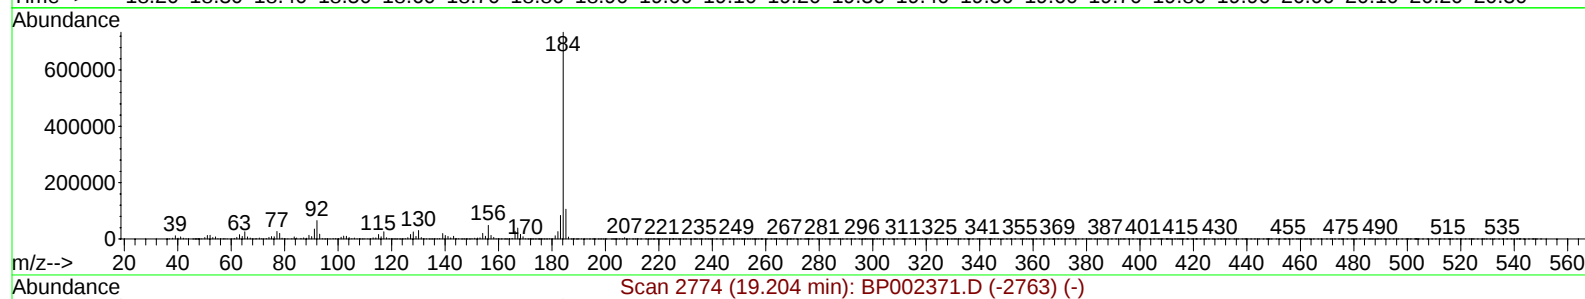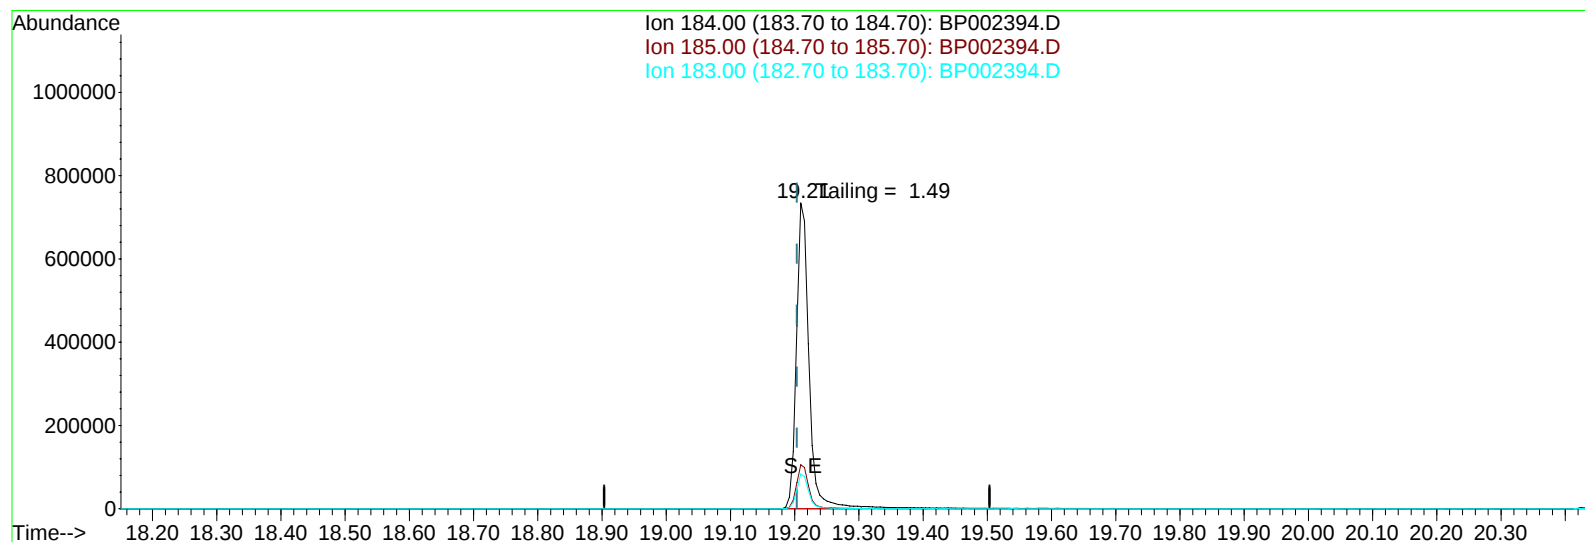

(77) Benzidine

19.209min (+0.006) 3061.32ng

response 1009867

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.39
183.00	11.50	11.38
0.00	0.00	0.00