

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP061220\
 Data File : BP002396.D
 Acq On : 12 Jun 2020 10:04
 Operator : CG/JU
 Sample : PB129455BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB129455BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.205	388	394	413	rBV	2794650	4303189	42.95%	8.603%
2	6.775	654	661	690	rBV	2719638	4552248	45.44%	9.101%
3	7.587	792	799	812	rBV	609363	986580	9.85%	1.972%
4	7.910	846	854	865	rBV	2390607	3929600	39.22%	7.856%
5	8.734	986	994	1009	rBV	1948177	3214905	32.09%	6.427%
6	10.363	1263	1271	1288	rBV	784625	1373265	13.71%	2.746%
7	12.857	1687	1695	1716	rBV	4291886	6985353	69.73%	13.966%
8	14.239	1919	1930	1943	rBV	1206100	1876226	18.73%	3.751%
9	15.734	2177	2184	2204	rBV	3416824	5199103	51.90%	10.394%
10	16.992	2391	2398	2412	rBV	1540571	2270003	22.66%	4.538%
11	19.586	2833	2839	2855	rBV	7410091	10018186	100.00%	20.029%
12	21.098	3091	3096	3106	rBV	2051953	2588474	25.84%	5.175%
13	23.298	3463	3470	3483	rVB	1422748	2720968	27.16%	5.440%




Sum of corrected areas: 50018100

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061220\
Data File : BP002396.D
Acq On : 12 Jun 2020 10:04
Operator : CG/JU
Sample : PB129455BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129455BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

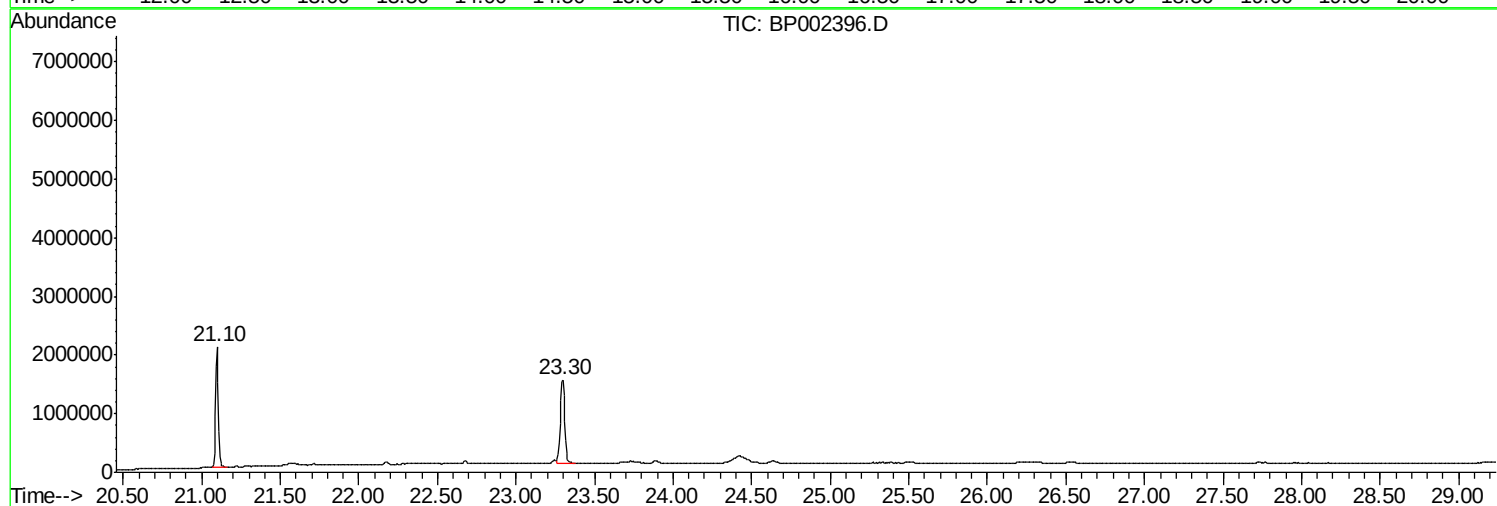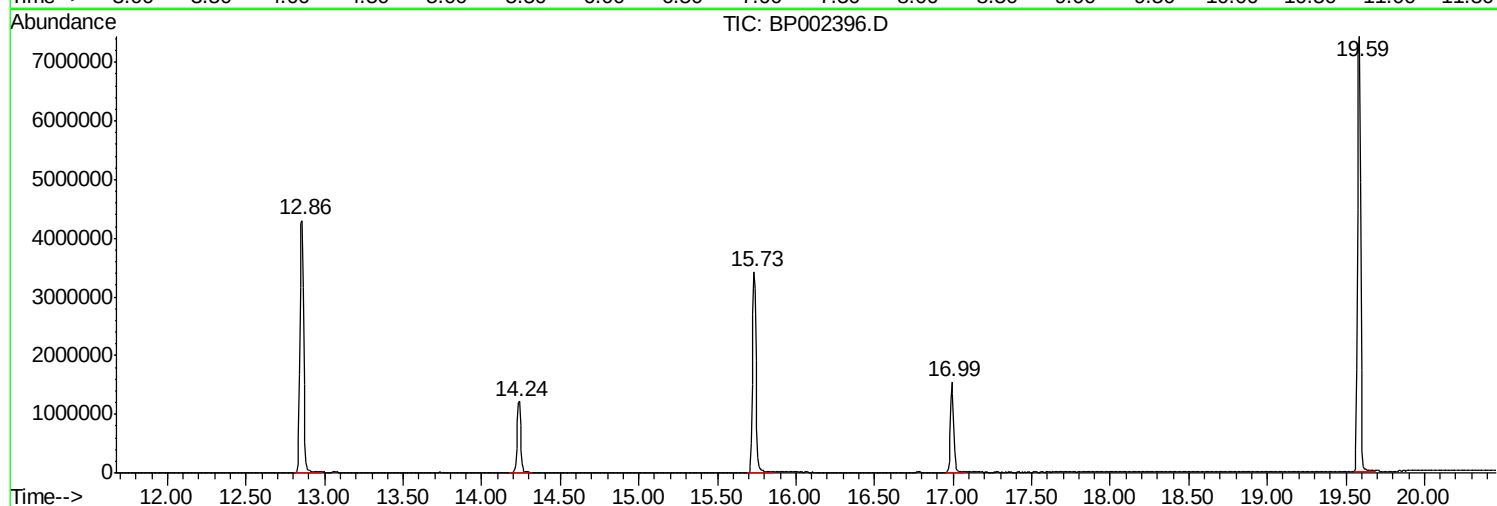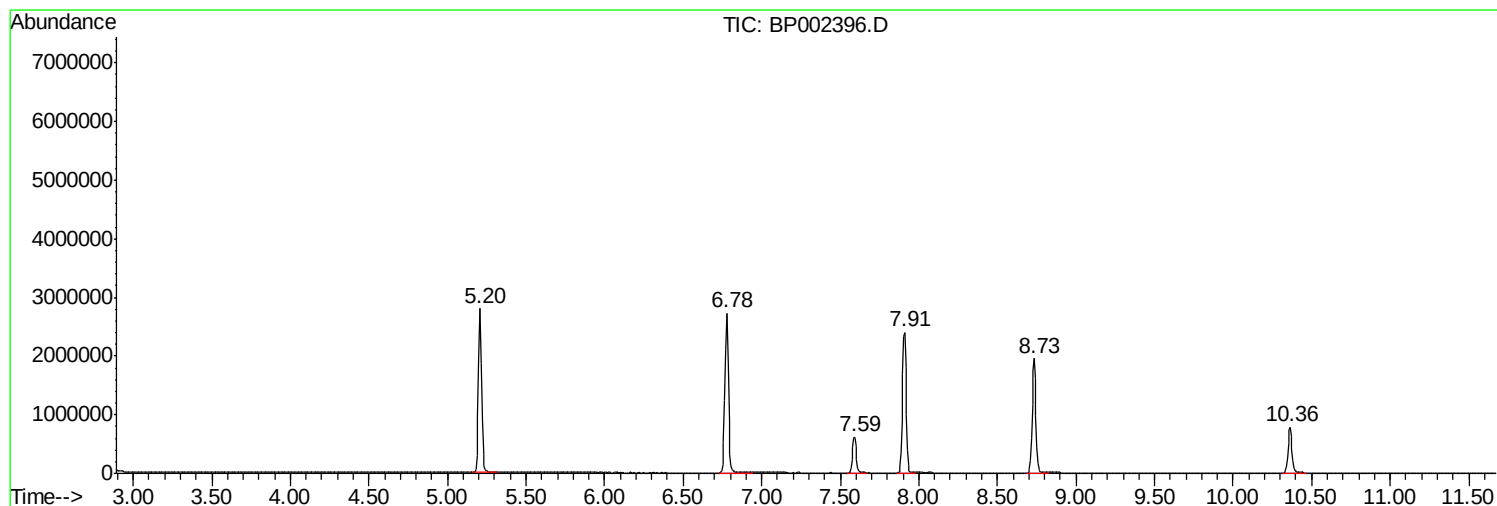

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP061220\
Data File : BP002396.D
Acq On : 12 Jun 2020 10:04
Operator : CG/JU
Sample : PB129455BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129455BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP061220\
Data File : BP002396.D
Acq On : 12 Jun 2020 10:04
Operator : CG/JU
Sample : PB129455BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129455BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc