

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061220\
Data File : BP002397.D
Acq On : 12 Jun 2020 13:45
Operator : CG/JU
Sample : PB129511BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129511BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.205	387	394	410	rBV	3011567	4598567	44.73%	8.700%
2	6.781	652	662	680	rBV	2930005	4871575	47.38%	9.217%
3	7.593	793	800	811	rBV	681994	1055019	10.26%	1.996%
4	7.911	846	854	866	rBV	2592288	4224236	41.08%	7.992%
5	8.734	985	994	1013	rBV	2062722	3413120	33.20%	6.457%
6	10.369	1263	1272	1288	rBV	839658	1469395	14.29%	2.780%
7	12.863	1688	1696	1716	rBV	4550703	7325669	71.25%	13.859%
8	14.246	1924	1931	1942	rBV	1288820	1944834	18.92%	3.679%
9	15.746	2178	2186	2205	rBV	3441937	5380769	52.33%	10.180%
10	17.004	2392	2400	2414	rBV	1602762	2362002	22.97%	4.469%
11	19.592	2834	2840	2854	rBV	7613849	10281784	100.00%	19.452%
12	21.104	3092	3097	3111	rBV	2222420	2761736	26.86%	5.225%
13	21.222	3113	3117	3124	rVV	79606	114004	1.11%	0.216%
14	22.692	3363	3367	3377	rVB2	64043	106807	1.04%	0.202%
15	23.310	3465	3472	3482	rVB	1531560	2826178	27.49%	5.347%
16	23.904	3569	3573	3579	rVB3	64348	121030	1.18%	0.229%




Sum of corrected areas: 52856725

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061220\
Data File : BP002397.D
Acq On : 12 Jun 2020 13:45
Operator : CG/JU
Sample : PB129511BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129511BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

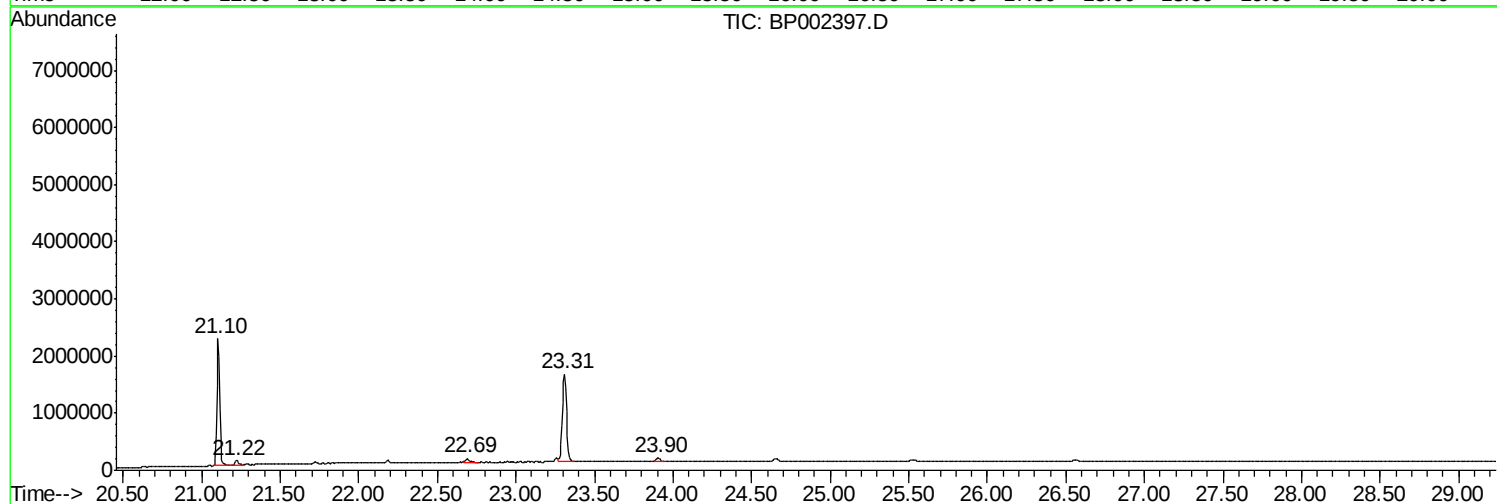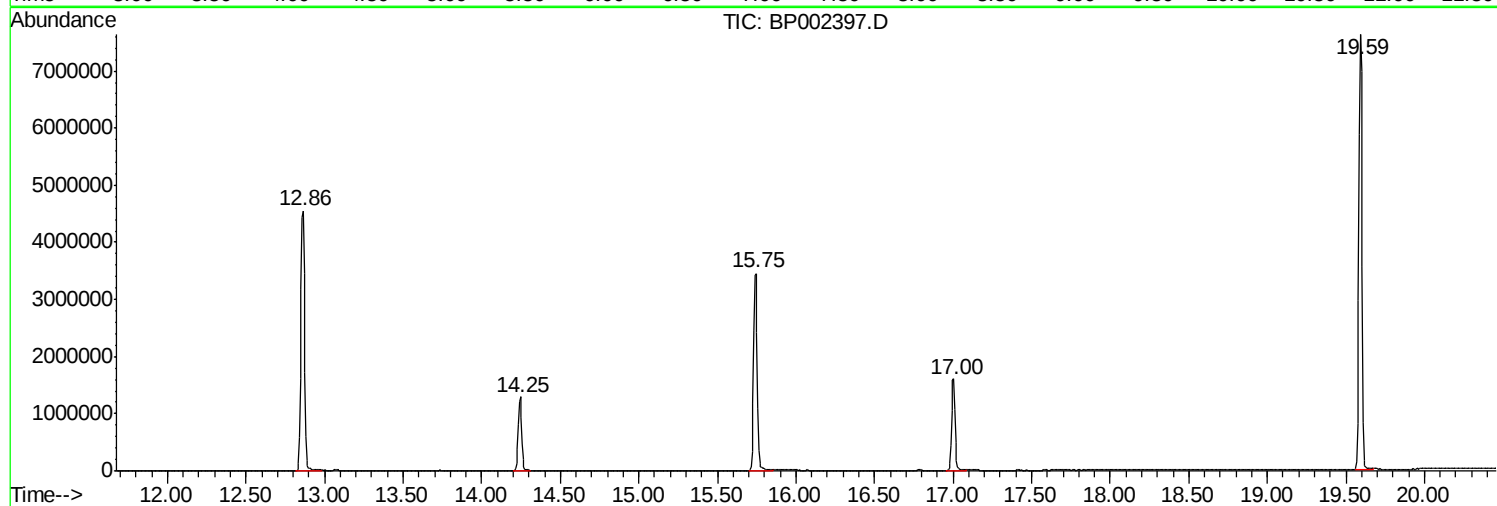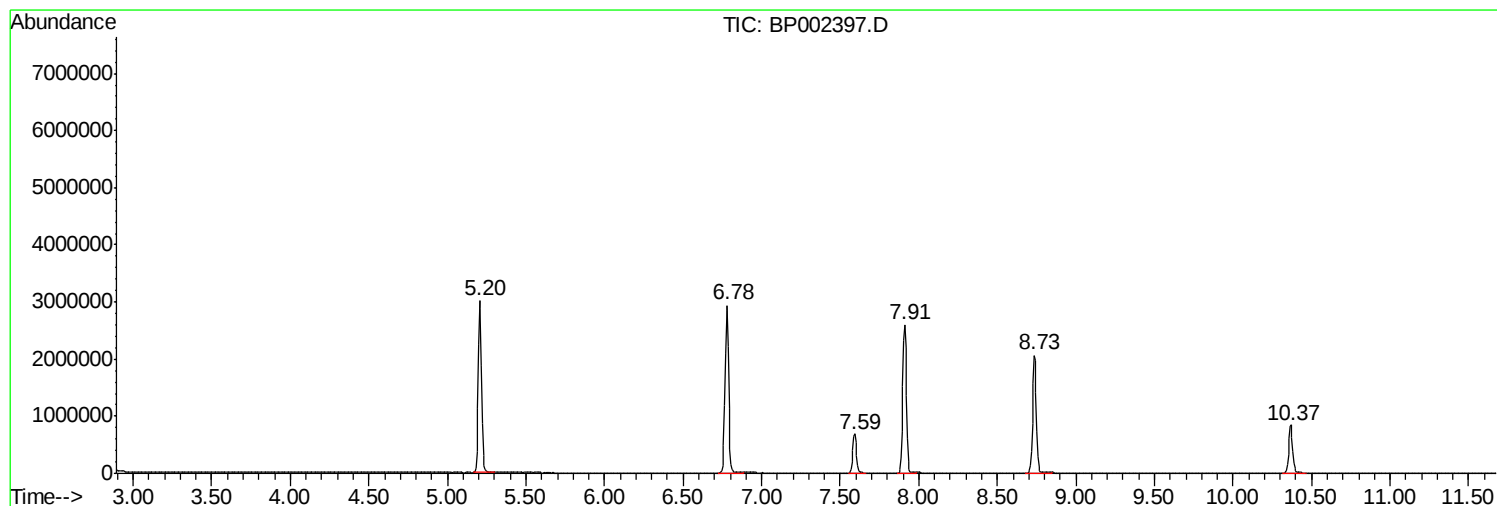

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP061220\
Data File : BP002397.D
Acq On : 12 Jun 2020 13:45
Operator : CG/JU
Sample : PB129511BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129511BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP061220\
Data File : BP002397.D
Acq On : 12 Jun 2020 13:45
Operator : CG/JU
Sample : PB129511BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129511BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc