

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061220\
 Data File : BP002399.D
 Acq On : 12 Jun 2020 15:11
 Operator : CG/JU
 Sample : PB129506BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB129506BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.210	388	395	412	rBV	2925528	4561768	44.11%	8.641%
2	6.781	654	662	687	rBV	2970077	4823053	46.63%	9.136%
3	7.593	793	800	811	rBV	662975	1044825	10.10%	1.979%
4	7.910	846	854	886	rVB	2608550	4205611	40.66%	7.966%
5	8.734	986	994	1019	rBV	2054883	3408972	32.96%	6.457%
6	10.363	1263	1271	1290	rBV	814781	1458700	14.10%	2.763%
7	12.857	1688	1695	1721	rBV	4503653	7307962	70.66%	13.843%
8	14.239	1923	1930	1953	rBV	1303674	1974451	19.09%	3.740%
9	15.739	2178	2185	2210	rBV	3629940	5405269	52.26%	10.239%
10	16.998	2392	2399	2413	rBV	1633308	2374809	22.96%	4.498%
11	19.592	2834	2840	2858	rBV	7744294	10342369	100.00%	19.590%
12	21.104	3092	3097	3109	rBV	2204451	2740507	26.50%	5.191%
13	23.250	3458	3462	3465	rBV	81645	130058	1.26%	0.246%
14	23.303	3465	3471	3484	rVB2	1505912	2859917	27.65%	5.417%
15	23.898	3568	3572	3581	rVB4	77084	154600	1.49%	0.293%




Sum of corrected areas: 52792871

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061220\
Data File : BP002399.D
Acq On : 12 Jun 2020 15:11
Operator : CG/JU
Sample : PB129506BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129506BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

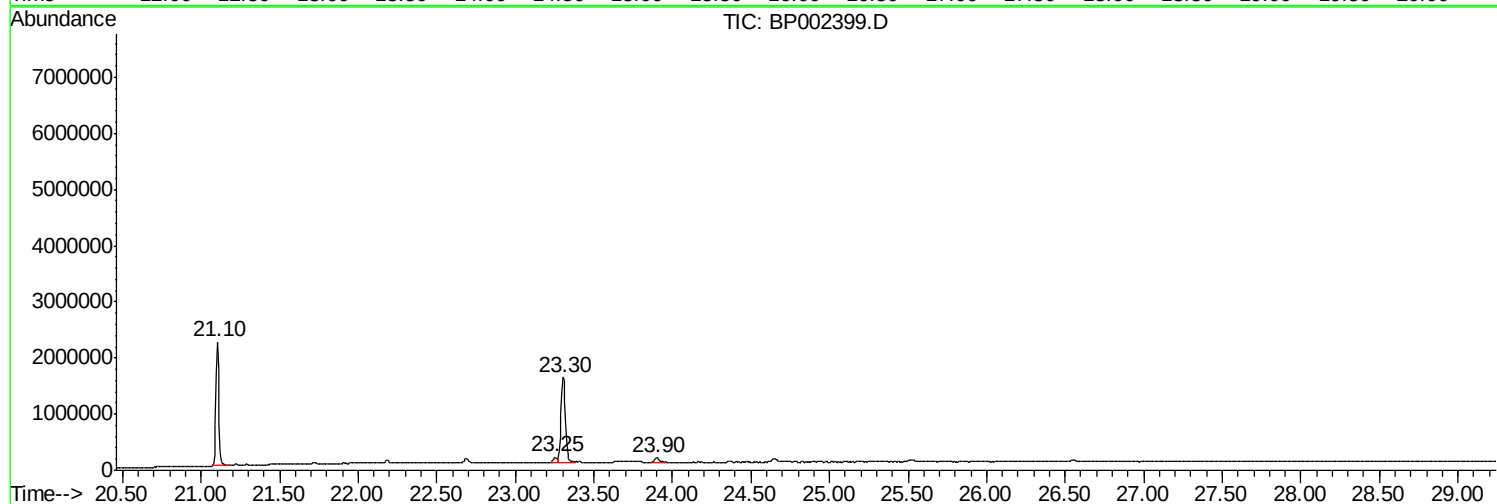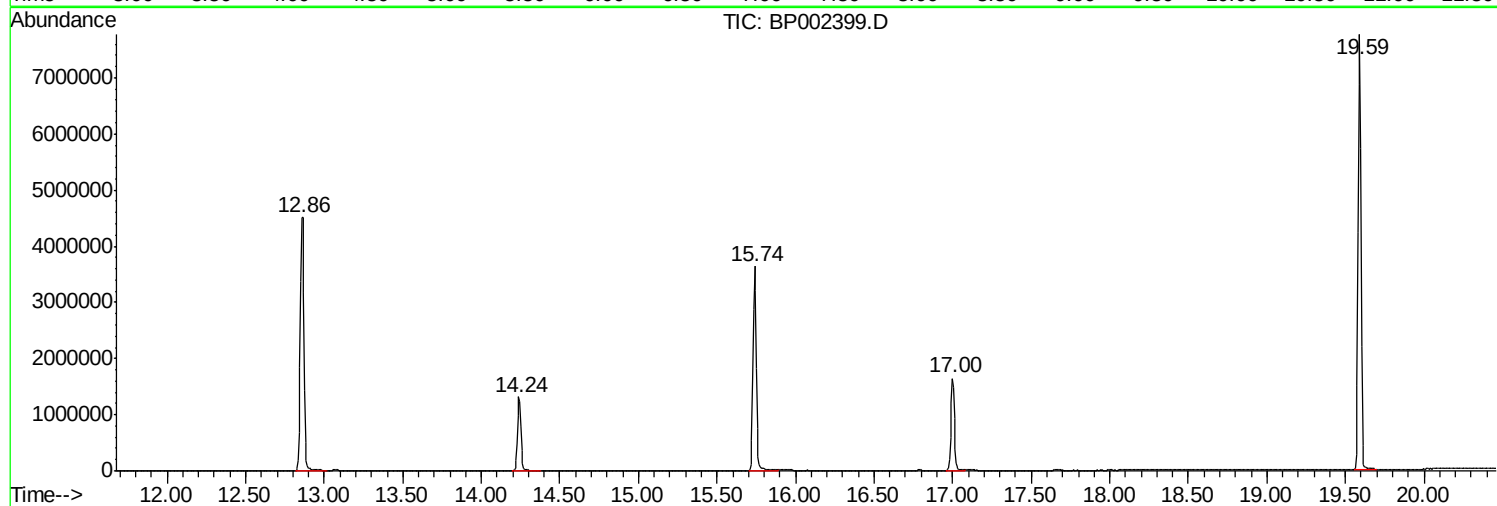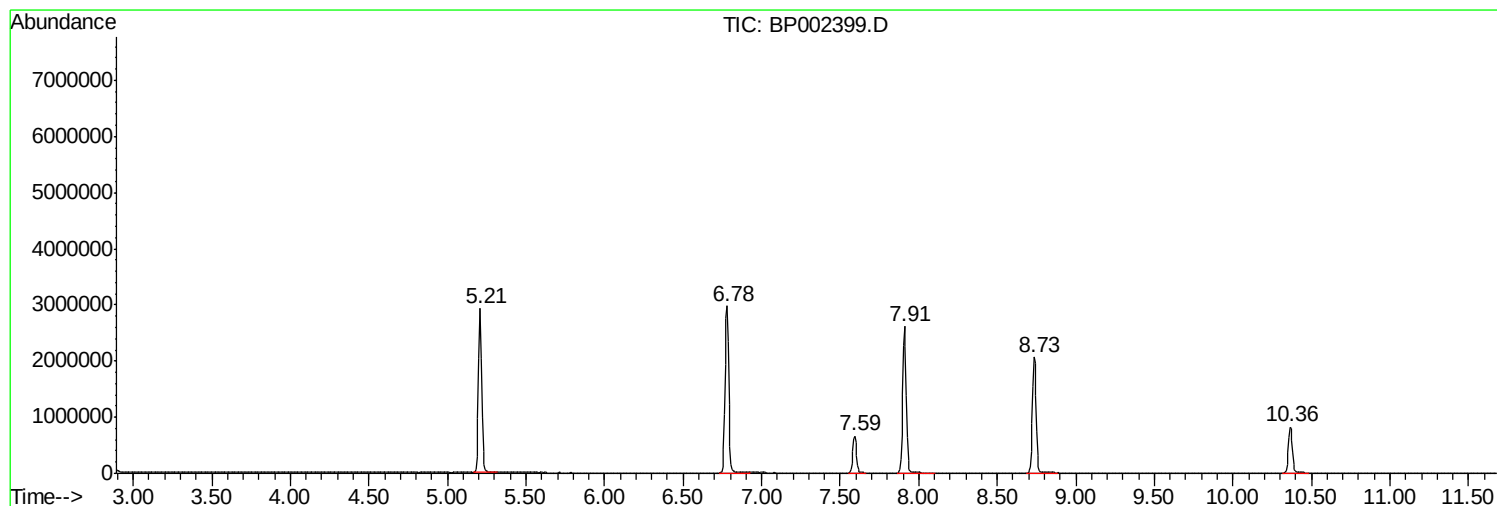

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP061220\
Data File : BP002399.D
Acq On : 12 Jun 2020 15:11
Operator : CG/JU
Sample : PB129506BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129506BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP061220\
Data File : BP002399.D
Acq On : 12 Jun 2020 15:11
Operator : CG/JU
Sample : PB129506BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129506BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc