


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061220\
 Data File : BP002394.D
 Acq On : 12 Jun 2020 08:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 05 15:08:53 2020

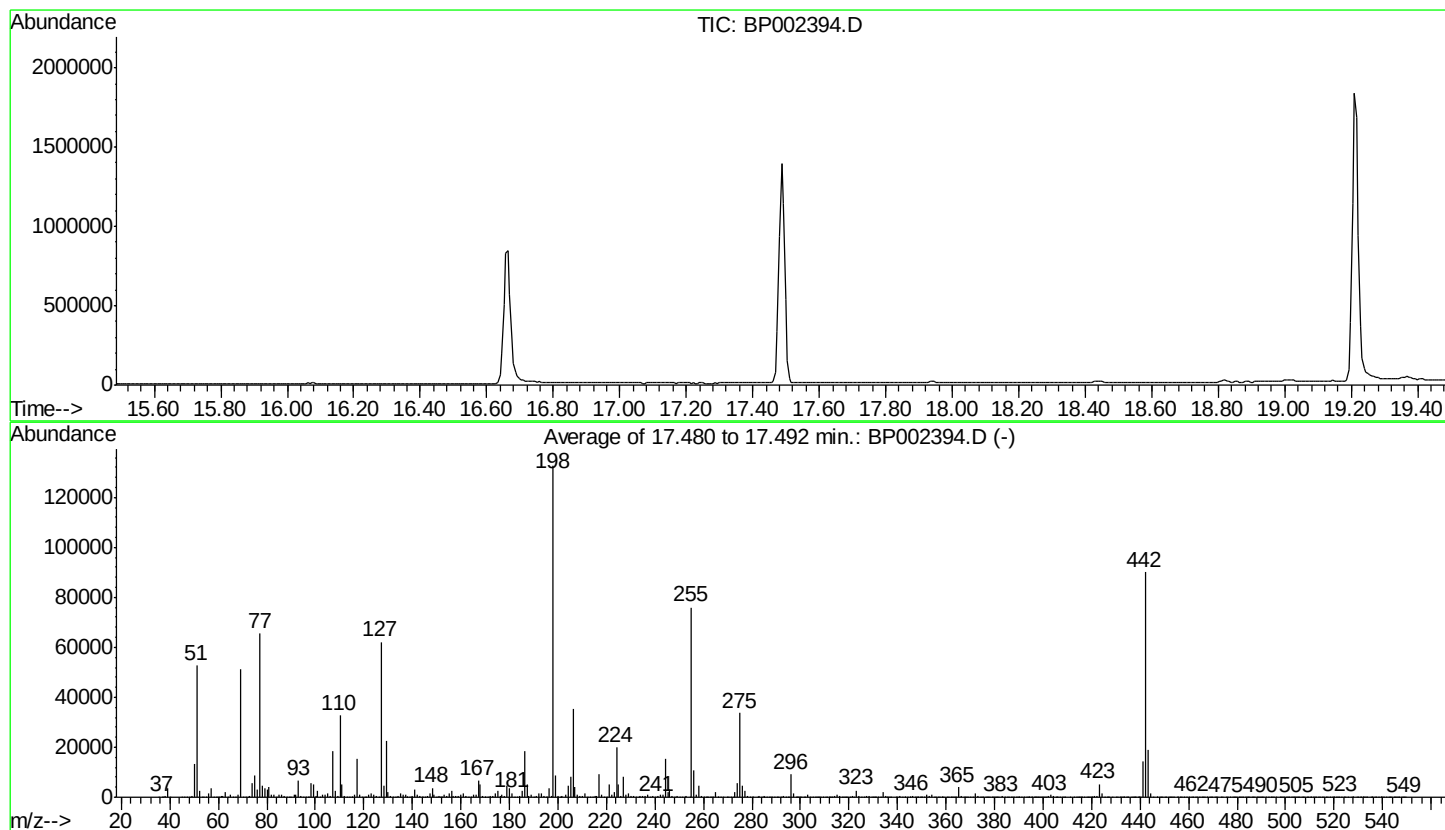

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	52683	PASS
68	69	0.00	2	1.7	858	PASS
69	198	0.00	100	38.6	51247	PASS
70	69	0.00	2	0.4	216	PASS
127	198	10	80	46.8	62109	PASS
197	198	0.00	2	0.4	587	PASS
198	198	100	100	100.0	132722	PASS
199	198	5	9	6.7	8928	PASS
275	198	10	60	25.4	33698	PASS
365	198	1	100	3.1	4076	PASS
441	198	0.01	100	10.7	14161	PASS
442	198	50	100	67.9	90082	PASS
443	442	15	24	20.8	18724	PASS