
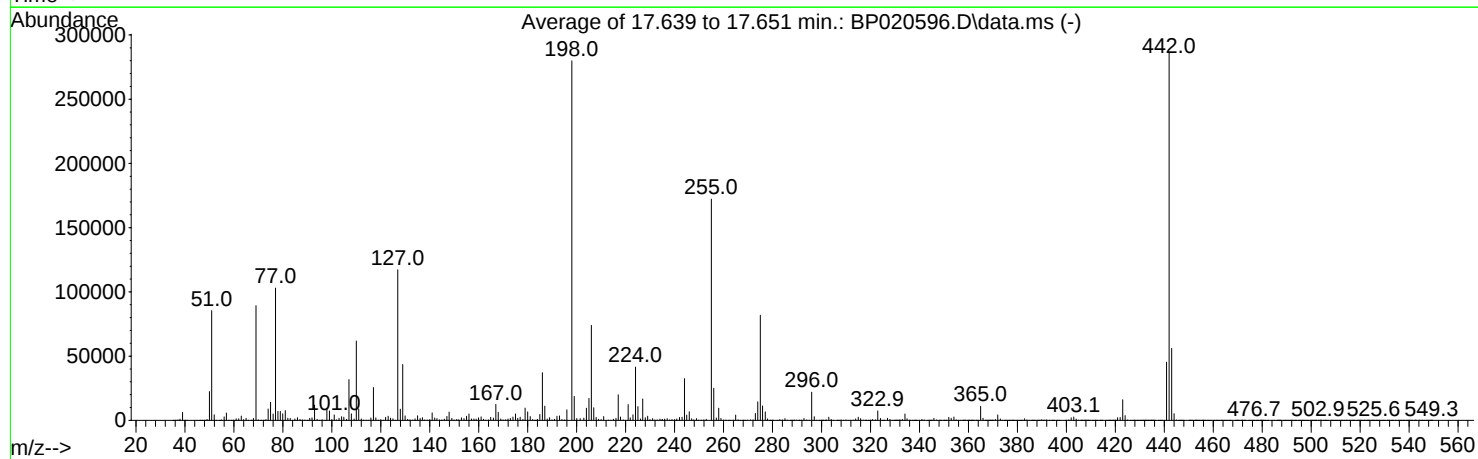


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061224\
Data File : BP020596.D
Acq On : 12 Jun 2024 10:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 30 03:41:03 2024

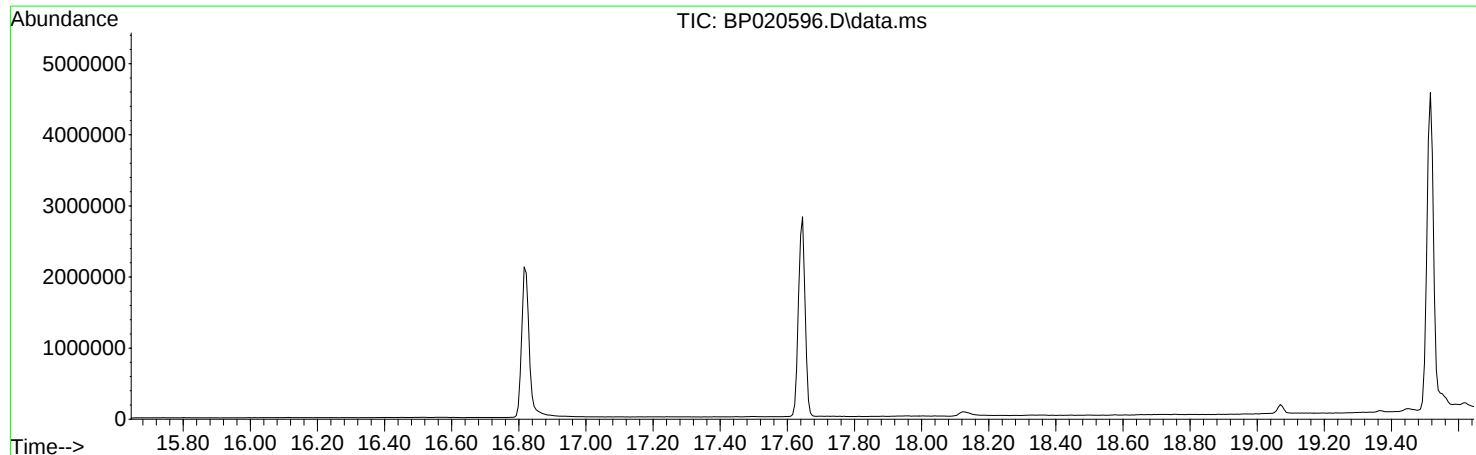




AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	85418	PASS
68	69	0.00	2	1.7	1503	PASS
69	198	0.00	100	31.9	89257	PASS
70	69	0.00	2	0.5	475	PASS
127	198	10	80	41.9	117163	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	279915	PASS
199	198	5	9	6.7	18727	PASS
275	198	10	60	29.3	81899	PASS
365	198	1	100	3.9	10969	PASS
441	198	0.01	100	16.2	45281	PASS
442	442	100	100	100.0	286357	PASS
443	442	15	24	19.6	56056	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061224\
Data File : BP020596.D
Acq On : 12 Jun 2024 10:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 12 12:28:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

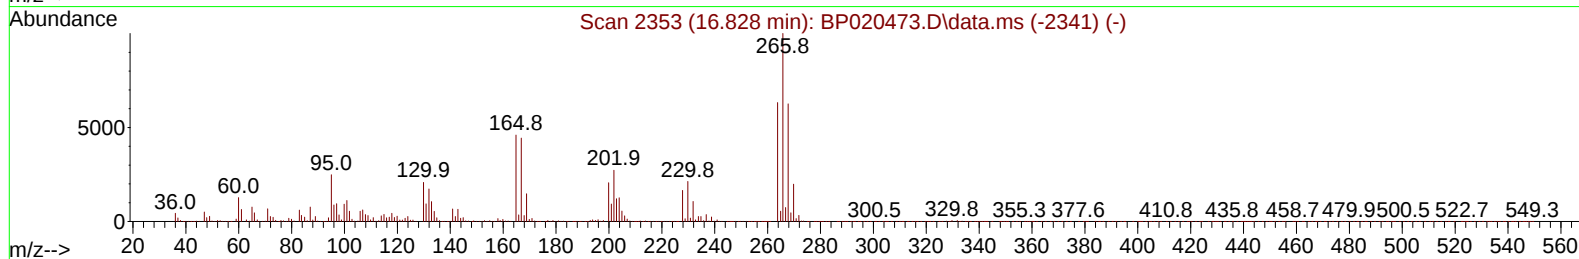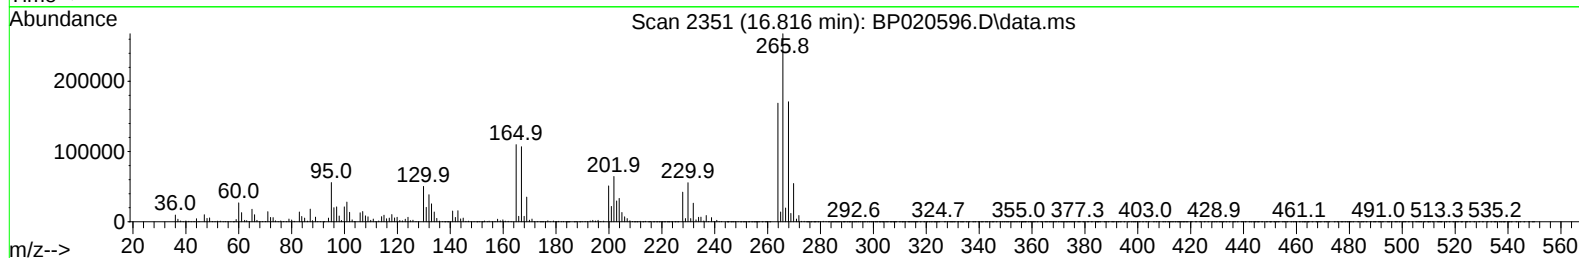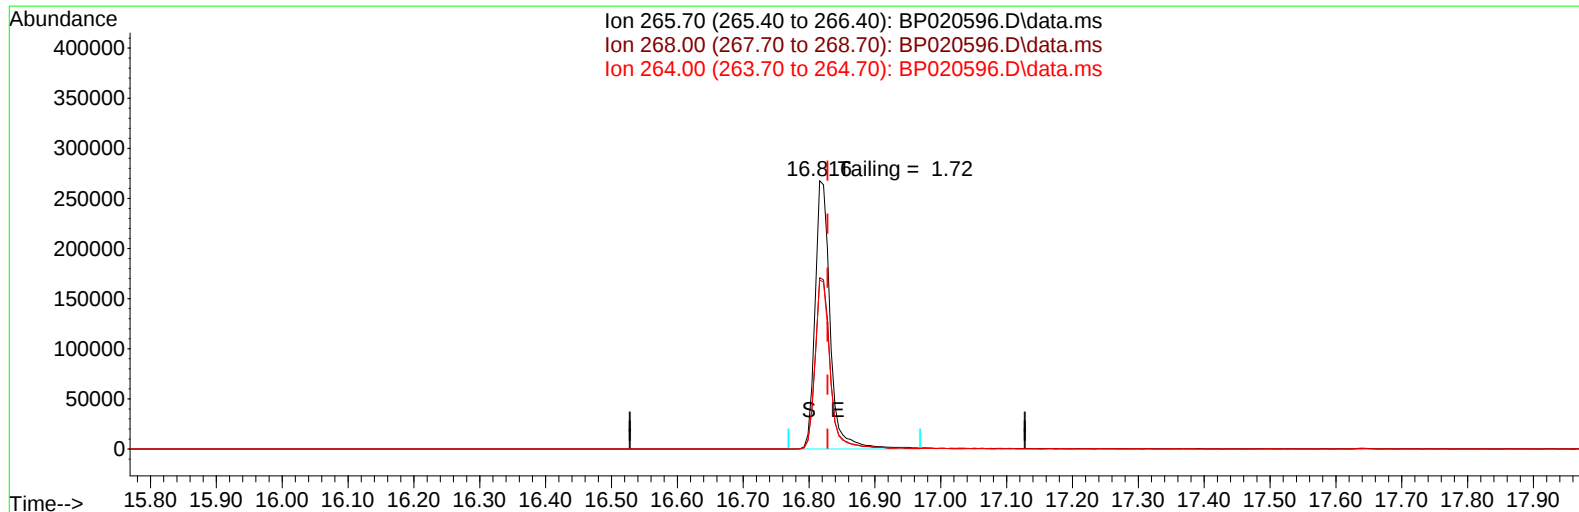

TIC: BP020596.D\data.ms

(70) Pentachlorophenol (C)

16.816min (-0.012) 111404.76 ng




response 428519

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.86
264.00	63.30	63.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061224\
Data File : BP020596.D
Acq On : 12 Jun 2024 10:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 12 12:28:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

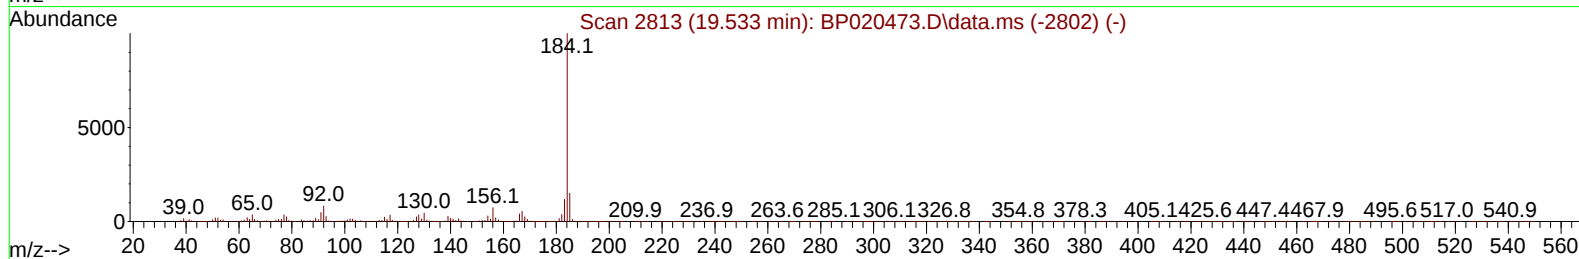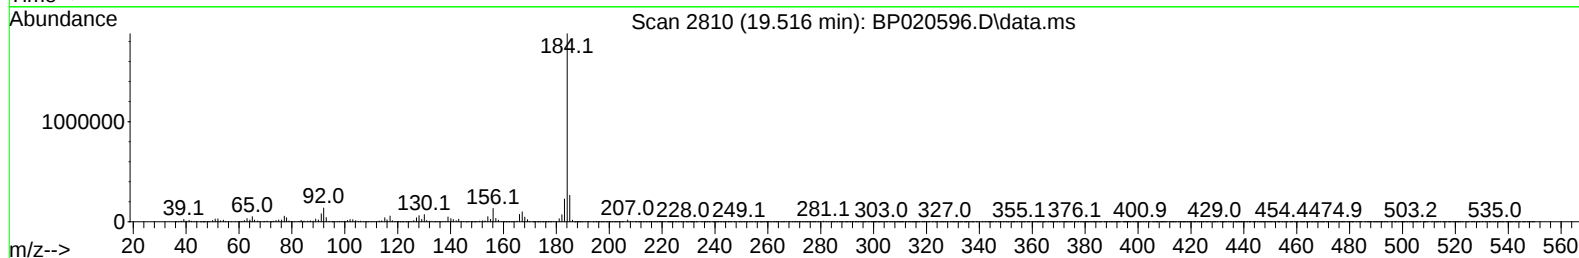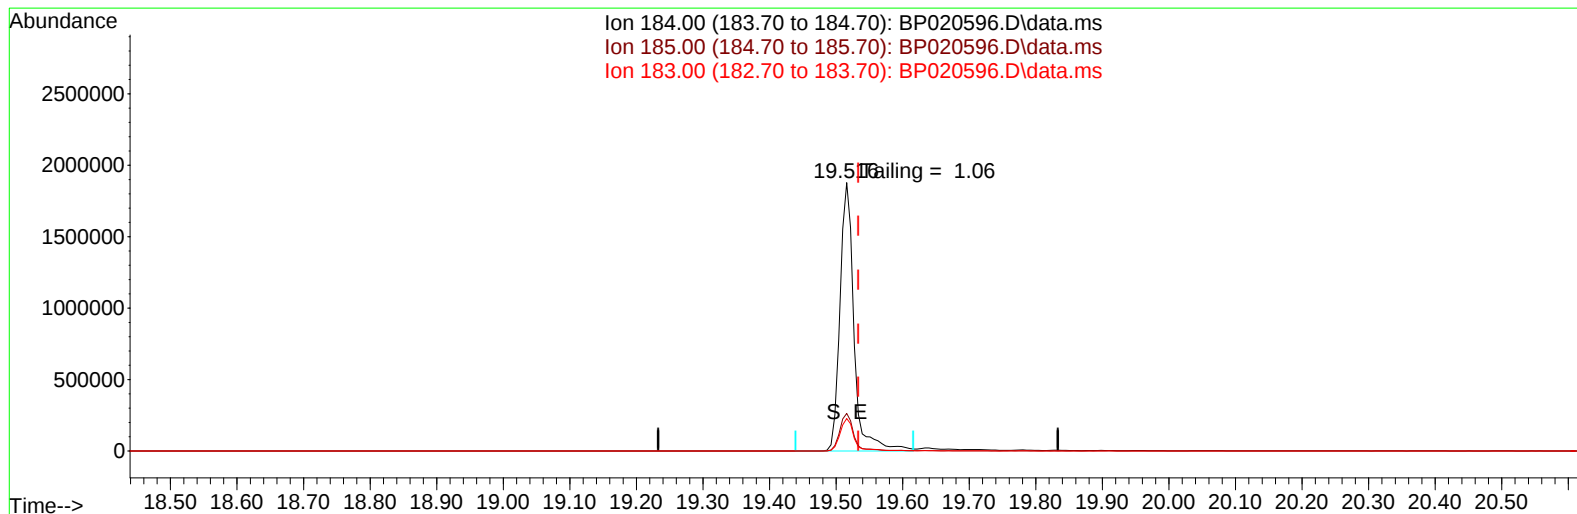

TIC: BP020596.D\data.ms

(77) Benzidine

19.516min (-0.017) 31494.05 ng

response 2753872

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.01
183.00	11.70	12.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/12/2024	BNA_P	<u>BP020596.D</u>
Compound Name	Response	Retention Time
DDT	1362101	20.816
DDD	17772	20.404
DDE	1033	19.822
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18805	1380906	1.36

Instrument :
BNA_P
ClientSampleId :
DFTPP