
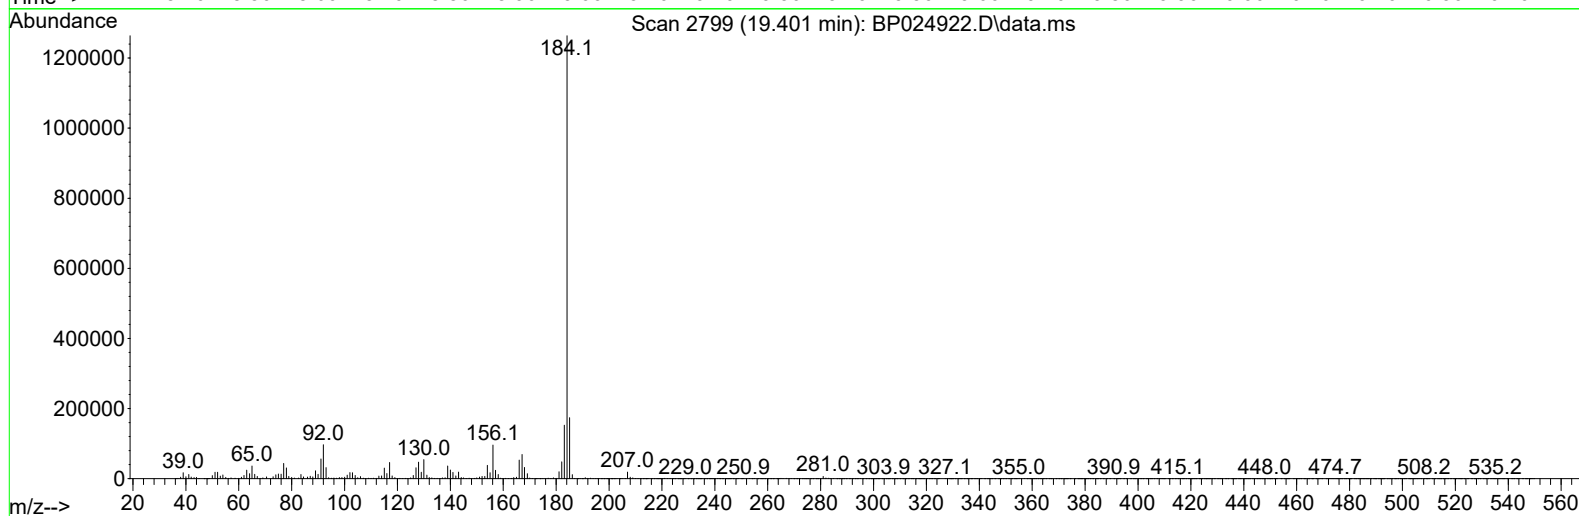


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061225\
Data File : BP024922.D
Acq On : 12 Jun 2025 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 12 12:06:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

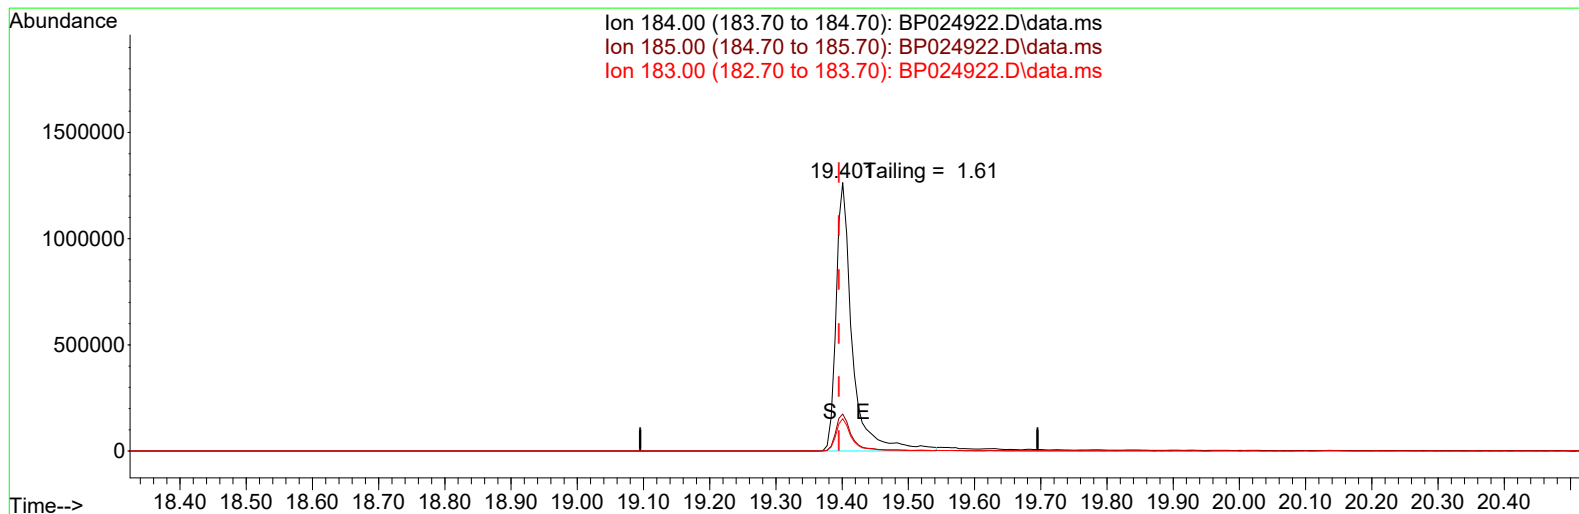



TIC: BP024922.D\data.ms

(77) Benzidine**19.401min (+ 0.006) 324533.09 ng****response 2120816**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.76
183.00	11.90	12.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061225\
Data File : BP024922.D
Acq On : 12 Jun 2025 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 12 12:06:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

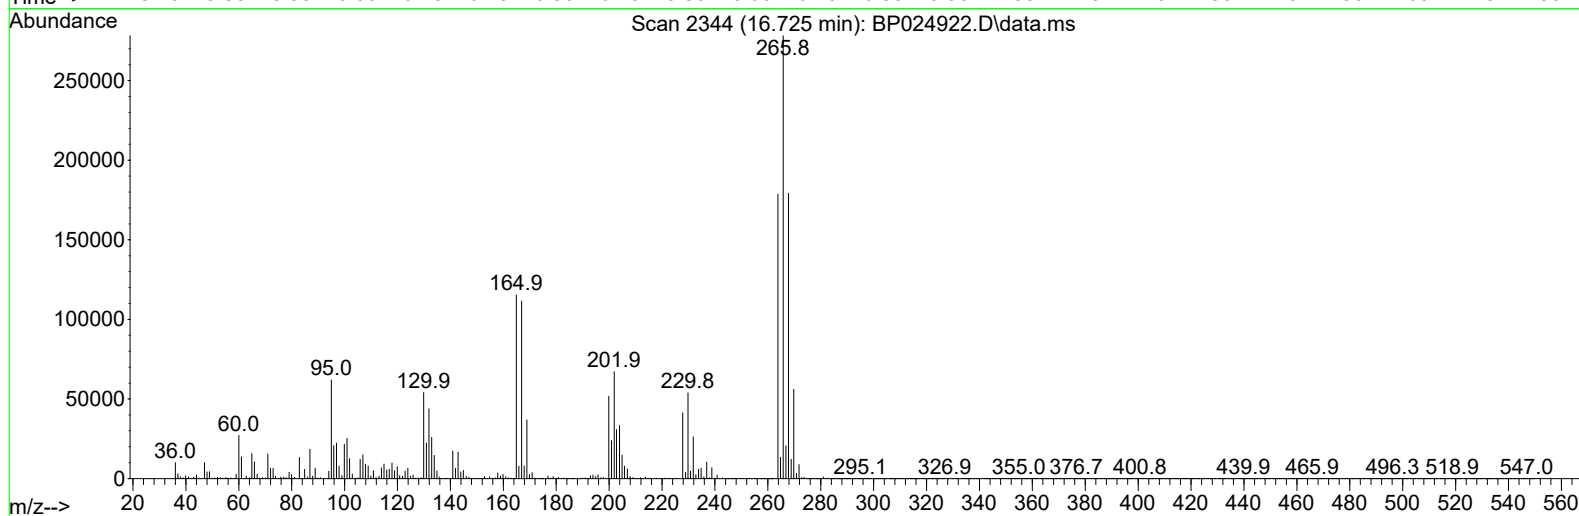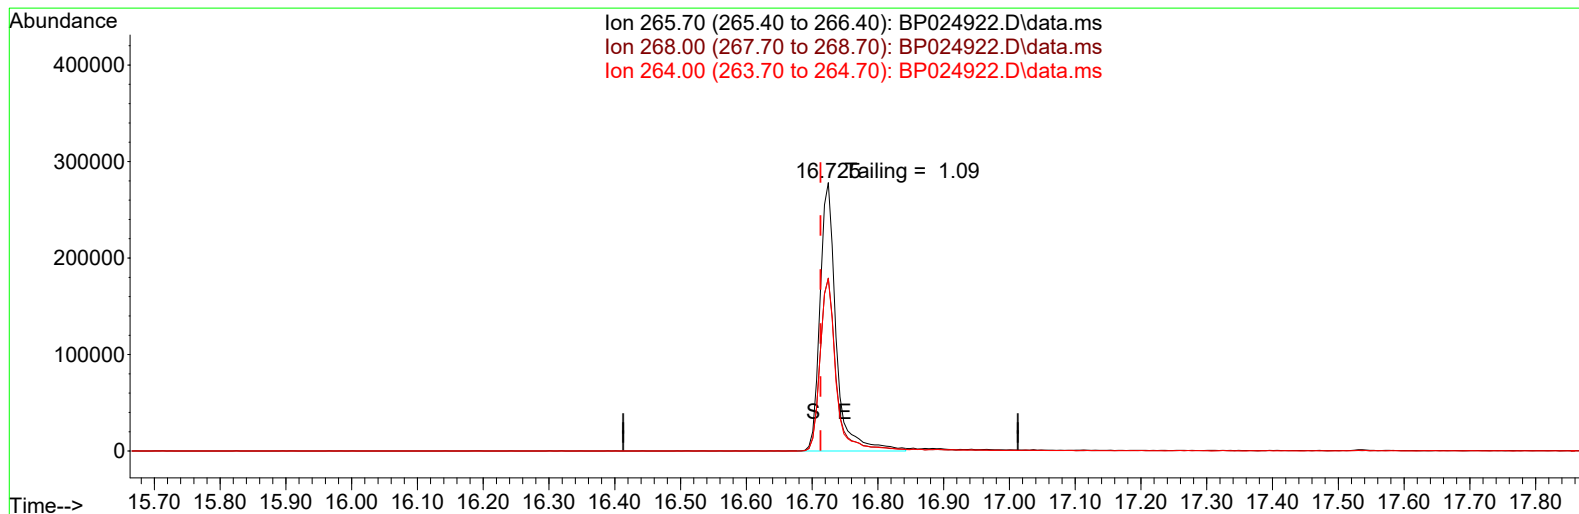

TIC: BP024922.D\data.ms

(70) Pentachlorophenol (C)

16.725min (+ 0.012) 1006246.67 ng

response 477279

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.45
264.00	62.10	64.24
0.00	0.00	0.00