
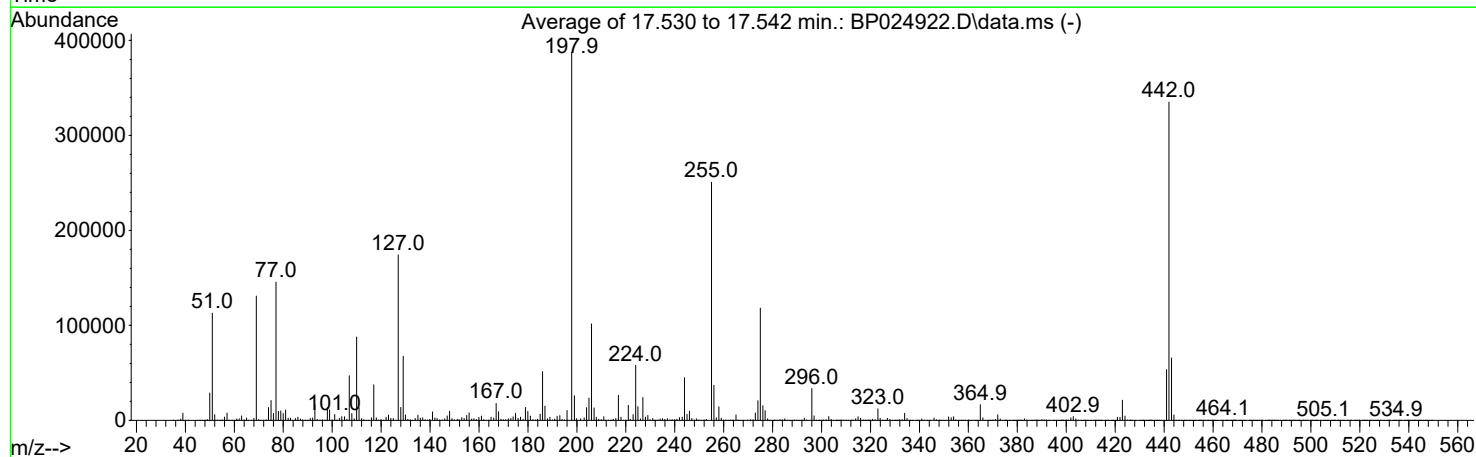


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061225\
Data File : BP024922.D
Acq On : 12 Jun 2025 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 06 16:20:27 2025

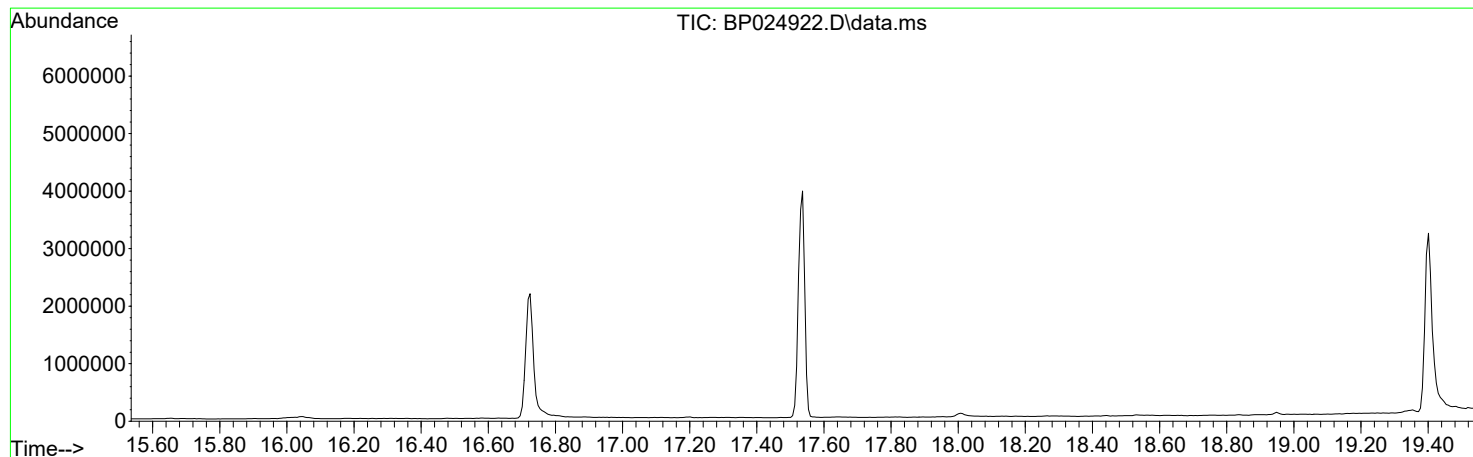

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	112814	PASS
68	69	0.00	2	1.7	2287	PASS
69	198	0.00	100	33.8	130887	PASS
70	69	0.00	2	0.6	768	PASS
127	198	10	80	45.0	174154	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	387259	PASS
199	198	5	9	6.7	25880	PASS
275	198	10	60	30.5	118301	PASS
365	198	1	100	4.3	16600	PASS
441	198	0.01	100	13.8	53386	PASS
442	442	100	100	100.0	335019	PASS
443	442	15	24	19.6	65683	PASS

DDT Breakdown



Date	Instrument Name	DFTPP Data File
6/12/2025	BNA_P	<u>BP024922.D</u>
Compound Name	Response	Retention Time
DDT	1408354	20.677
DDD	56555	20.236
DDE	1953	19.689
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
58508	1466862	3.99

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061225\
Data File : BP024922.D
Acq On : 12 Jun 2025 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 12 12:06:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

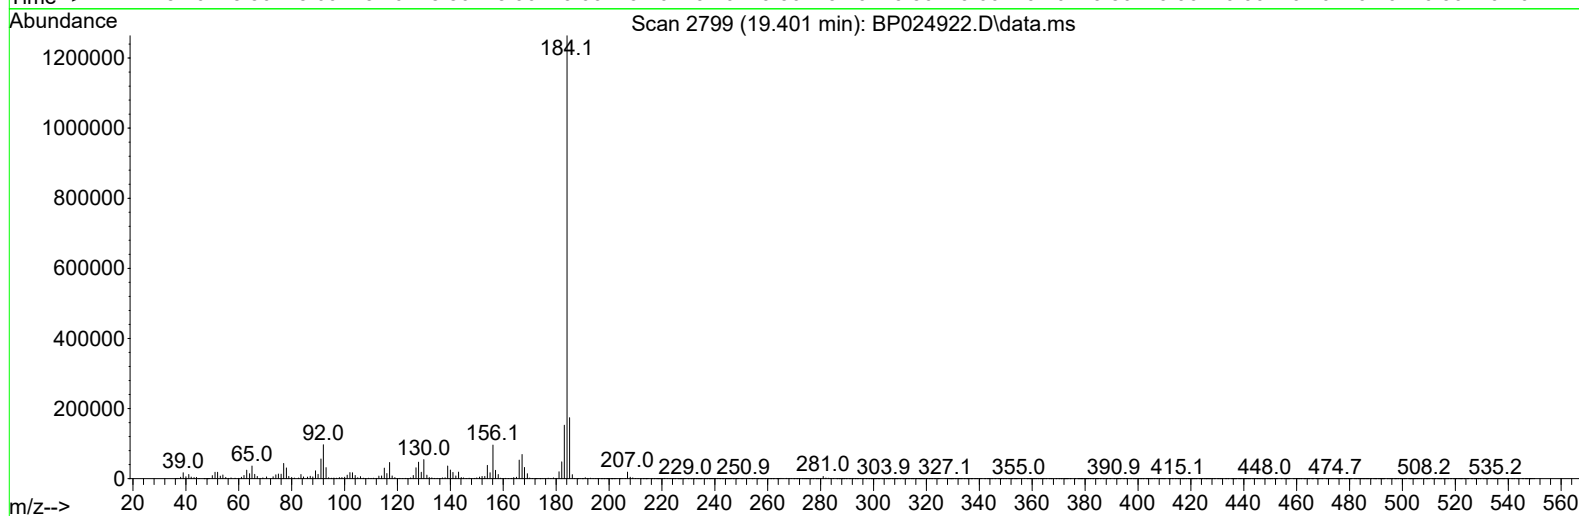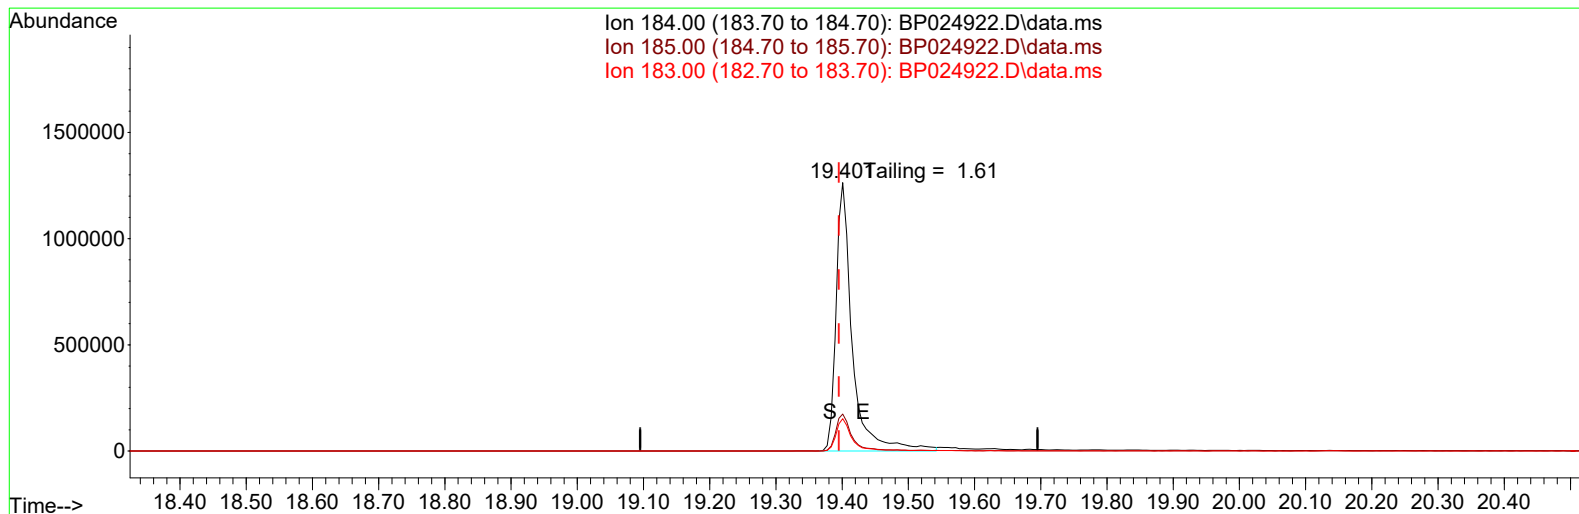

TIC: BP024922.D\data.ms

(77) Benzidine

19.401min (+ 0.006) 324533.09 ng



response 2120816

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.76
183.00	11.90	12.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061225\
Data File : BP024922.D
Acq On : 12 Jun 2025 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 12 12:06:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

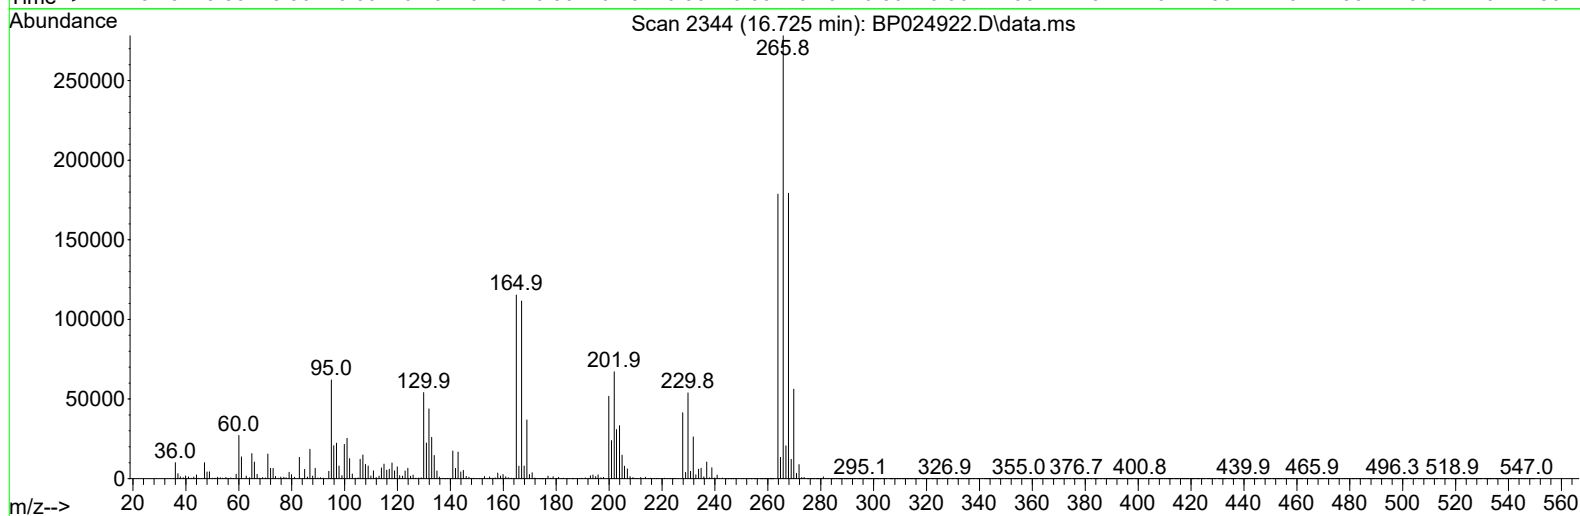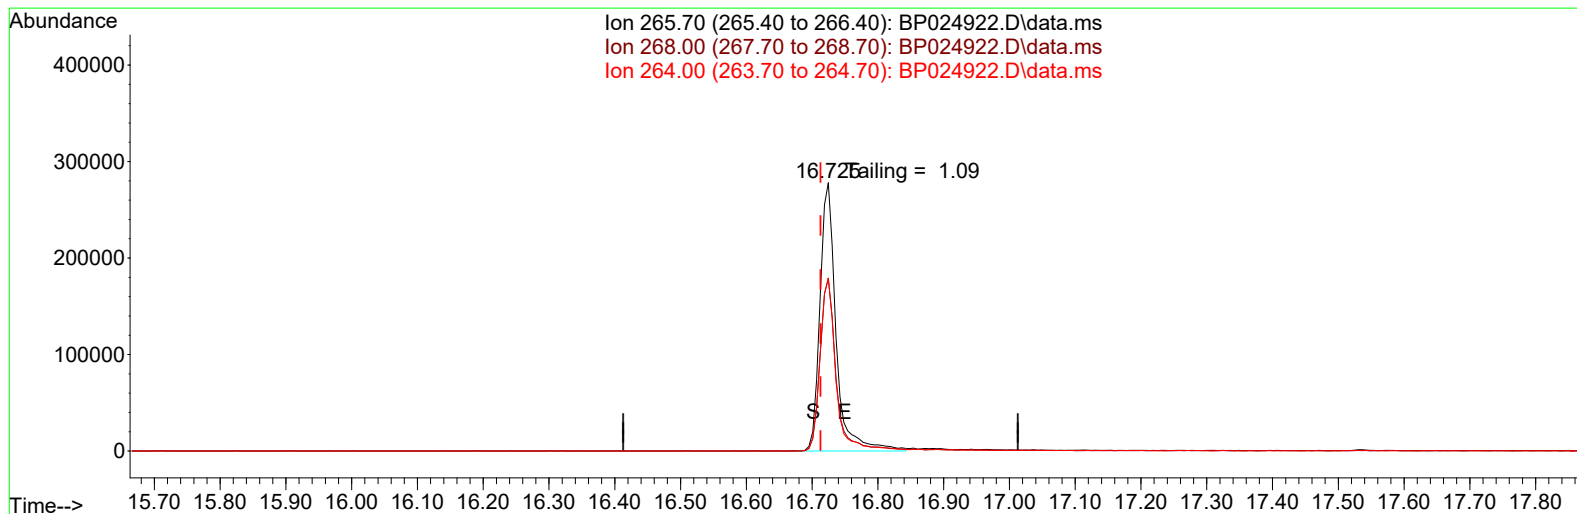

TIC: BP024922.D\data.ms

(70) Pentachlorophenol (C)

16.725min (+ 0.012) 1006246.67 ng

response 477279

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.45
264.00	62.10	64.24
0.00	0.00	0.00