
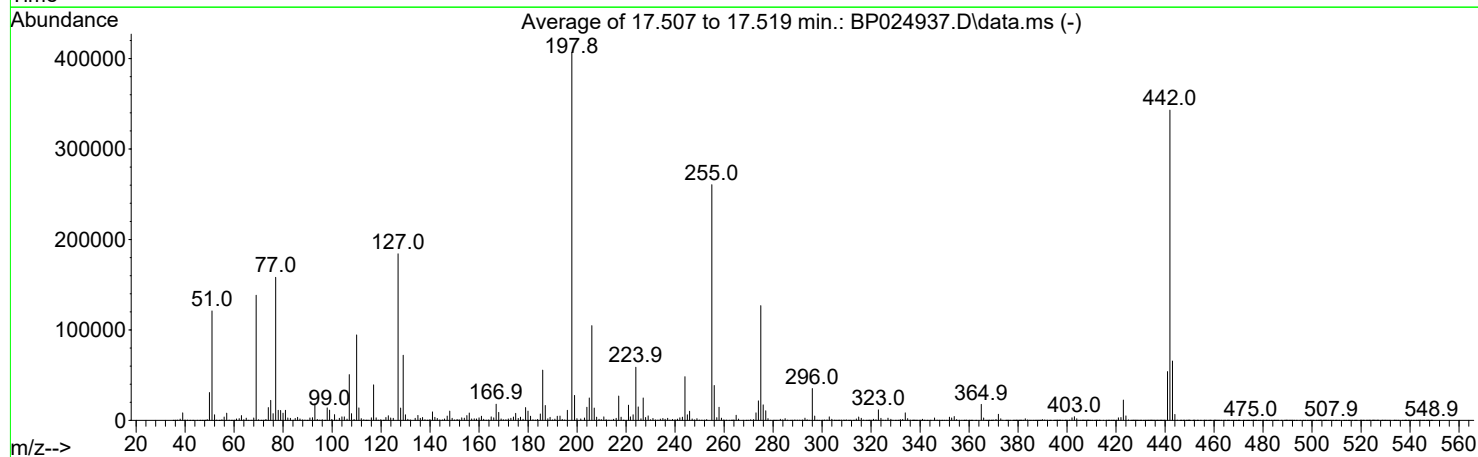


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061325\
Data File : BP024937.D
Acq On : 13 Jun 2025 10:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 06 16:20:27 2025

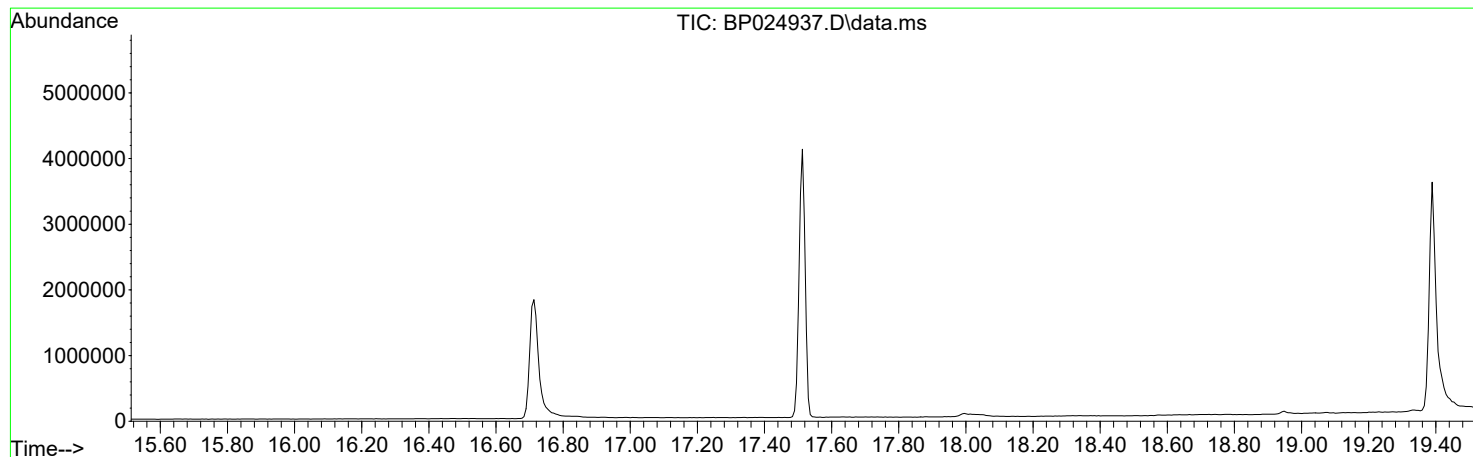

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	120987	PASS
68	69	0.00	2	1.9	2659	PASS
69	198	0.00	100	34.0	138414	PASS
70	69	0.00	2	0.5	647	PASS
127	198	10	80	45.3	184208	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	406757	PASS
199	198	5	9	6.8	27551	PASS
275	198	10	60	31.2	126932	PASS
365	198	1	100	4.3	17624	PASS
441	198	0.01	100	13.3	53925	PASS
442	442	100	100	100.0	343022	PASS
443	442	15	24	19.1	65568	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/13/2025	BNA_P	<u>BP024937.D</u>
Compound Name	Response	Retention Time
DDT	1413370	20.677
DDD	71314	20.224
DDE	3361	19.689
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
74675	1488045	5.02

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061325\
Data File : BP024937.D
Acq On : 13 Jun 2025 10:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 13 12:05:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

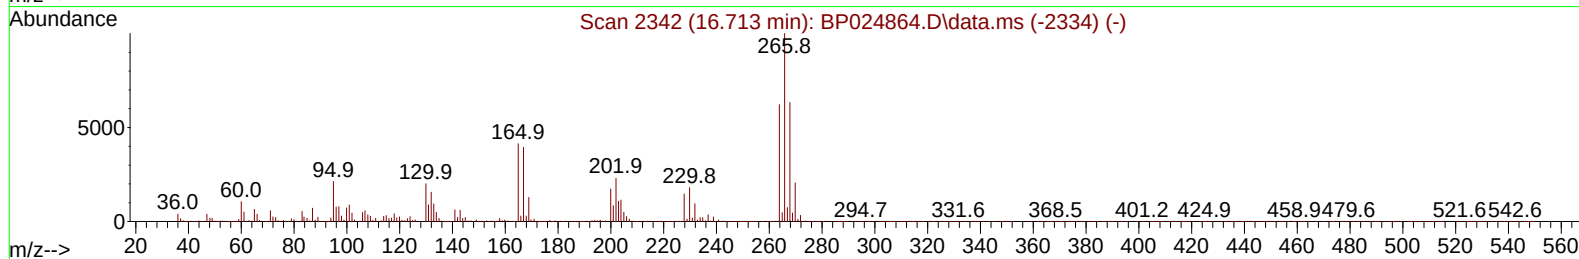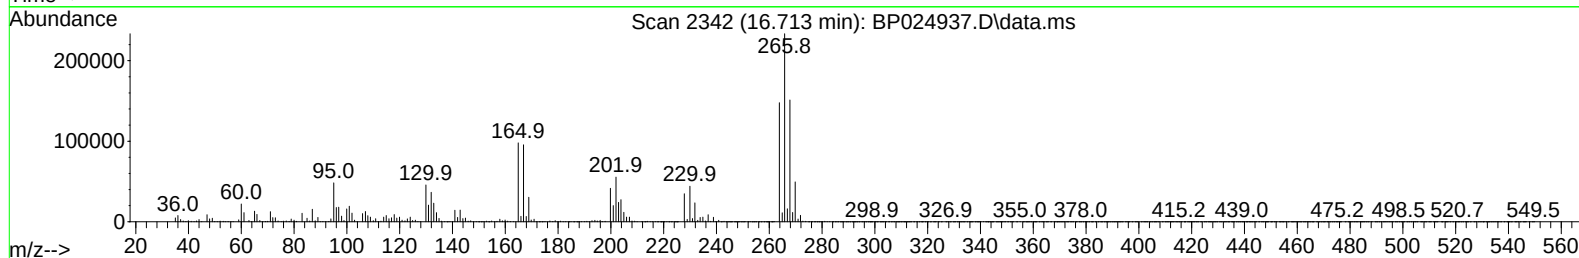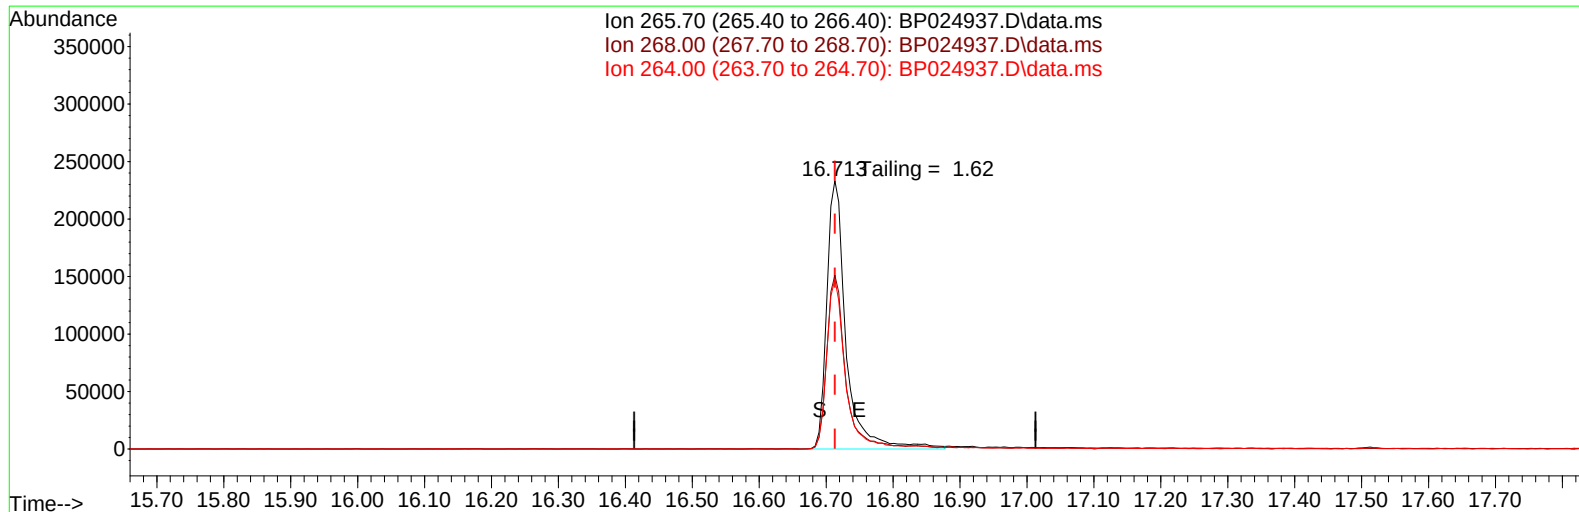

TIC: BP024937.D\data.ms

(70) Pentachlorophenol (C)

16.713min (-0.000) 217490.83 ng

response 455749

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.74
264.00	62.10	63.31
0.00	0.00	0.00

