
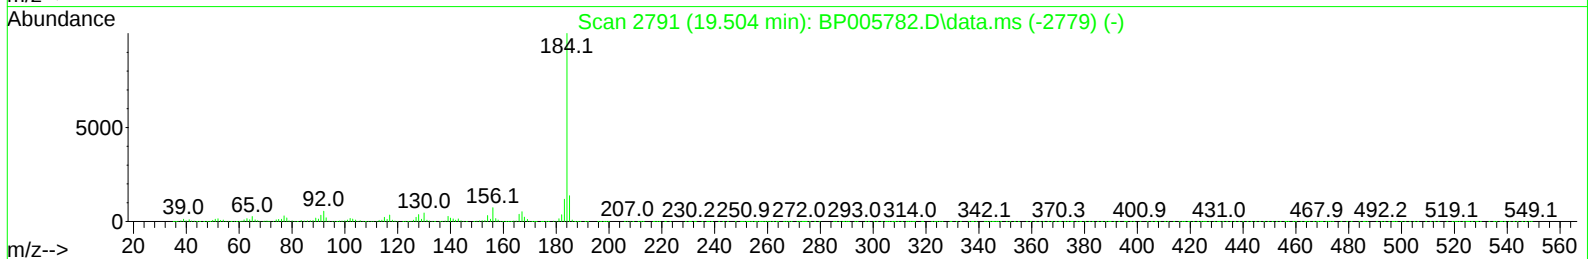
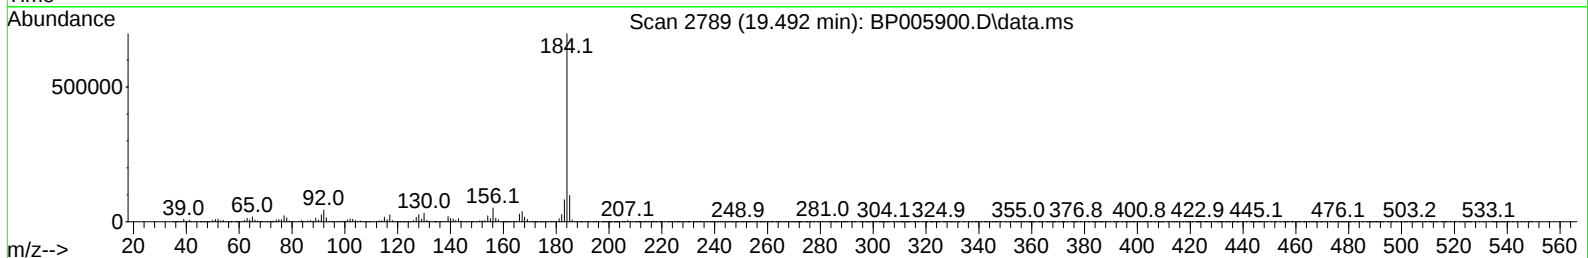


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061421\
 Data File : BP005900.D
 Acq On : 14 Jun 2021 11:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 13:10:08 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 11 13:53:36 2021
 Response via : Initial Calibration

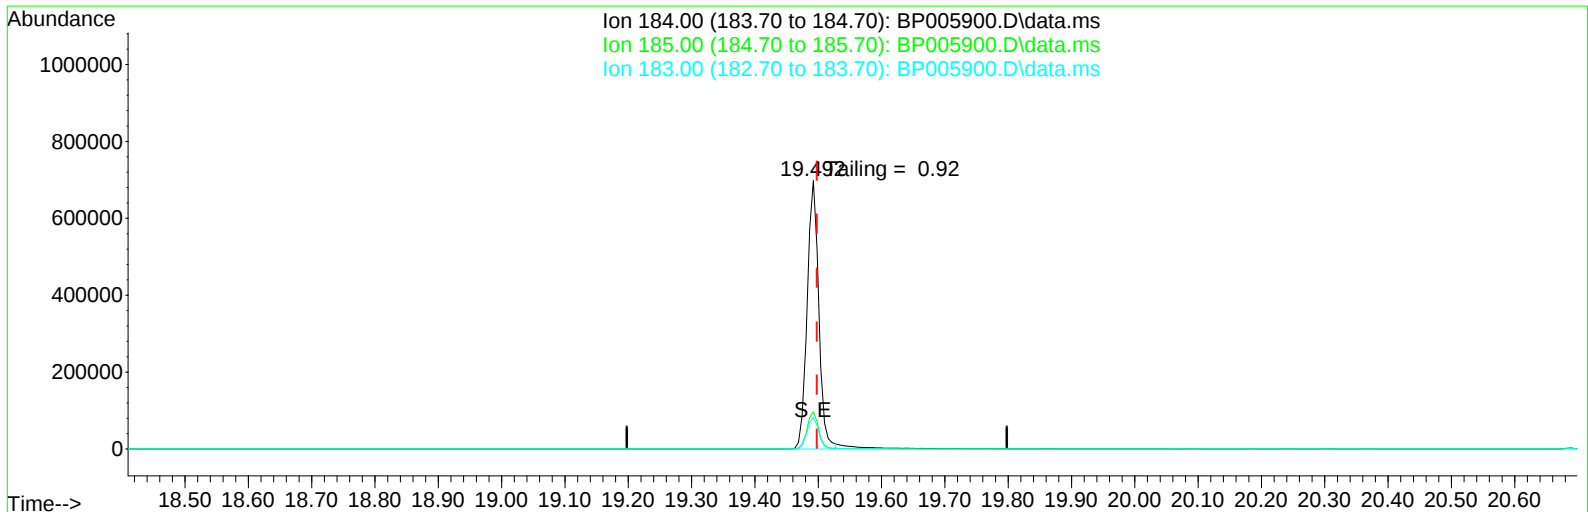




TIC: BP005900.D\data.ms

(77) Benzidine**19.492min (-0.006) 293731.88 ng****response 922908**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.93
183.00	11.90	11.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061421\
Data File : BP005900.D
Acq On : 14 Jun 2021 11:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 13:10:08 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 13:53:36 2021
Response via : Initial Calibration

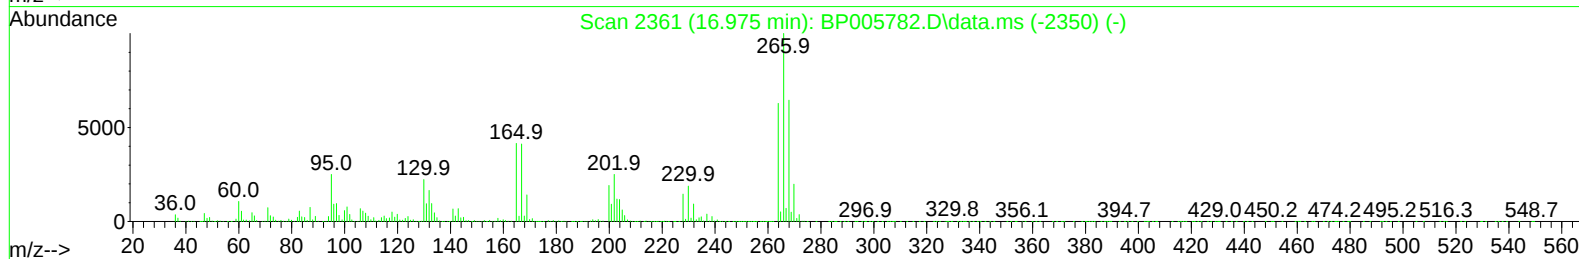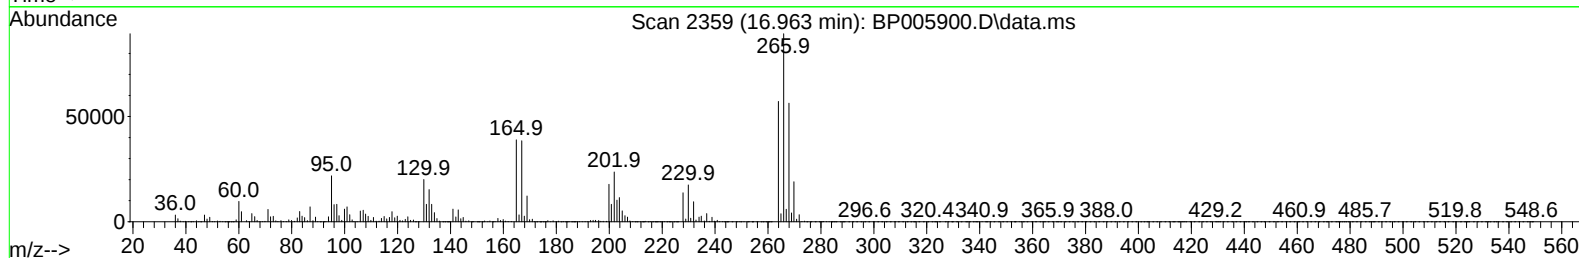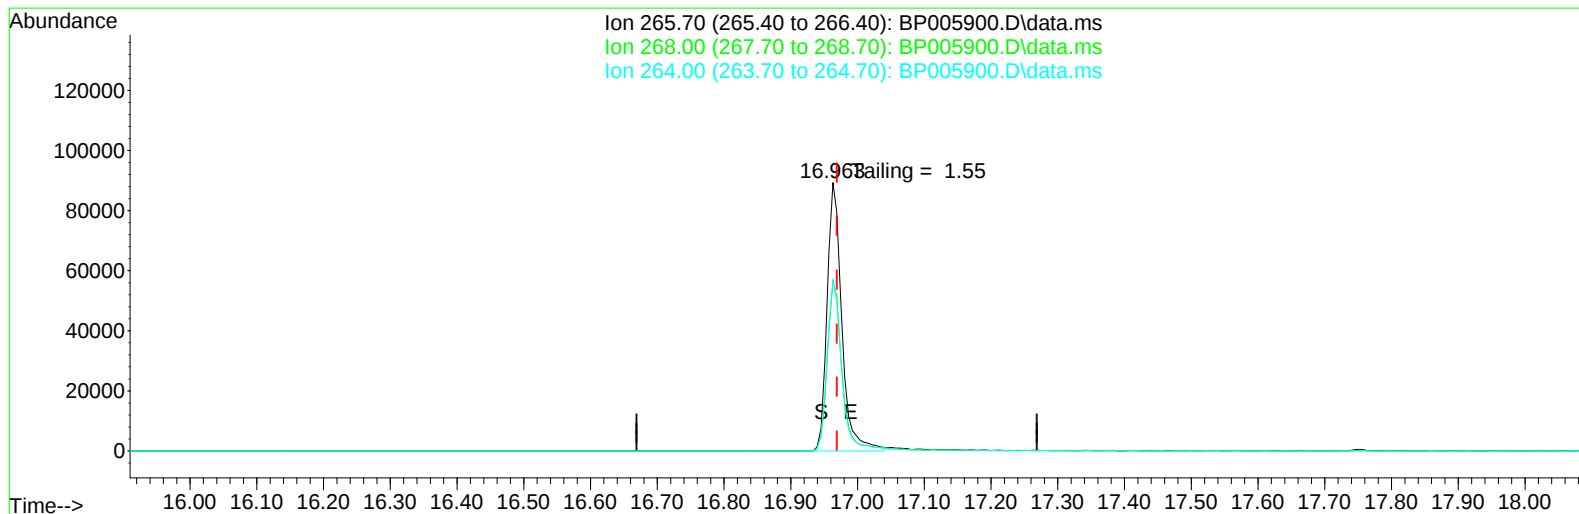

TIC: BP005900.D\data.ms

(70) Pentachlorophenol (C)

16.963min (-0.006) 651080.16 ng

response 139240

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.06
264.00	62.90	63.98
0.00	0.00	0.00