

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061421\
 Data File : BP005902.D
 Acq On : 14 Jun 2021 12:55
 Operator : CG/JU
 Sample : PB137054BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB137054BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005902.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.505	405	411	426	rBV	1158368	1755568	39.38%	9.474%
2	7.111	675	684	706	rBV	1052640	1707750	38.31%	9.216%
3	7.934	817	824	838	rVB	232688	369787	8.30%	1.996%
4	9.099	1015	1022	1037	rBV	610023	1062053	23.83%	5.732%
5	10.740	1293	1301	1312	rBV	257029	462424	10.37%	2.496%
6	13.193	1711	1718	1732	rBV	1762194	2503616	56.16%	13.511%
7	14.563	1943	1951	1961	rBV	407345	604961	13.57%	3.265%
8	16.051	2196	2204	2225	rBV	1526753	2180159	48.91%	11.766%
9	17.310	2410	2418	2432	rBV	509338	749304	16.81%	4.044%
10	19.857	2845	2851	2865	rBV	3715582	4457636	100.00%	24.057%
11	21.051	3050	3054	3058	rBV2	41425	67201	1.51%	0.363%
12	21.104	3059	3063	3067	rBV	67440	90312	2.03%	0.487%
13	21.157	3068	3072	3079	rBV	191779	275777	6.19%	1.488%
14	21.381	3105	3110	3121	rBV	804701	1042683	23.39%	5.627%
15	23.792	3514	3520	3531	rVB2	593341	1200598	26.93%	6.479%




Sum of corrected areas: 18529829

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061421\
Data File : BP005902.D
Acq On : 14 Jun 2021 12:55
Operator : CG/JU
Sample : PB137054BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137054BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

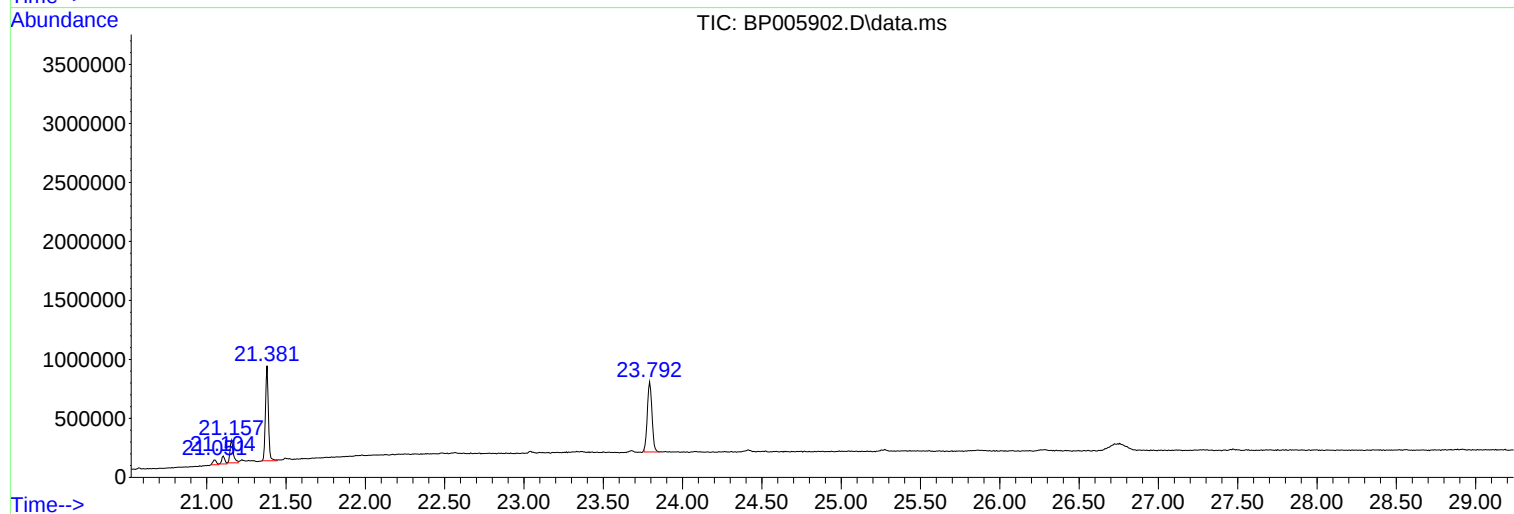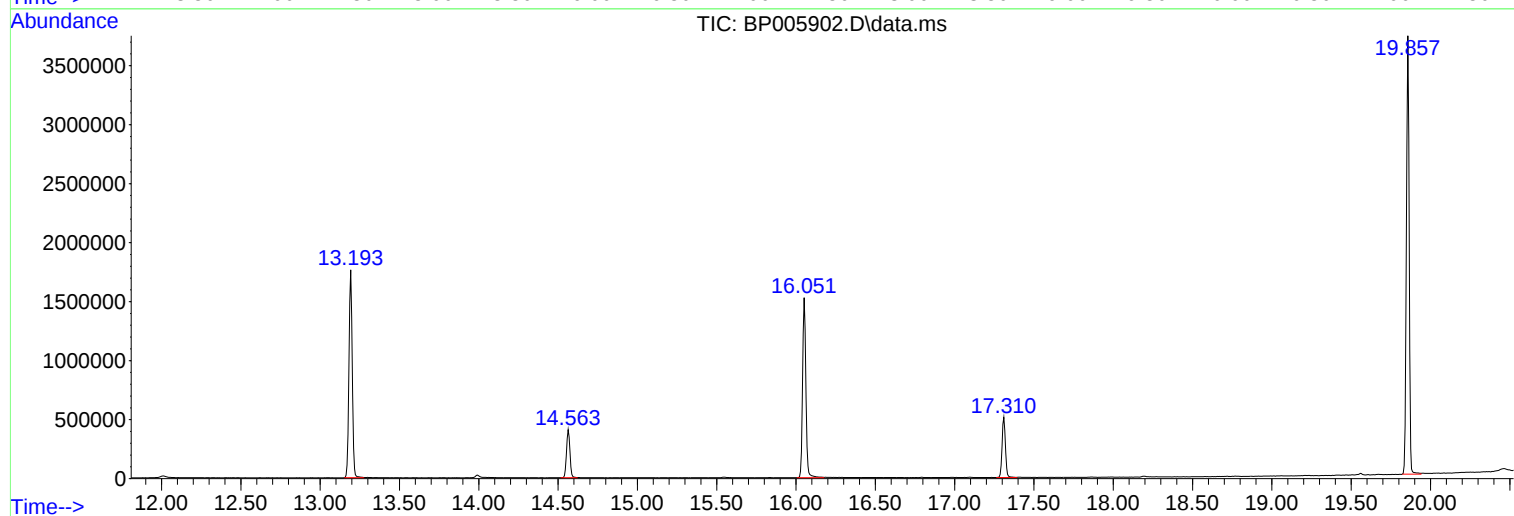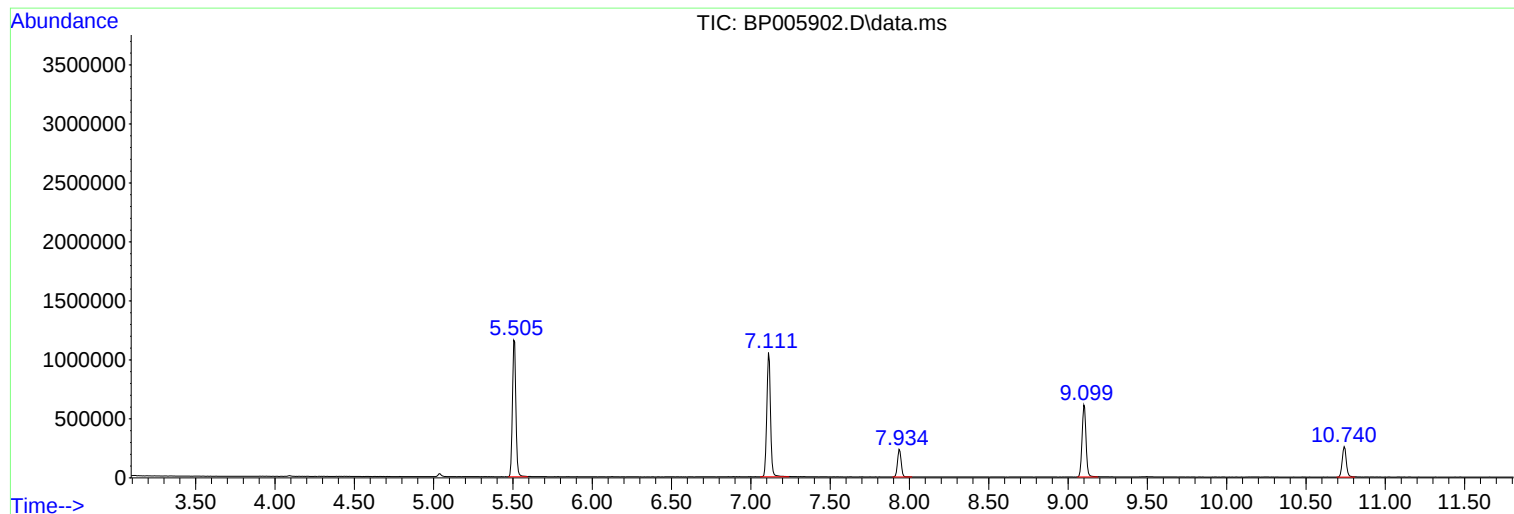

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061421\
Data File : BP005902.D
Acq On : 14 Jun 2021 12:55
Operator : CG/JU
Sample : PB137054BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137054BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061421\
Data File : BP005902.D
Acq On : 14 Jun 2021 12:55
Operator : CG/JU
Sample : PB137054BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137054BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------