
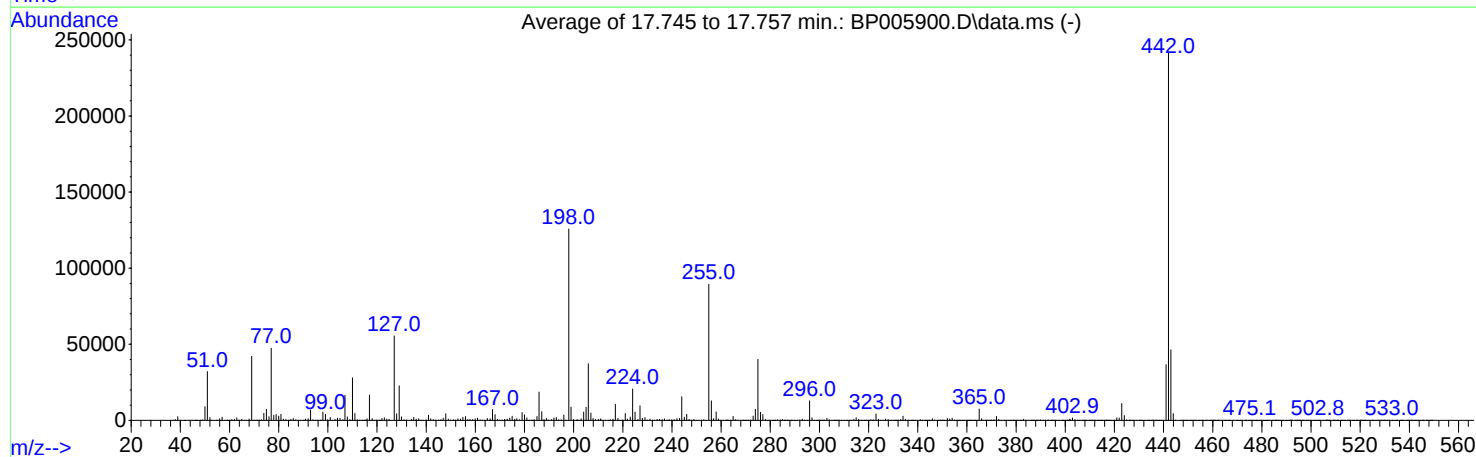


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061421\
 Data File : BP005900.D
 Acq On : 14 Jun 2021 11:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 14 13:15:03 2021

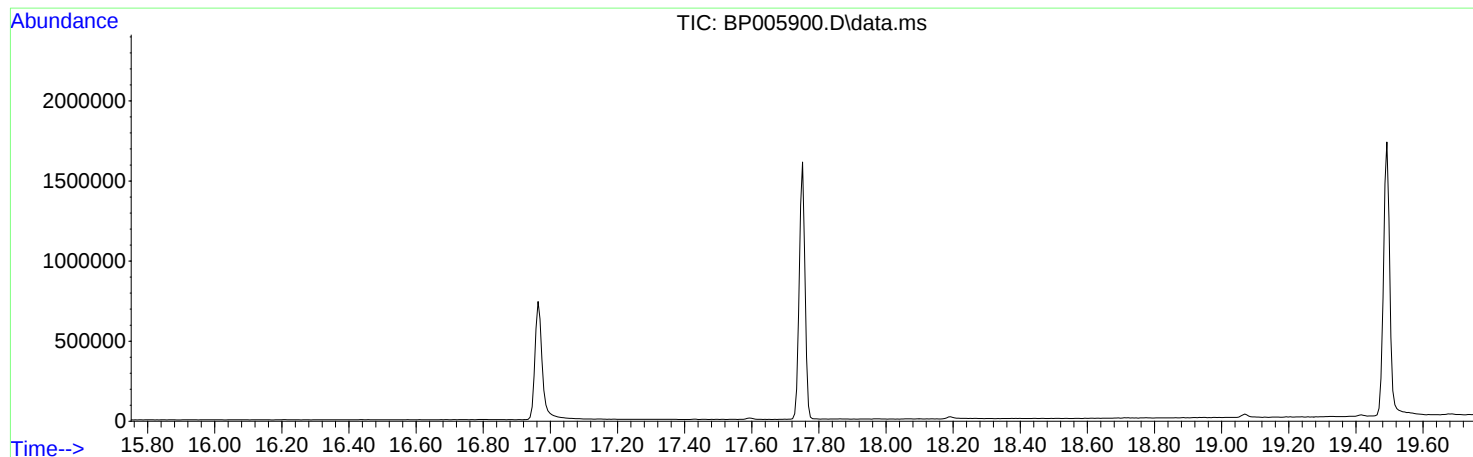




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.5	32113	PASS
68	69	0.00	2	1.9	795	PASS
69	198	0.00	100	33.4	42048	PASS
70	69	0.00	2	0.5	230	PASS
127	198	10	80	44.1	55493	PASS
197	198	0.00	2	0.1	156	PASS
198	198	100	100	100.0	125737	PASS
199	198	5	9	6.9	8733	PASS
275	198	10	60	31.9	40107	PASS
365	198	1	100	5.9	7438	PASS
441	198	0.01	100	29.2	36701	PASS
442	442	100	100	100.0	241699	PASS
443	442	15	24	19.2	46371	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061421\
 Data File : BP005900.D
 Acq On : 14 Jun 2021 11:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 14 13:10:08 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 11 13:53:36 2021
 Response via : Initial Calibration

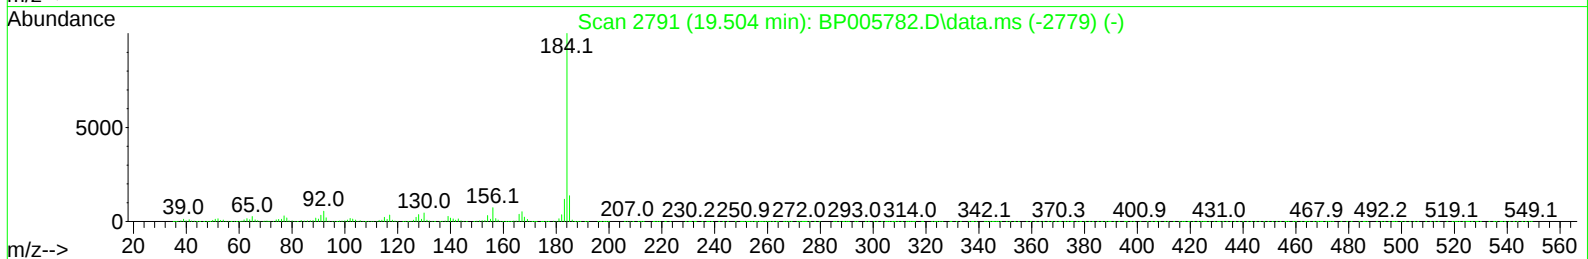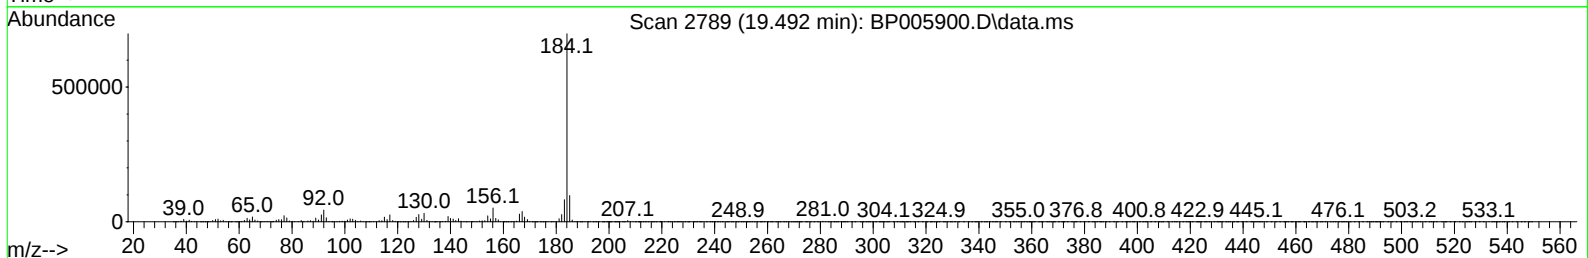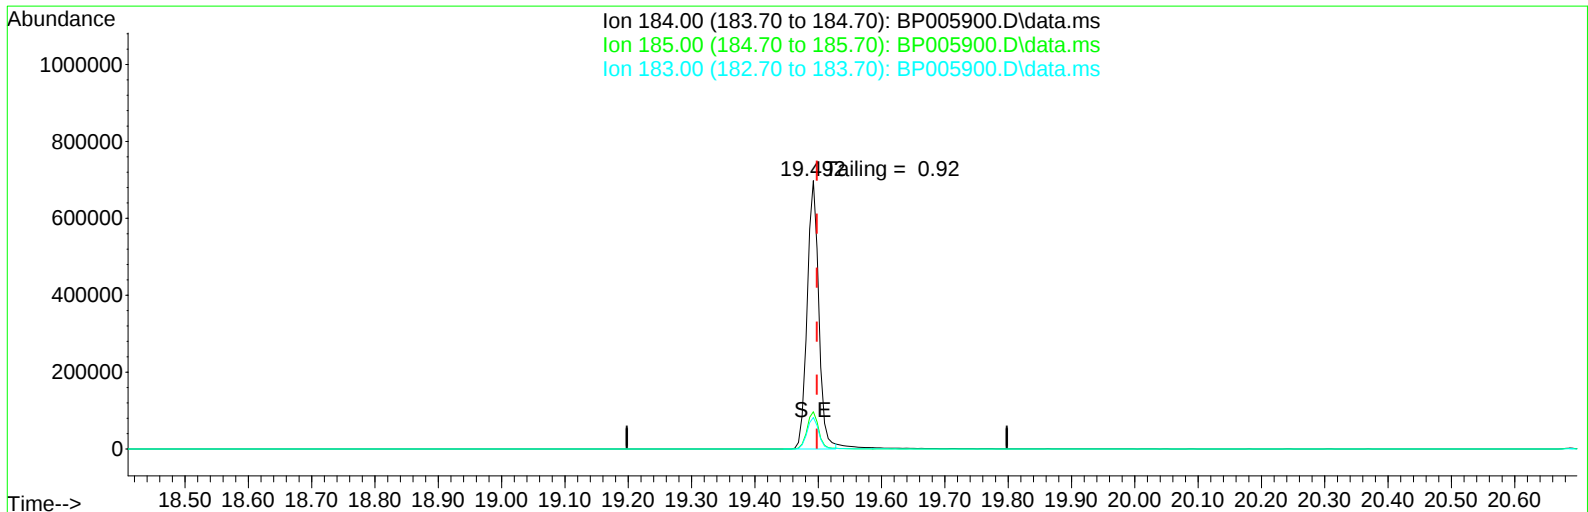

TIC: BP005900.D\data.ms

(77) Benzidine

19.492min (-0.006) 293731.88 ng




response 922908

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.93
183.00	11.90	11.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061421\
 Data File : BP005900.D
 Acq On : 14 Jun 2021 11:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 14 13:10:08 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 11 13:53:36 2021
 Response via : Initial Calibration

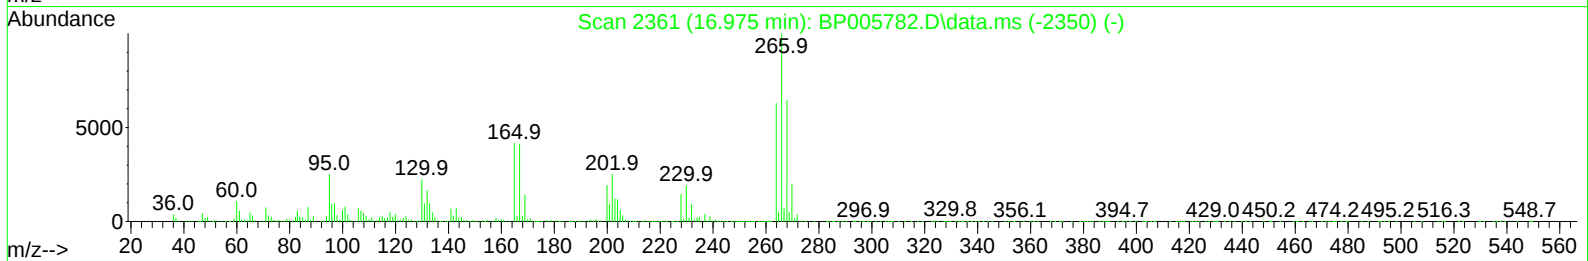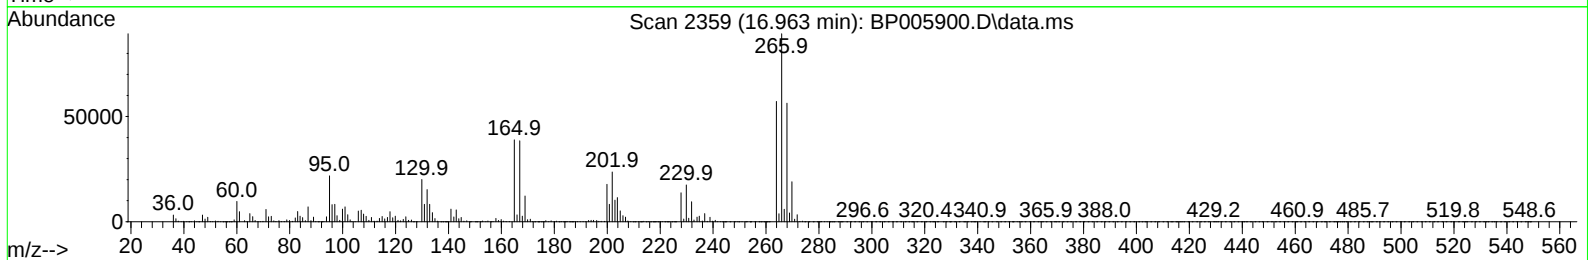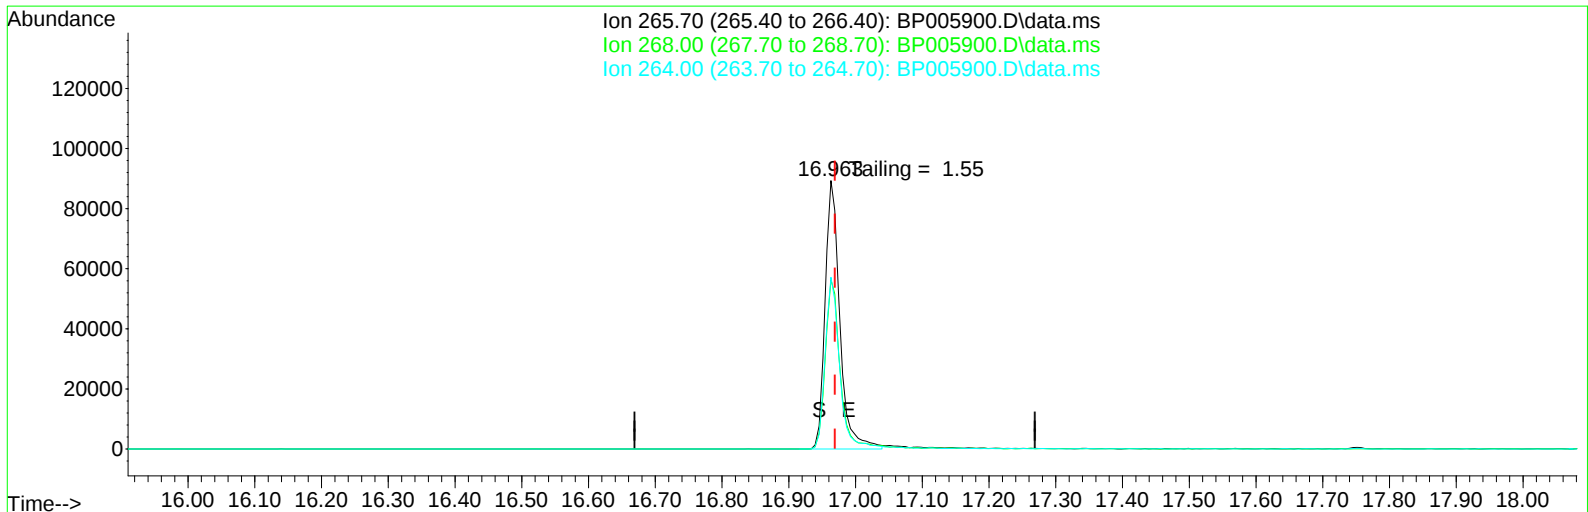

TIC: BP005900.D\data.ms

(70) Pentachlorophenol (C)

16.963min (-0.006) 651080.16 ng

response 139240

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.06
264.00	62.90	63.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/14/2021	BNA_P	BP005900.D
Compound Name	Response	Retention Time
DDT	520652	20.68
DDD	4257	20.26
DDE	1543	19.76
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5800	526452	1.10