
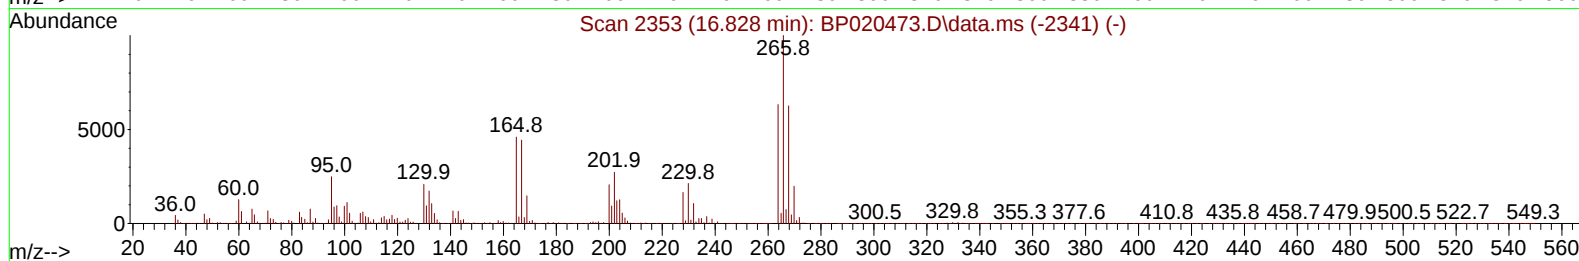
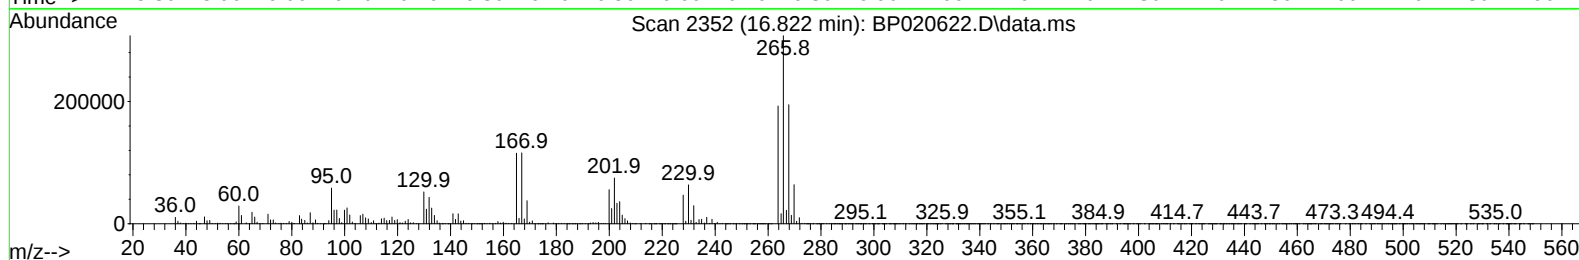


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061424\
Data File : BP020622.D
Acq On : 14 Jun 2024 11:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 12:17:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

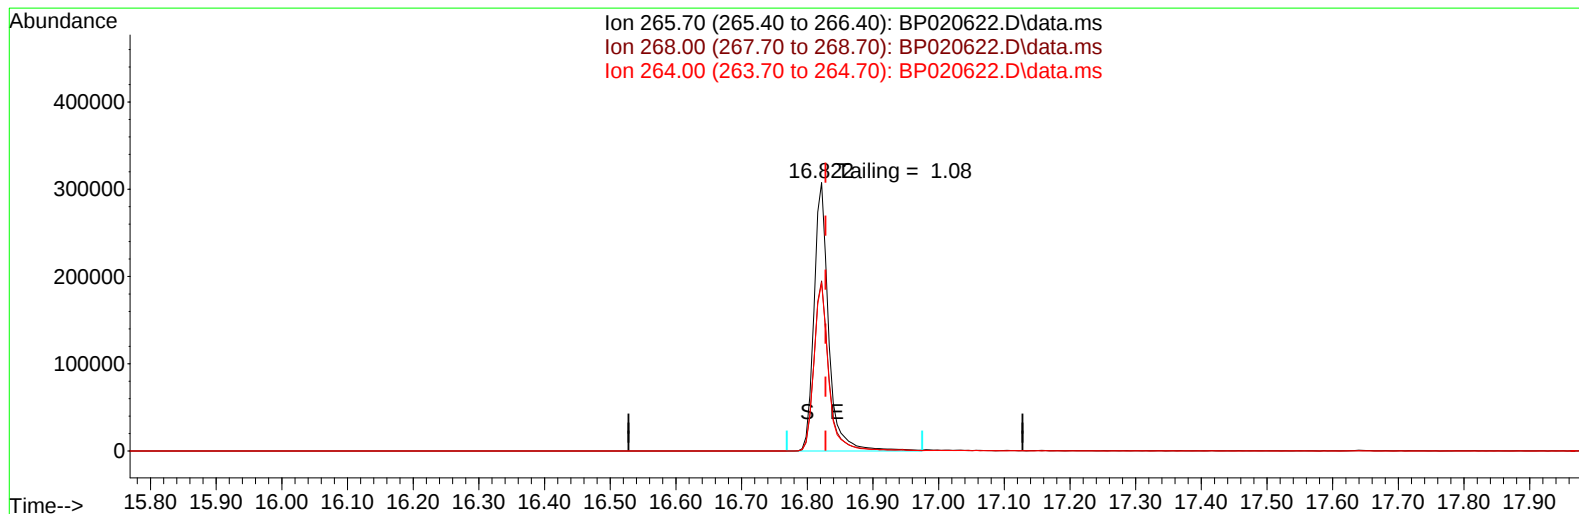

TIC: BP020622.D\data.ms

(70) Pentachlorophenol (C)




16.822min (-0.006) 1522180.97 ng

response 478647

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.36
264.00	63.30	62.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061424\
Data File : BP020622.D
Acq On : 14 Jun 2024 11:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 12:17:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

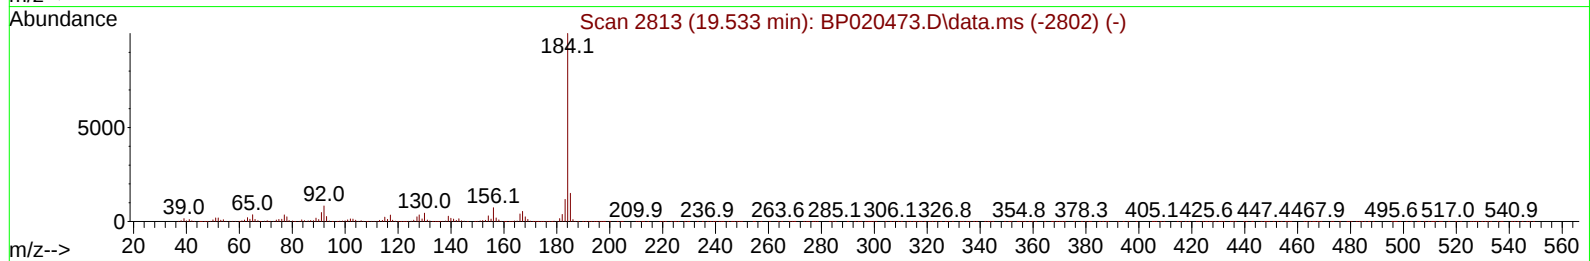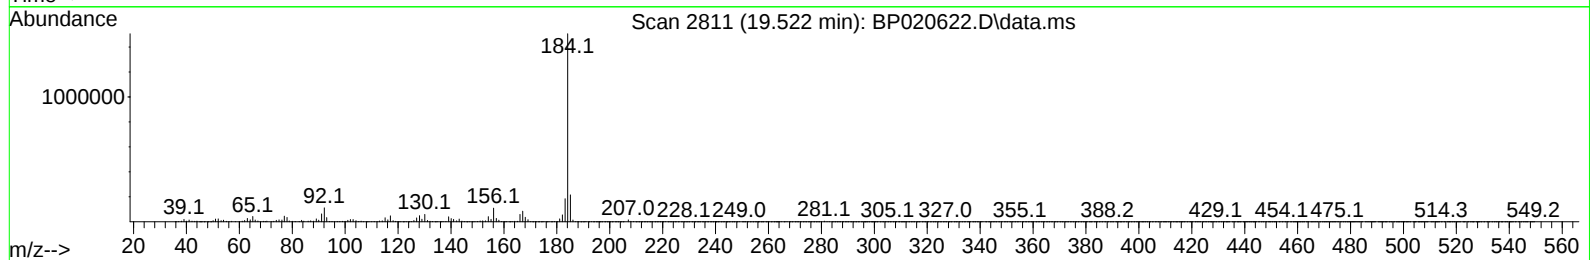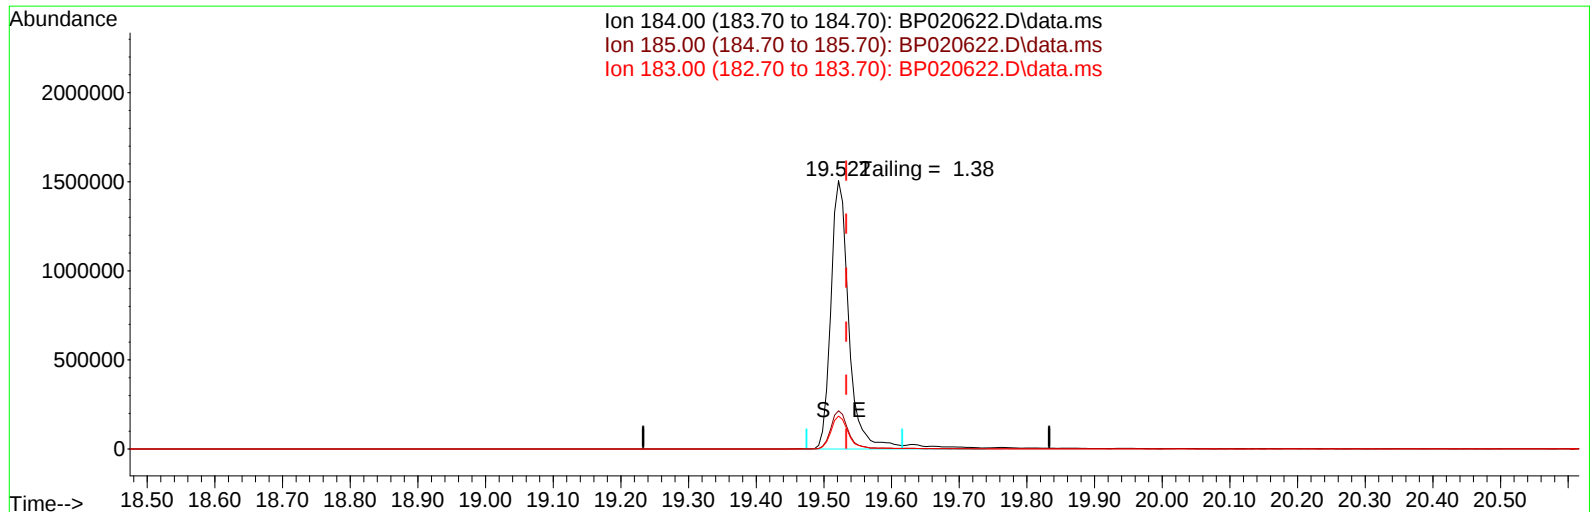

TIC: BP020622.D\data.ms

(77) Benzidine

19.522min (-0.011) 147316.10 ng

response 2757309

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.27
183.00	11.70	12.30
0.00	0.00	0.00