


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061424\
Data File : BP020622.D
Acq On : 14 Jun 2024 11:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 30 03:41:03 2024

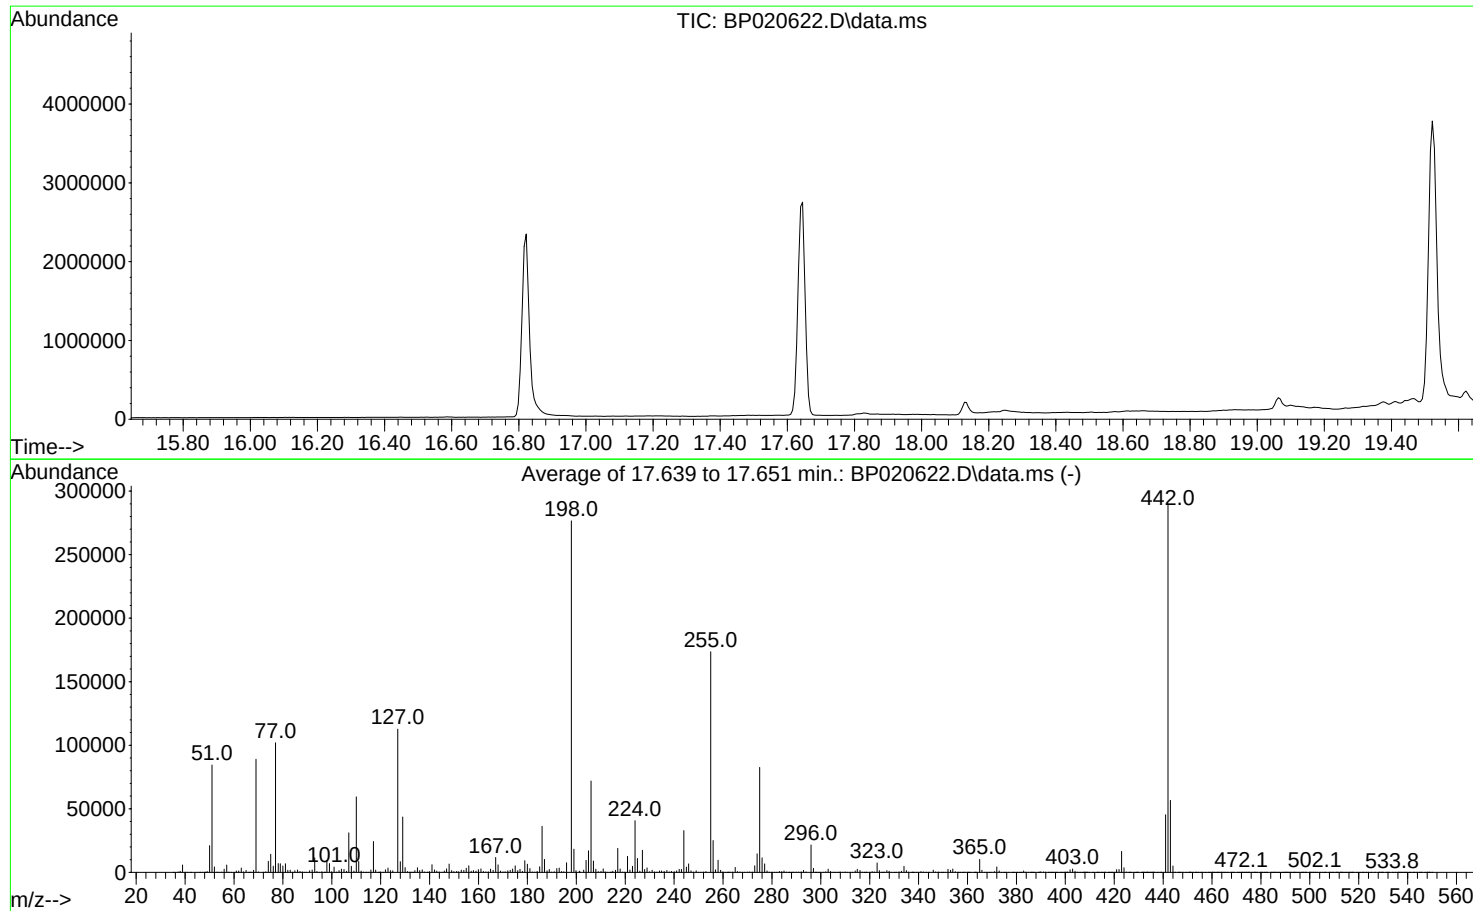


AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	84434	PASS
68	69	0.00	2	1.8	1611	PASS
69	198	0.00	100	32.2	88992	PASS
70	69	0.00	2	0.5	407	PASS
127	198	10	80	40.8	112714	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	276544	PASS
199	198	5	9	6.6	18281	PASS
275	198	10	60	29.9	82641	PASS
365	198	1	100	3.7	10224	PASS
441	198	0.01	100	16.4	45373	PASS
442	442	100	100	100.0	289458	PASS
443	442	15	24	19.6	56725	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061424\
Data File : BP020622.D
Acq On : 14 Jun 2024 11:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 14 12:17:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

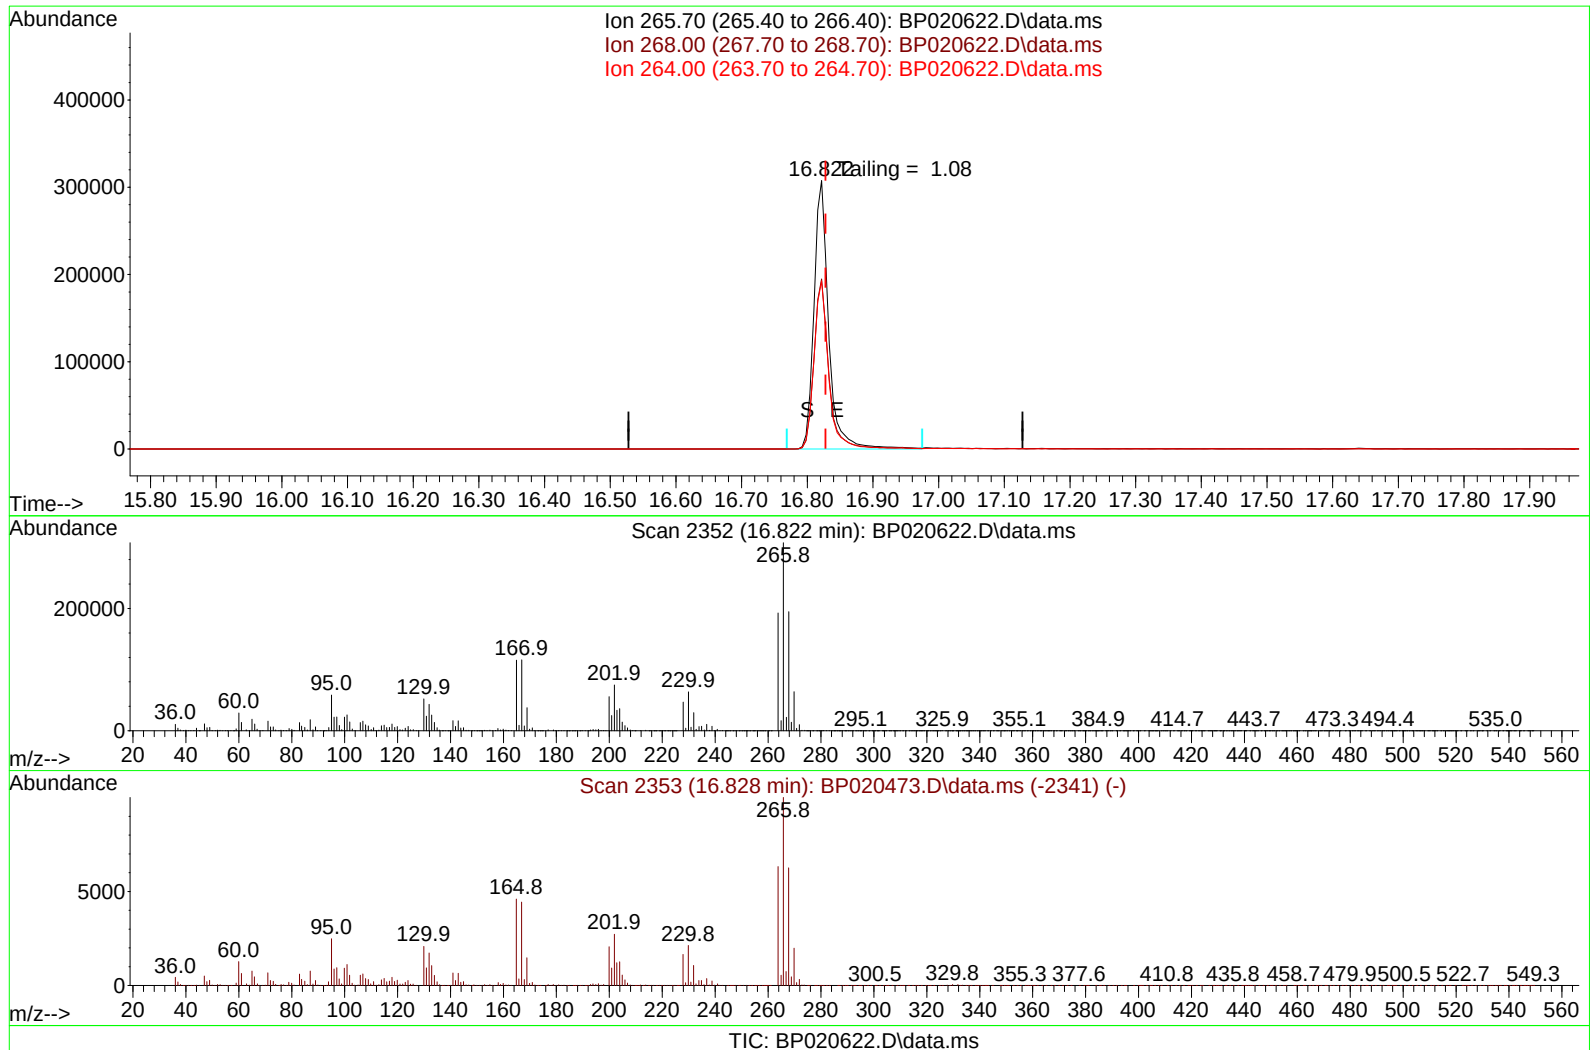

TIC: BP020622.D\data.ms

(70) Pentachlorophenol (C)

16.822min (-0.006) 1522180.97 ng




response 478647

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.36
264.00	63.30	62.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061424\
Data File : BP020622.D
Acq On : 14 Jun 2024 11:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 14 12:17:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

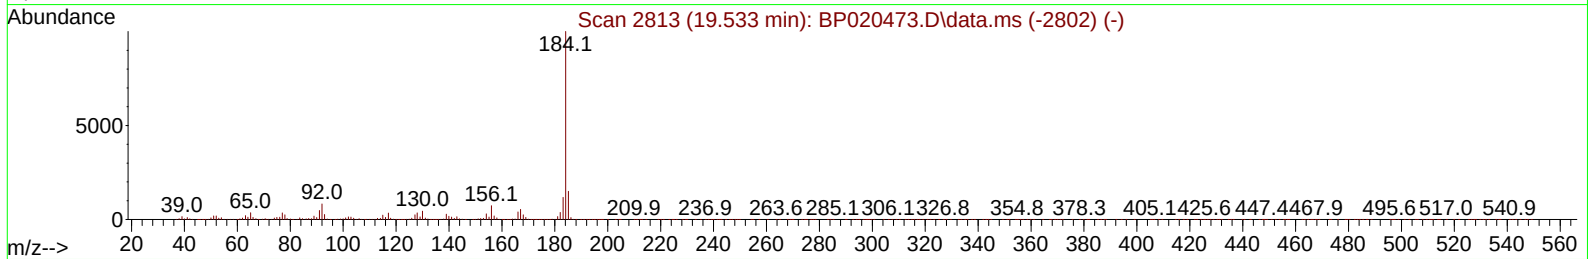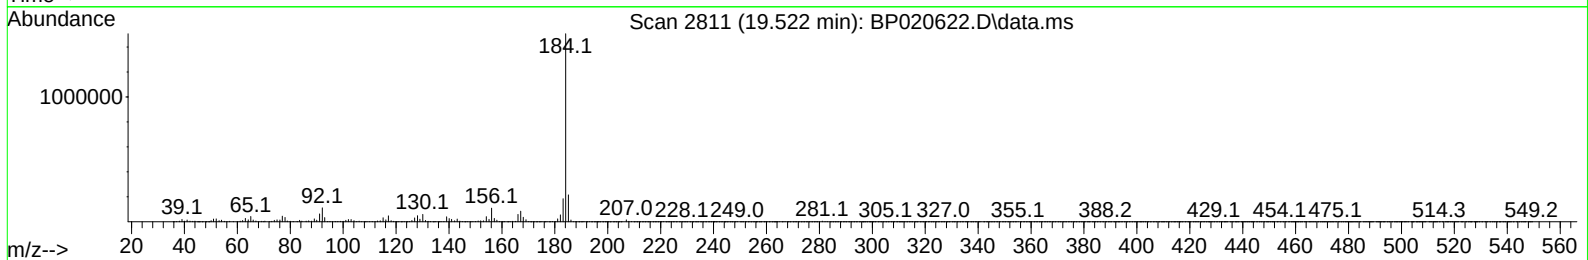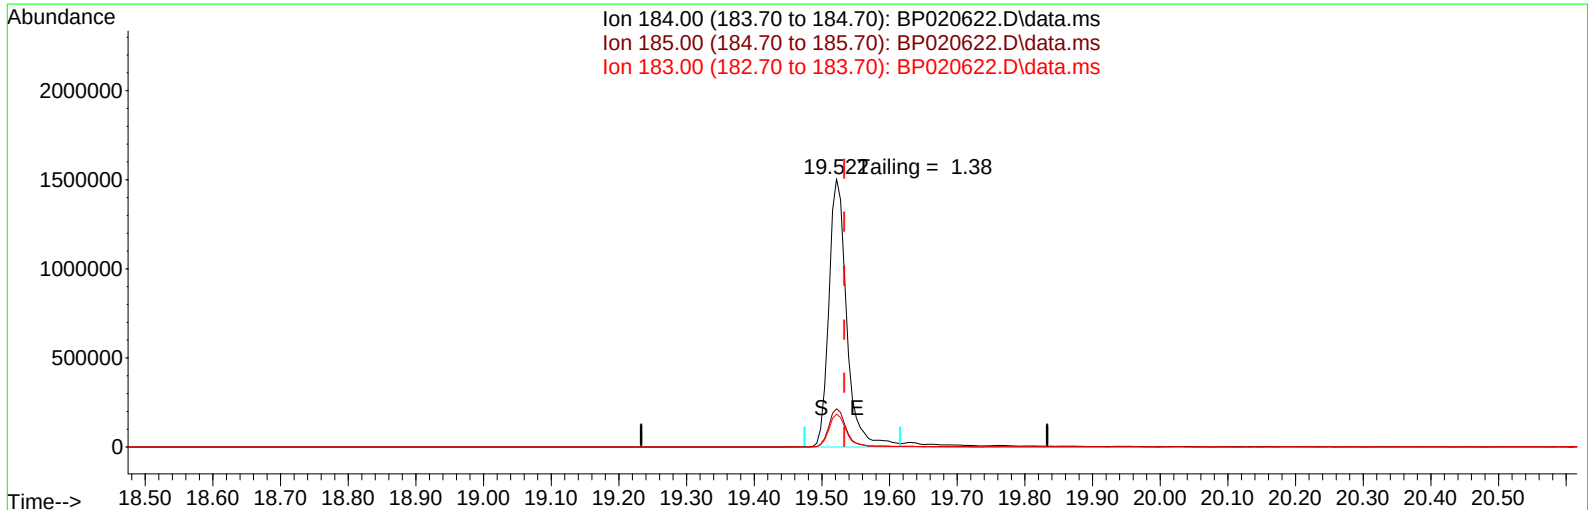

TIC: BP020622.D\data.ms

(77) Benzidine

19.522min (-0.011) 147316.10 ng

response 2757309

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.27
183.00	11.70	12.30
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/14/2024	BNA_P	<u>BP020622.D</u>
Compound Name	Response	Retention Time
DDT	1232780	20.816
DDD	23360	20.41
DDE	3137	19.822
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26497	1259277	2.10

Instrument :
BNA_P
ClientSampleId :
DFTPP