
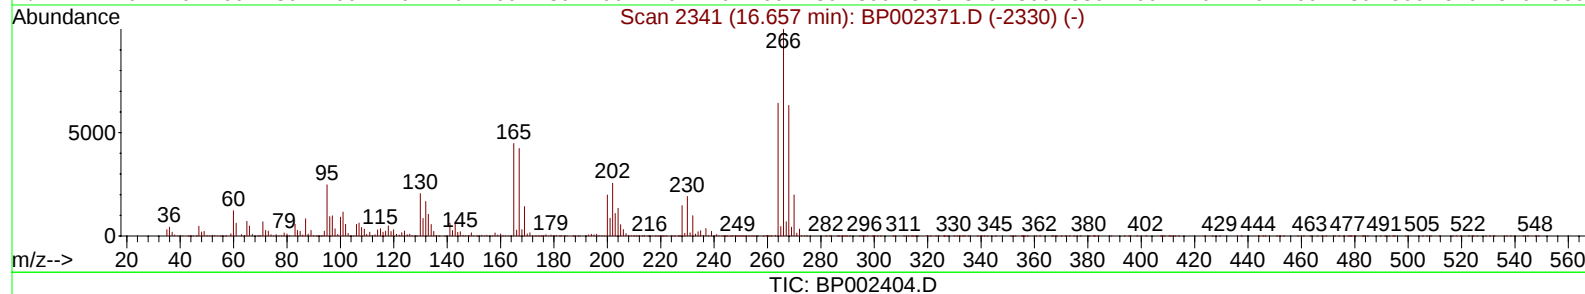
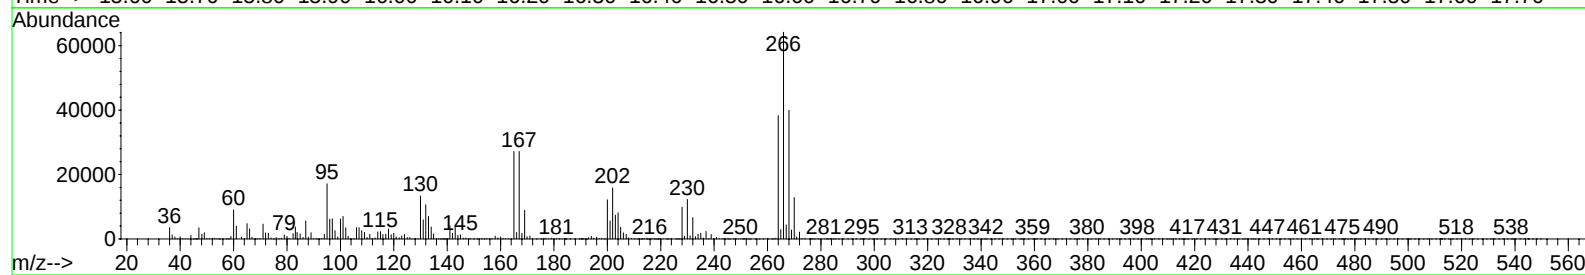


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061520\
Data File : BP002404.D
Acq On : 15 Jun 2020 09:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 17:28:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 15:08:53 2020
Response via : Initial Calibration

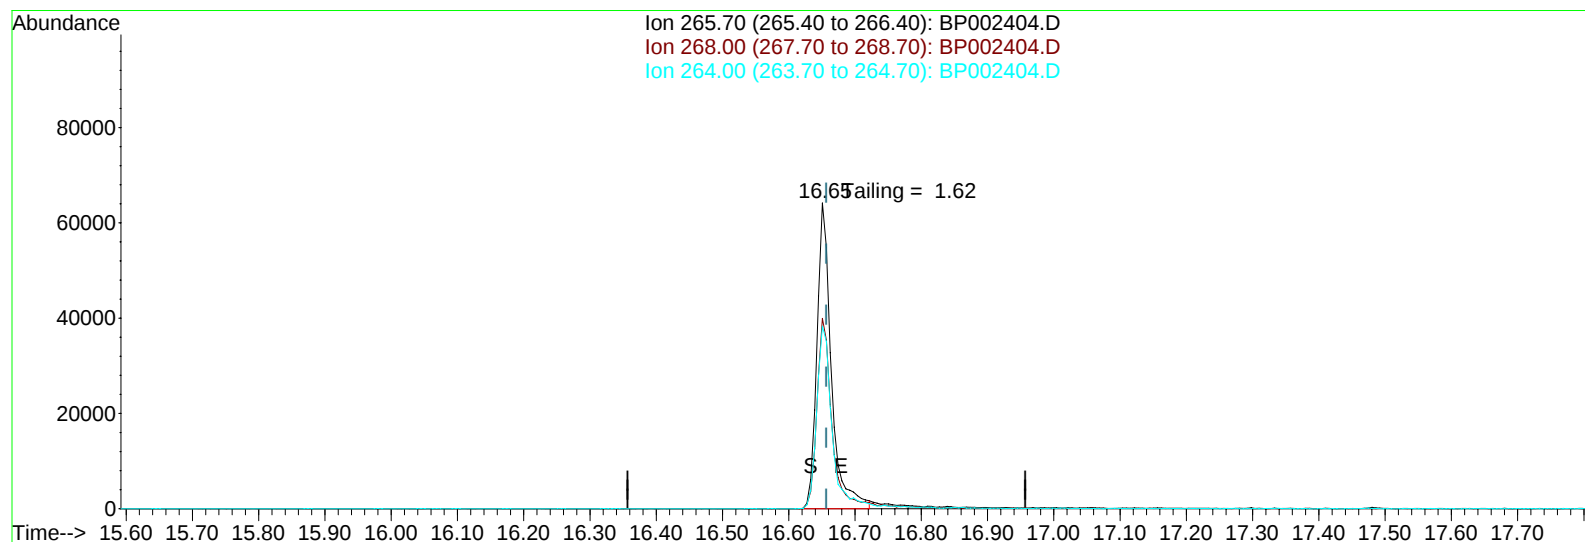

(70) Pentachlorophenol (C)




16.651min (-0.006) 16833.22ng

response 101540

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	62.26
264.00	64.20	59.71
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061520\
 Data File : BP002404.D
 Acq On : 15 Jun 2020 09:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 17:28:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 15:08:53 2020
 Response via : Initial Calibration

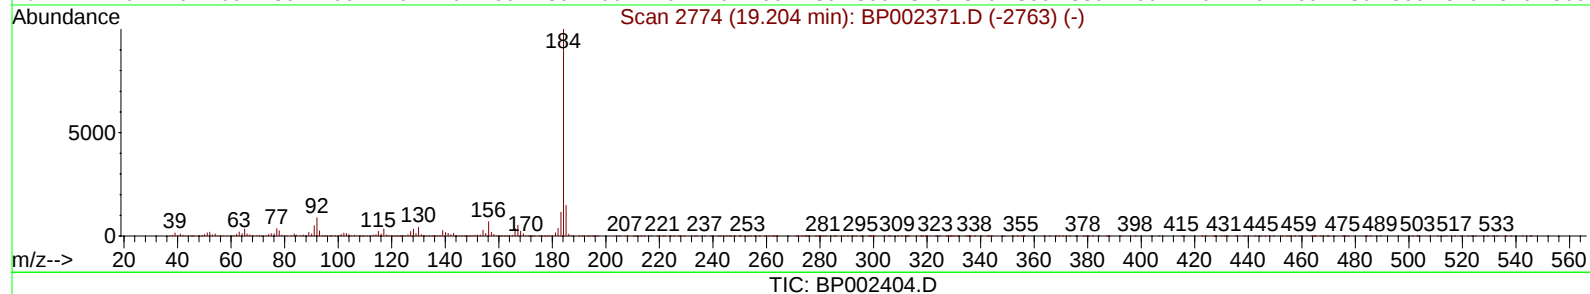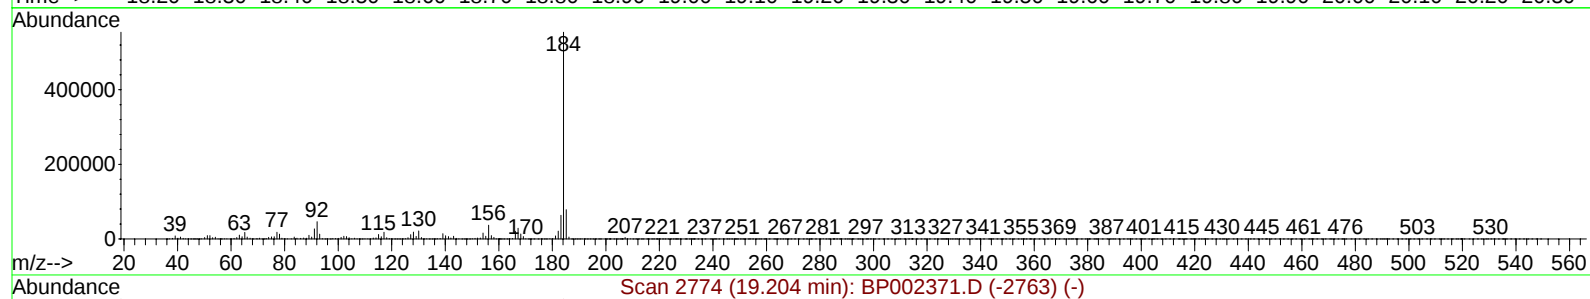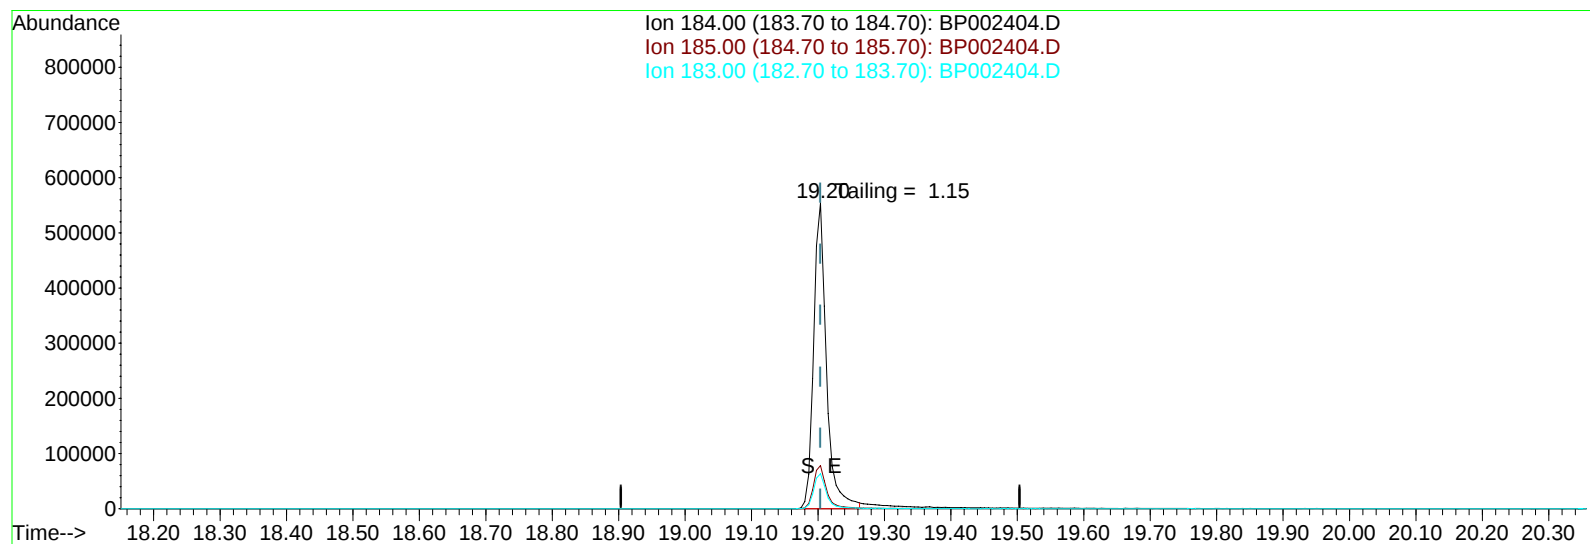

TIC: BP002404.D

(77) Benzidine

19.204min (+0.000) 35382.51ng

response 776392

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.15
183.00	11.50	11.47
0.00	0.00	0.00