

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061520\
Data File : BP002408.D
Acq On : 15 Jun 2020 14:31
Operator : CG/JU
Sample : PB129539BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129539BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.205	388	394	410	rBV	3041190	4637603	44.10%	8.632%
2	6.781	654	662	682	rBV	3041500	4924227	46.82%	9.166%
3	7.593	792	800	813	rBV	697477	1108071	10.54%	2.062%
4	7.910	846	854	865	rBV	2620878	4265454	40.56%	7.939%
5	8.734	986	994	1020	rBV	2043984	3451078	32.82%	6.424%
6	10.363	1263	1271	1289	rBV	906048	1571535	14.94%	2.925%
7	12.857	1686	1695	1718	rBV	4532166	7281439	69.24%	13.553%
8	14.240	1923	1930	1947	rBV2	1337224	2096218	19.93%	3.902%
9	15.739	2178	2185	2206	rBV	3561855	5340149	50.78%	9.940%
10	16.998	2392	2399	2413	rBV	1747226	2549328	24.24%	4.745%
11	19.592	2834	2840	2850	rBV	7826798	10516372	100.00%	19.574%
12	21.104	3091	3097	3107	rBV	2288701	2941087	27.97%	5.474%
13	23.304	3464	3471	3486	rVB2	1616687	3042627	28.93%	5.663%




Sum of corrected areas: 53725188

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061520\
Data File : BP002408.D
Acq On : 15 Jun 2020 14:31
Operator : CG/JU
Sample : PB129539BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129539BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

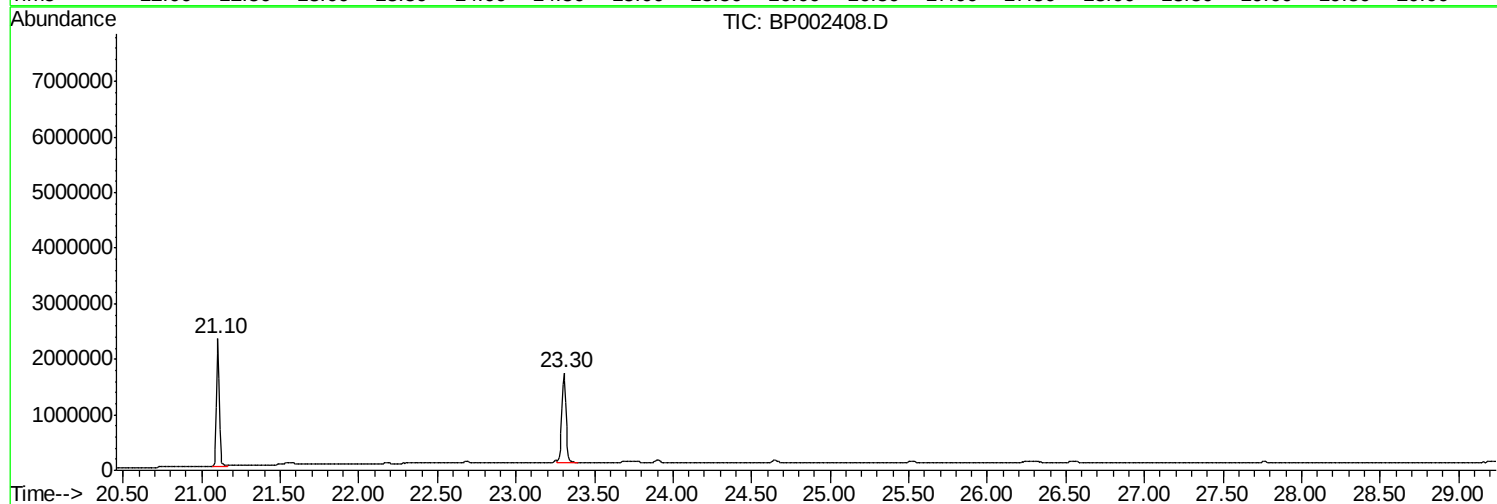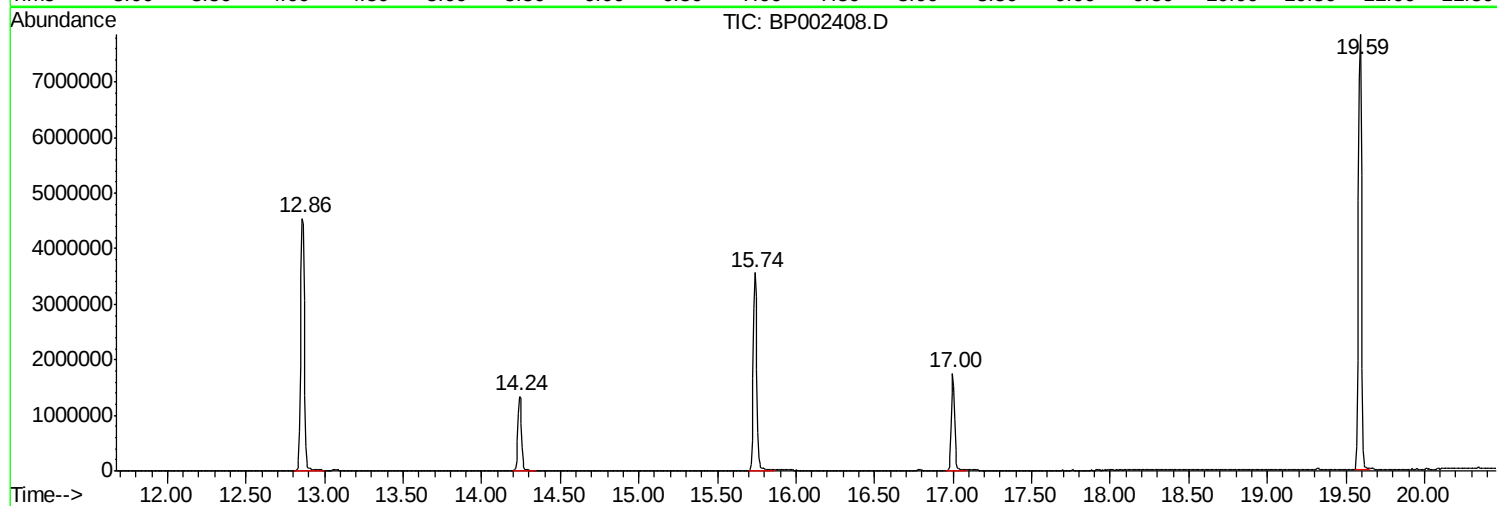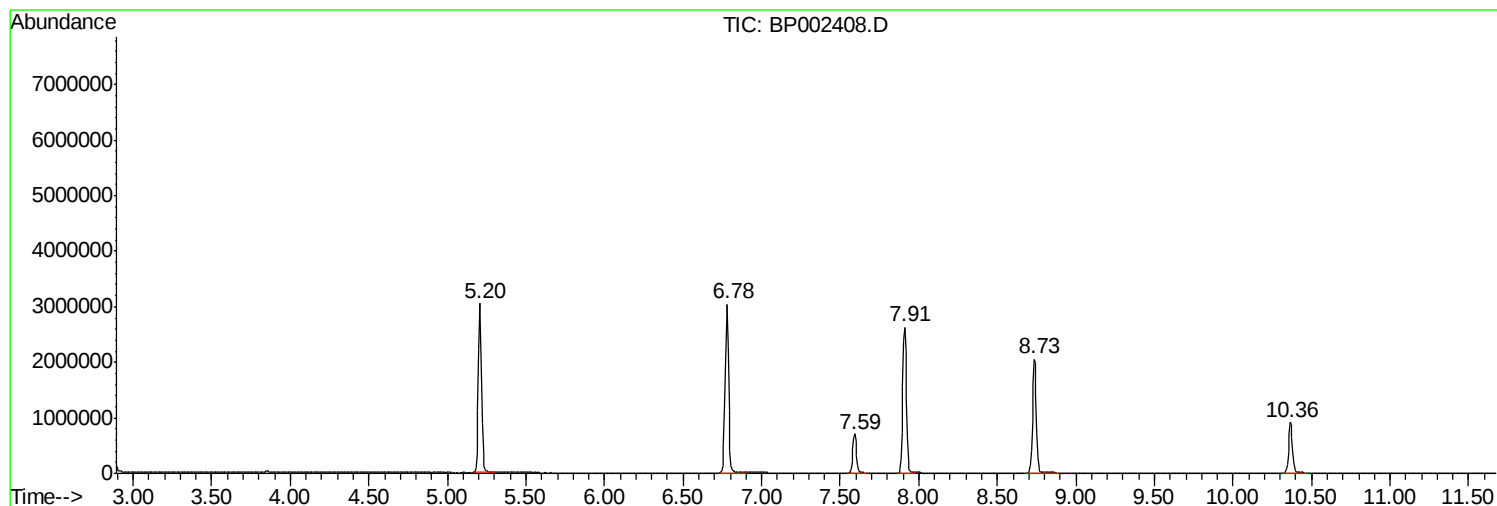

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP061520\
Data File : BP002408.D
Acq On : 15 Jun 2020 14:31
Operator : CG/JU
Sample : PB129539BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129539BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP061520\
Data File : BP002408.D
Acq On : 15 Jun 2020 14:31
Operator : CG/JU
Sample : PB129539BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129539BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc