


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061520\
 Data File : BP002404.D
 Acq On : 15 Jun 2020 09:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 05 15:08:53 2020

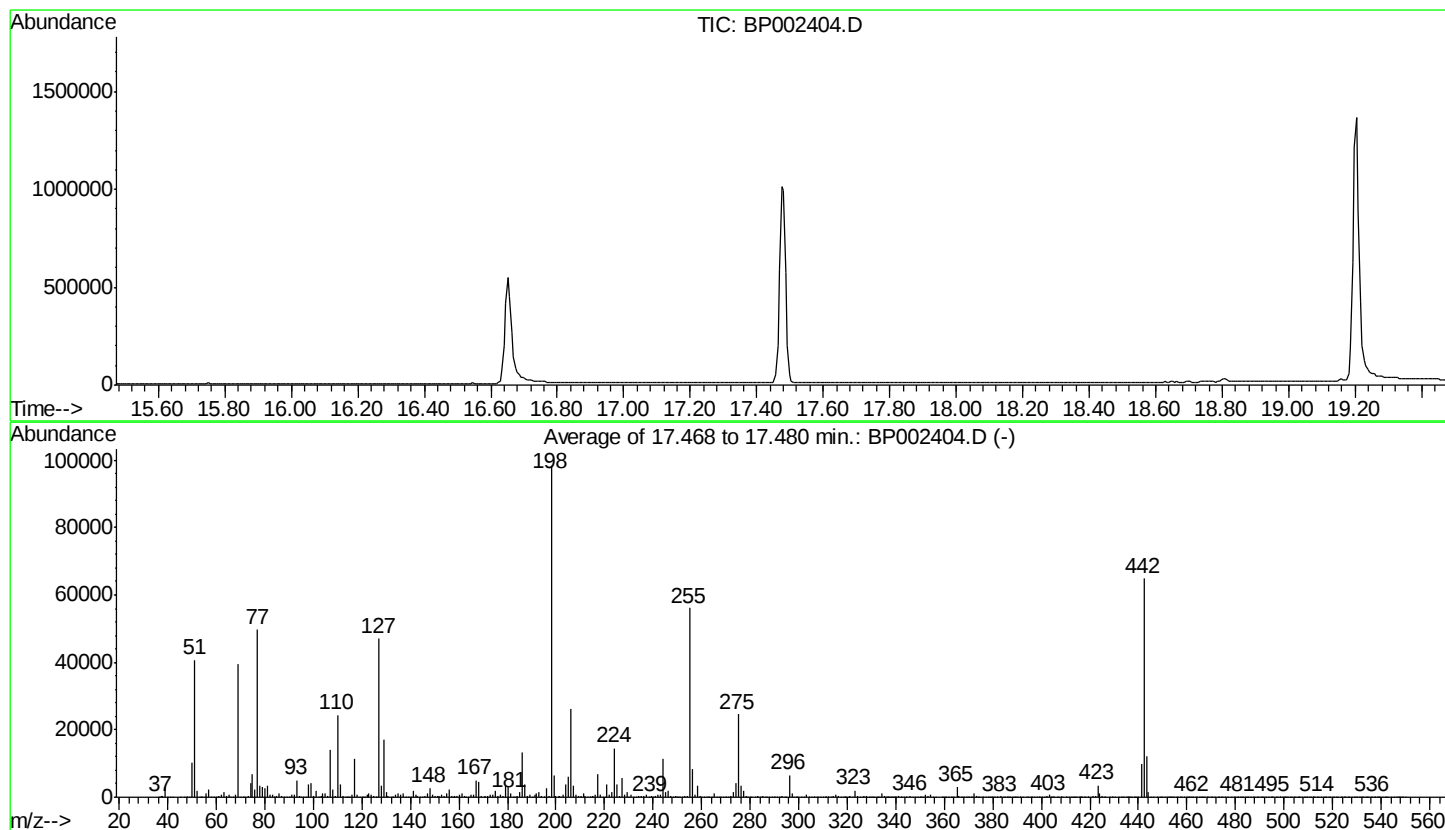

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	40645	PASS
68	69	0.00	2	1.8	716	PASS
69	198	0.00	100	40.0	39378	PASS
70	69	0.00	2	0.5	202	PASS
127	198	10	80	47.7	46933	PASS
197	198	0.00	2	0.4	370	PASS
198	198	100	100	100.0	98335	PASS
199	198	5	9	6.7	6589	PASS
275	198	10	60	25.0	24577	PASS
365	198	1	100	3.1	3067	PASS
441	198	0.01	100	10.0	9804	PASS
442	198	50	100	65.9	64764	PASS
443	442	15	24	18.9	12243	PASS