
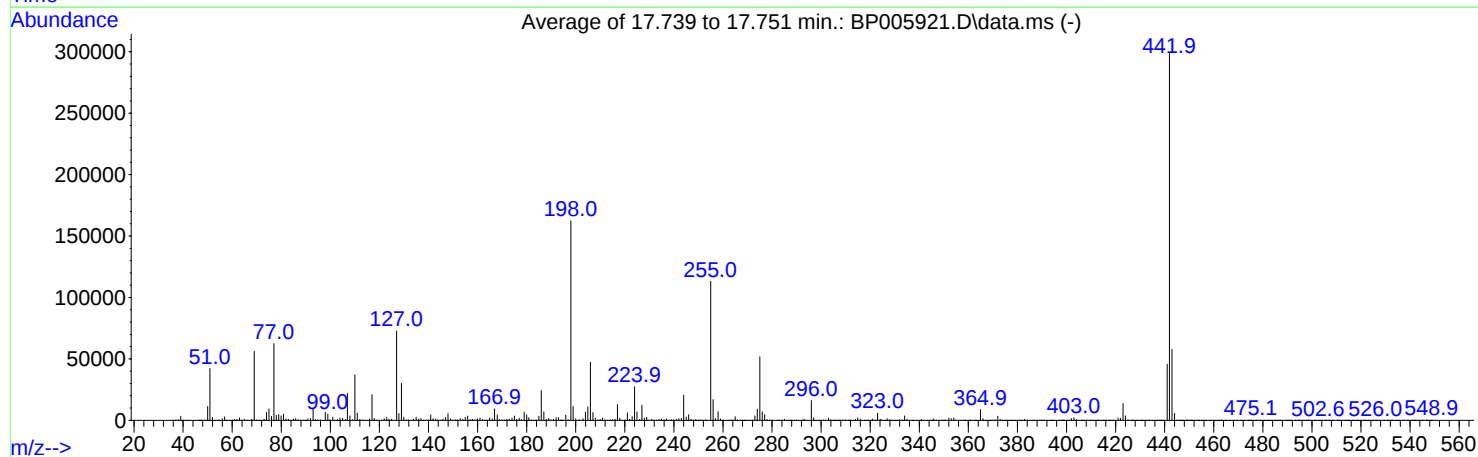


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061521\
 Data File : BP005921.D
 Acq On : 15 Jun 2021 09:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 16 11:35:30 2021

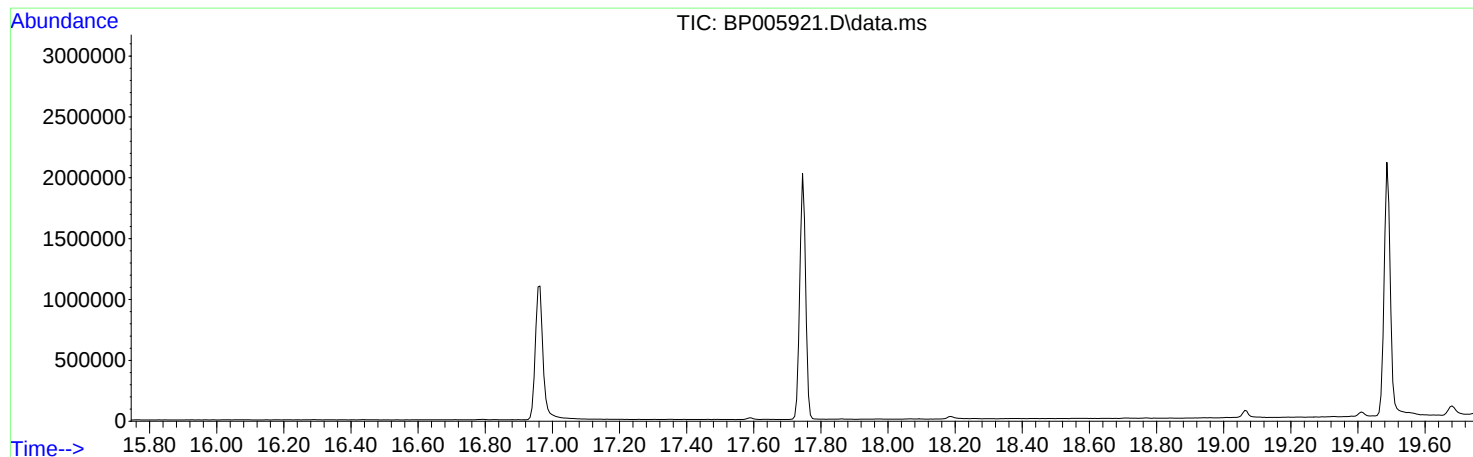




AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.0	42207	PASS
68	69	0.00	2	1.2	690	PASS
69	198	0.00	100	34.6	56222	PASS
70	69	0.00	2	0.7	373	PASS
127	198	10	80	44.7	72679	PASS
197	198	0.00	2	0.2	393	PASS
198	198	100	100	100.0	162423	PASS
199	198	5	9	7.0	11407	PASS
275	198	10	60	31.9	51768	PASS
365	198	1	100	5.4	8711	PASS
441	198	0.01	100	28.1	45704	PASS
442	442	100	100	100.0	299405	PASS
443	442	15	24	19.3	57824	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061521\
Data File : BP005921.D
Acq On : 15 Jun 2021 09:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 15 11:26:26 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 14 13:15:03 2021
Response via : Initial Calibration

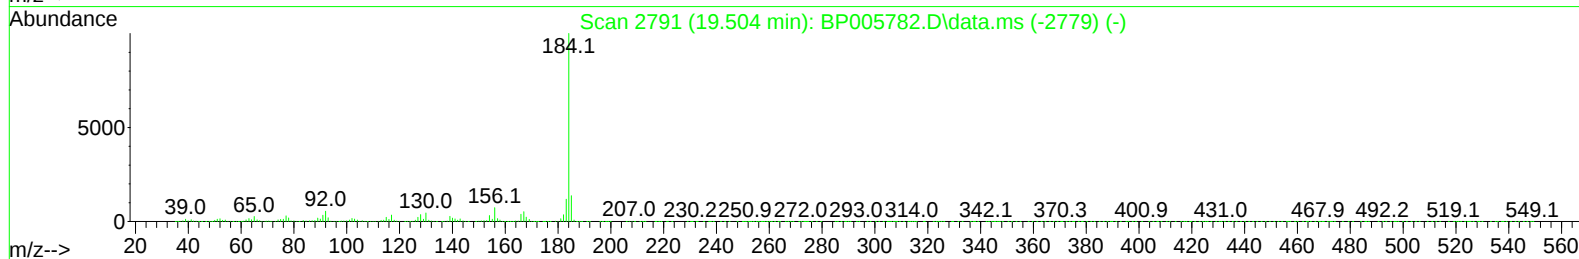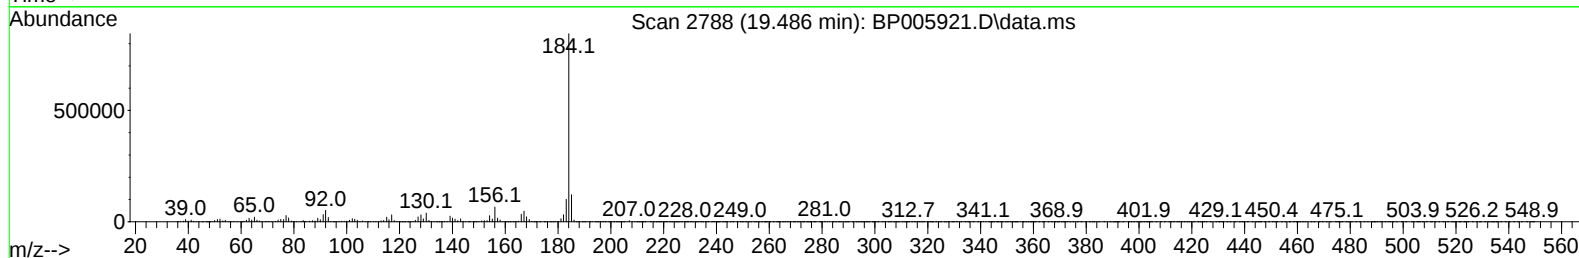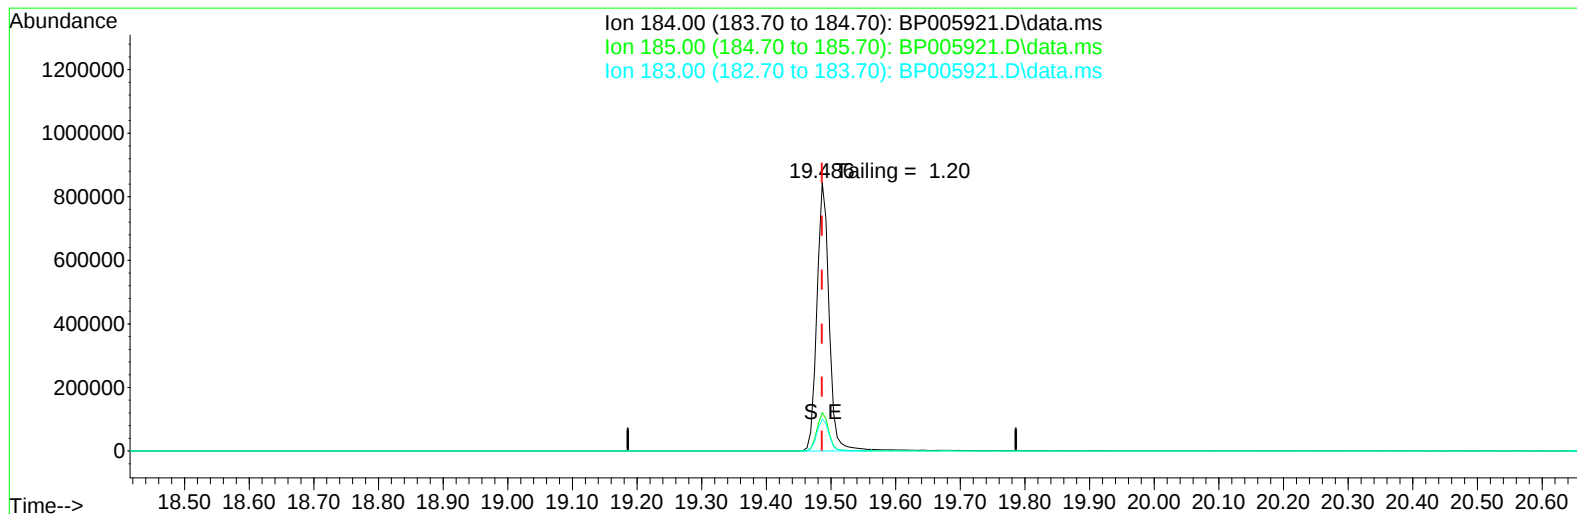

TIC: BP005921.D\data.ms

(77) Benzidine

19.486min (+ 0.000) 32347.05 ng




response 1120674

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.35
183.00	11.90	11.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061521\
 Data File : BP005921.D
 Acq On : 15 Jun 2021 09:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 15 11:26:26 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 14 13:15:03 2021
 Response via : Initial Calibration

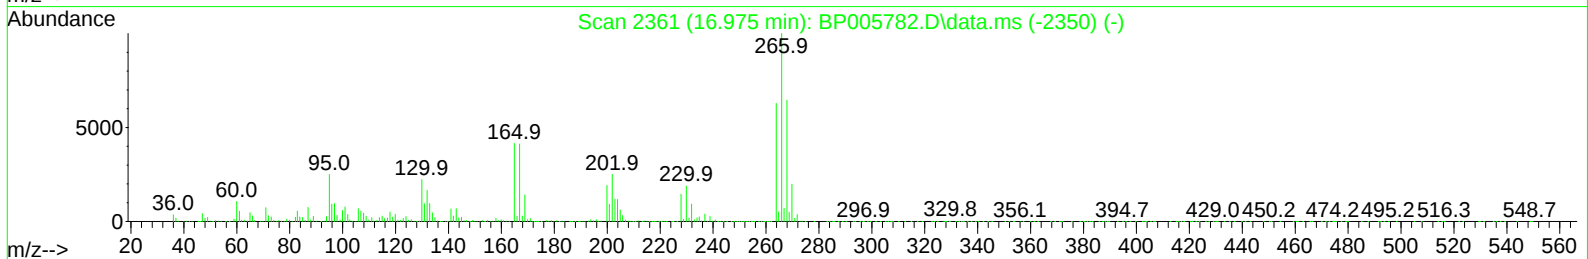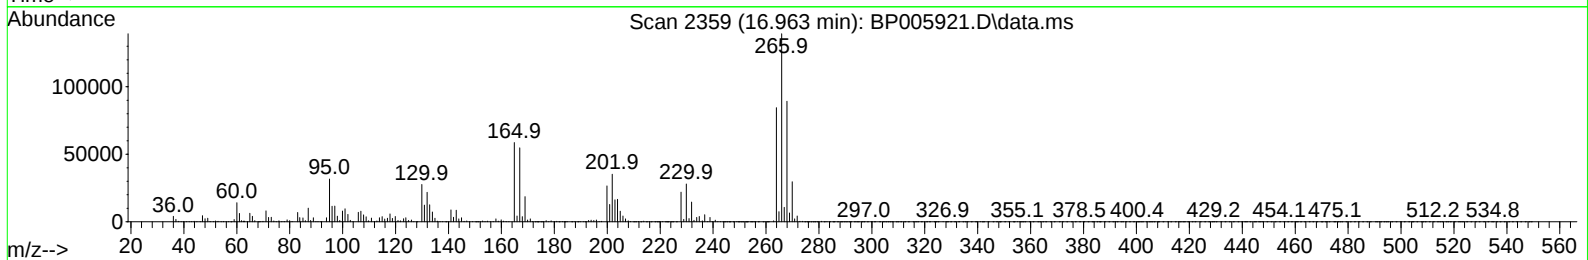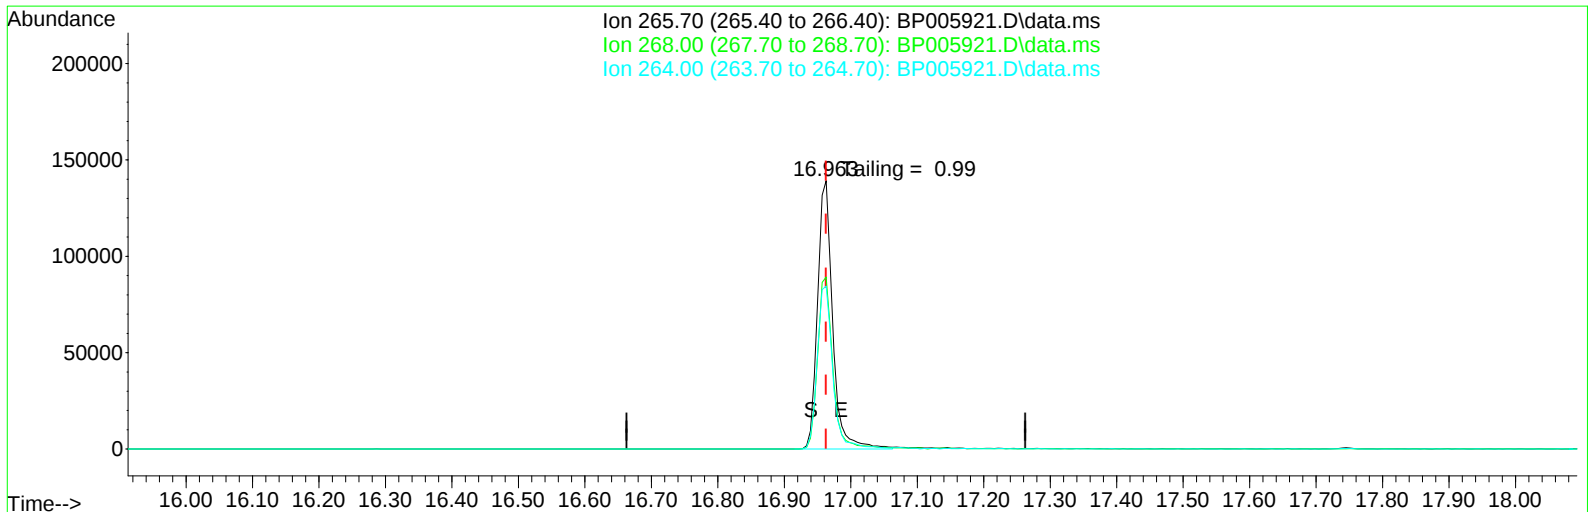

TIC: BP005921.D\data.ms

(70) Pentachlorophenol (C)

16.963min (+ 0.000) 148743.11 ng

response 221399

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.13
264.00	62.90	60.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/15/2021	BNA_P	BP005921.D
Compound Name	Response	Retention Time
DDT	709686	20.68
DDD	10720	20.25
DDE	2461	19.76
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13181	722867	1.82