
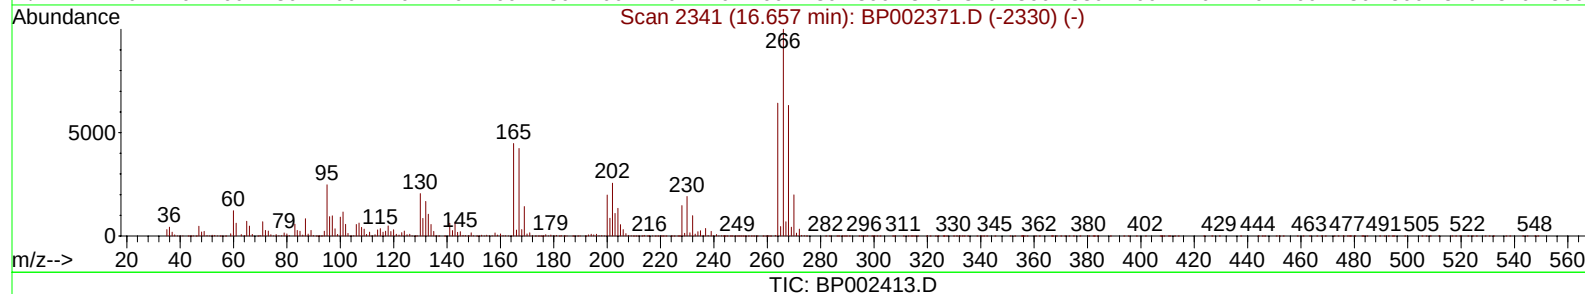
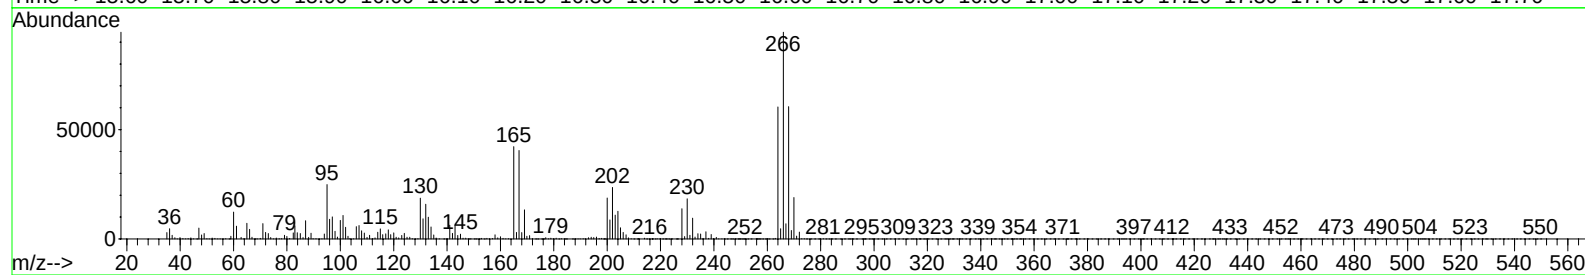


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061620\
 Data File : BP002413.D
 Acq On : 16 Jun 2020 07:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 17:48:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 15:08:53 2020
 Response via : Initial Calibration

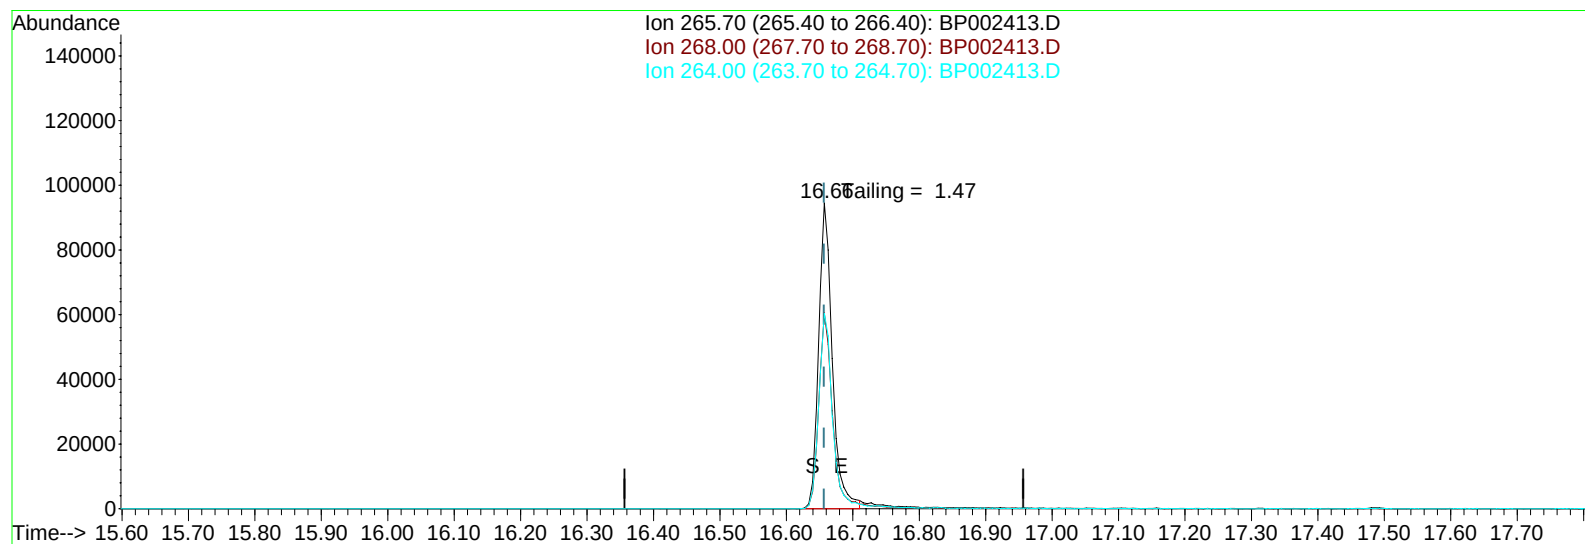

(70) Pentachlorophenol (C)




16.657min (+0.000) 109190.85ng

response 140530

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	63.98
264.00	64.20	63.89
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061620\
 Data File : BP002413.D
 Acq On : 16 Jun 2020 07:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 17:48:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 15:08:53 2020
 Response via : Initial Calibration

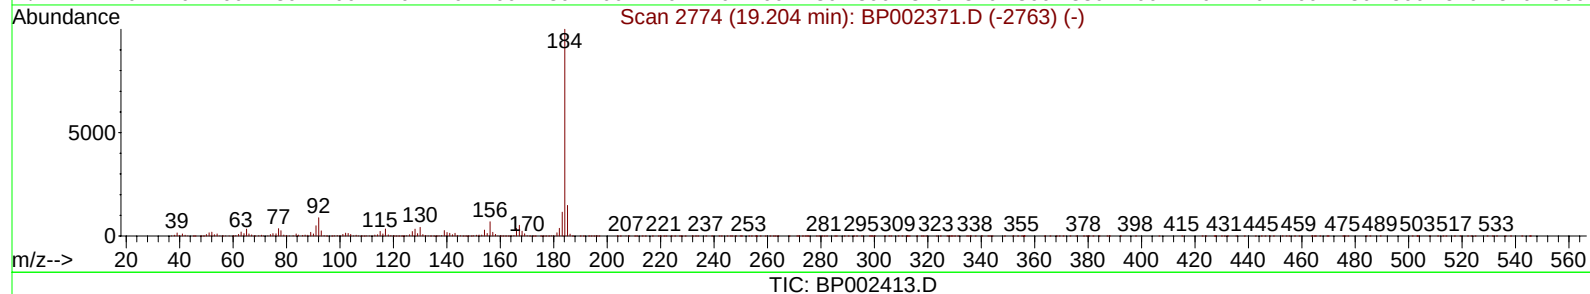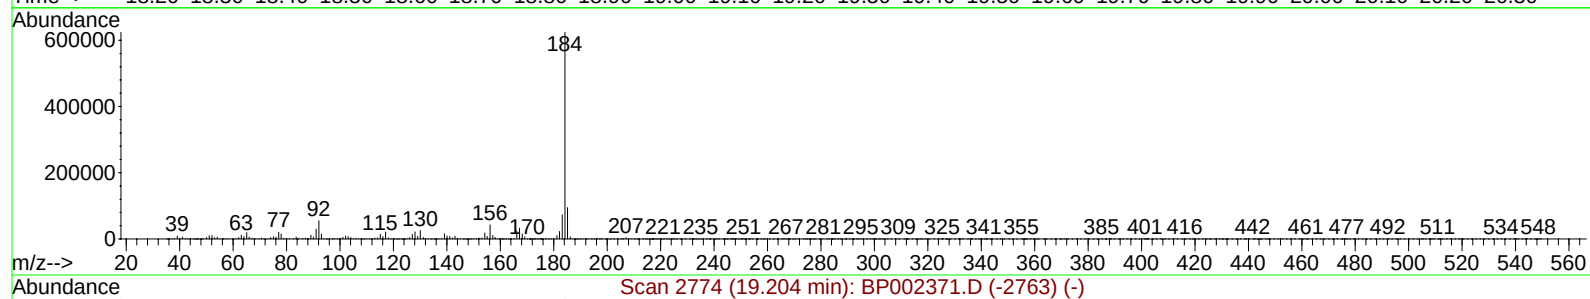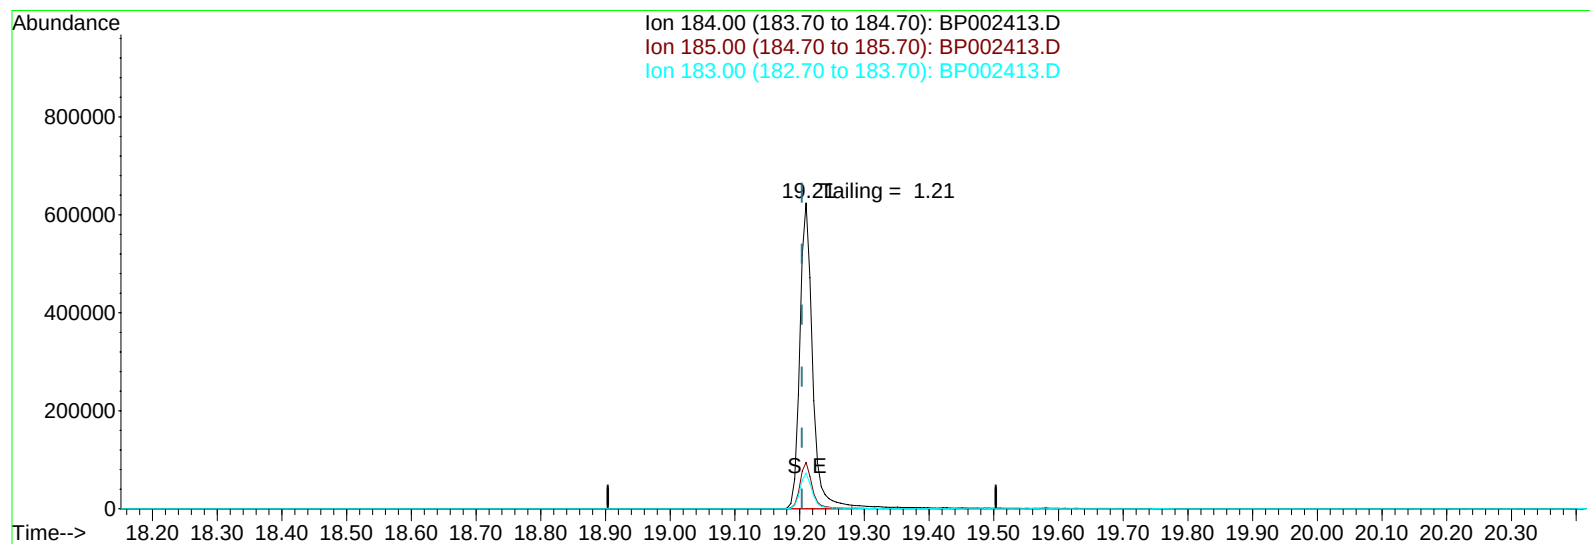

(77) Benzidine

19.210min (+0.006) 2966.19ng

response 871379

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	15.16
183.00	11.50	11.69
0.00	0.00	0.00