

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP061620\
 Data File : BP002415.D
 Acq On : 16 Jun 2020 15:02
 Operator : CG/JU
 Sample : PB129581BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB129581BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.205	387	394	417	rBV	3083413	4694642	44.73%	8.563%
2	6.775	653	661	683	rBV	2982241	4955536	47.21%	9.039%
3	7.593	792	800	810	rBV	709803	1116805	10.64%	2.037%
4	7.910	846	854	872	rBV	2644725	4332793	41.28%	7.903%
5	8.734	985	994	1015	rBV	2054151	3476231	33.12%	6.341%
6	10.363	1263	1271	1289	rBV	899041	1571258	14.97%	2.866%
7	12.857	1687	1695	1715	rBV	4734704	7393879	70.44%	13.486%
8	14.240	1923	1930	1947	rBV2	1357702	2118300	20.18%	3.864%
9	15.739	2178	2185	2216	rBV	3589507	5465581	52.07%	9.969%
10	16.998	2389	2399	2412	rBV	1779011	2593451	24.71%	4.730%
11	19.592	2834	2840	2857	rBV	8018093	10496289	100.00%	19.145%
12	21.104	3092	3097	3109	rBV	2350261	2965886	28.26%	5.410%
13	21.222	3113	3117	3126	rVV	99295	141547	1.35%	0.258%
14	23.257	3458	3463	3465	rBV	86026	137285	1.31%	0.250%
15	23.304	3465	3471	3481	rVB	1641144	3025611	28.83%	5.519%
16	23.898	3568	3572	3581	rVB	89649	167898	1.60%	0.306%
17	24.651	3695	3700	3710	rVB2	79065	172333	1.64%	0.314%


Sum of corrected areas: 54825325

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061620\
Data File : BP002415.D
Acq On : 16 Jun 2020 15:02
Operator : CG/JU
Sample : PB129581BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129581BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

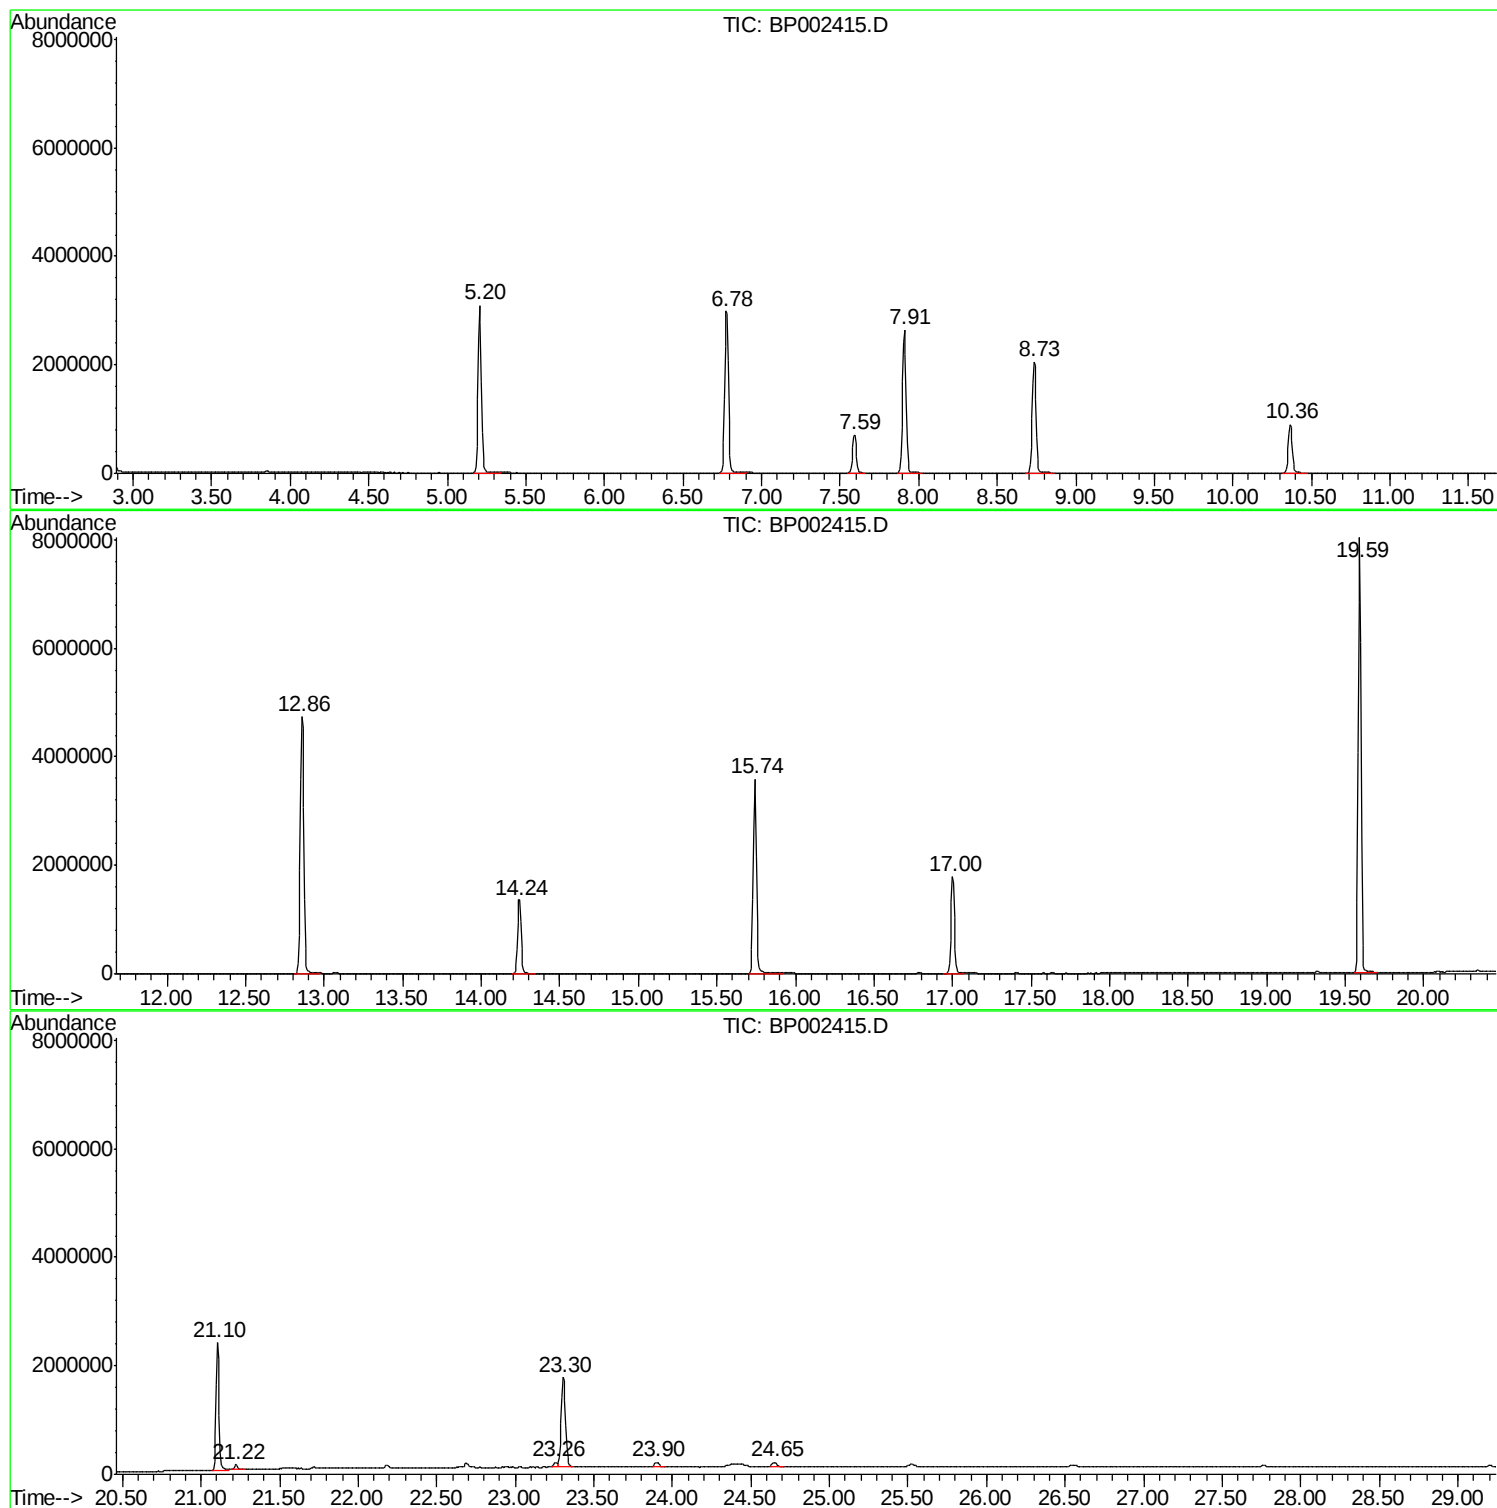

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP061620\
Data_File : BP002415.D
Acq_On : 16 Jun 2020 15:022
Operator : CG/JUU
Sample : PB129581BLL
Misc :
ALS_Vial : 3 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
PB129581BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
