


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061620\
 Data File : BP002413.D
 Acq On : 16 Jun 2020 07:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 05 15:08:53 2020

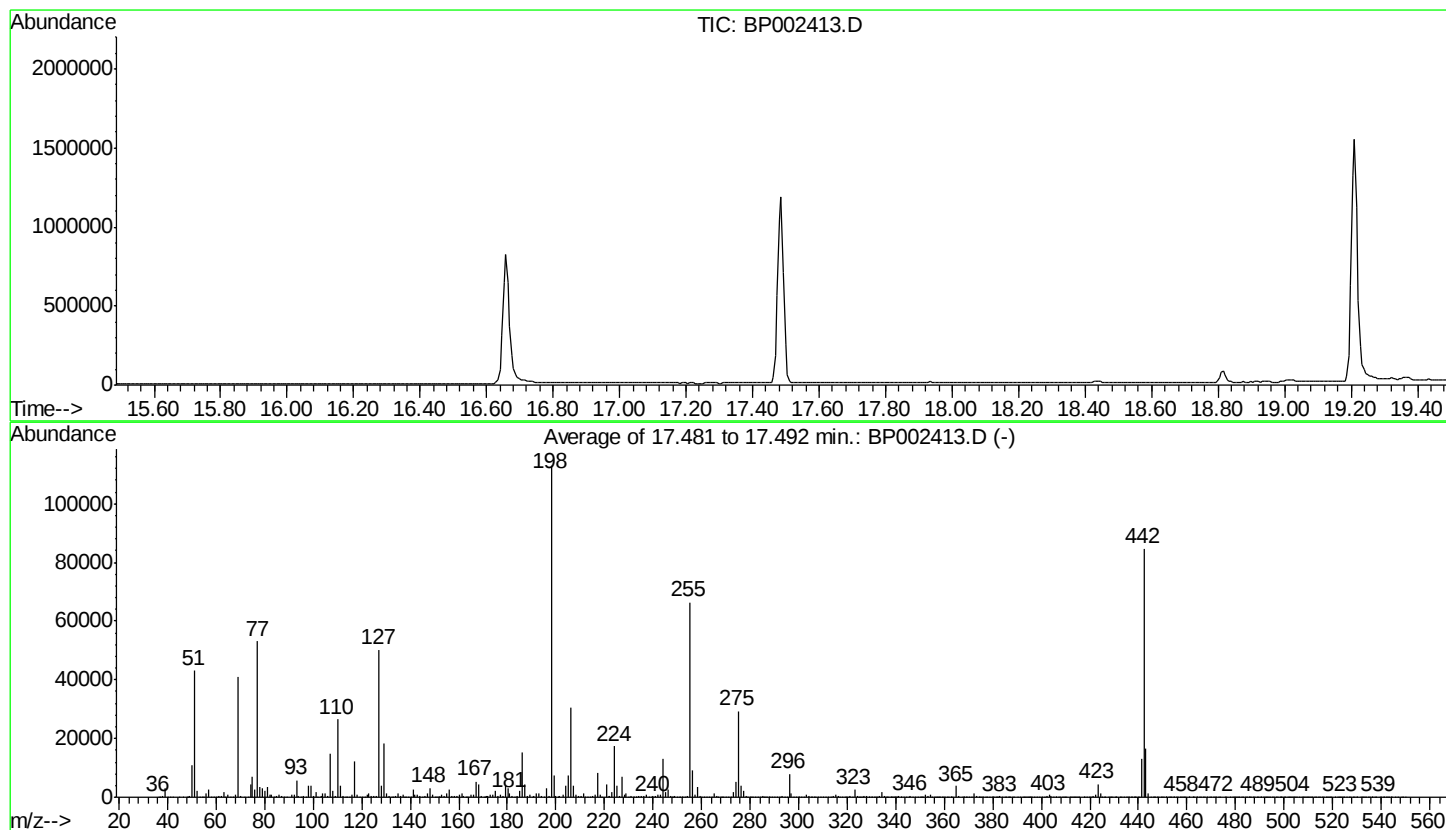

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	43013	PASS
68	69	0.00	2	1.7	698	PASS
69	198	0.00	100	36.5	41222	PASS
70	69	0.00	2	0.6	251	PASS
127	198	10	80	44.4	50184	PASS
197	198	0.00	2	0.4	430	PASS
198	198	100	100	100.0	112989	PASS
199	198	5	9	6.6	7486	PASS
275	198	10	60	25.9	29224	PASS
365	198	1	100	3.3	3779	PASS
441	198	0.01	100	11.6	13098	PASS
442	198	50	100	75.1	84802	PASS
443	442	15	24	19.7	16687	PASS