
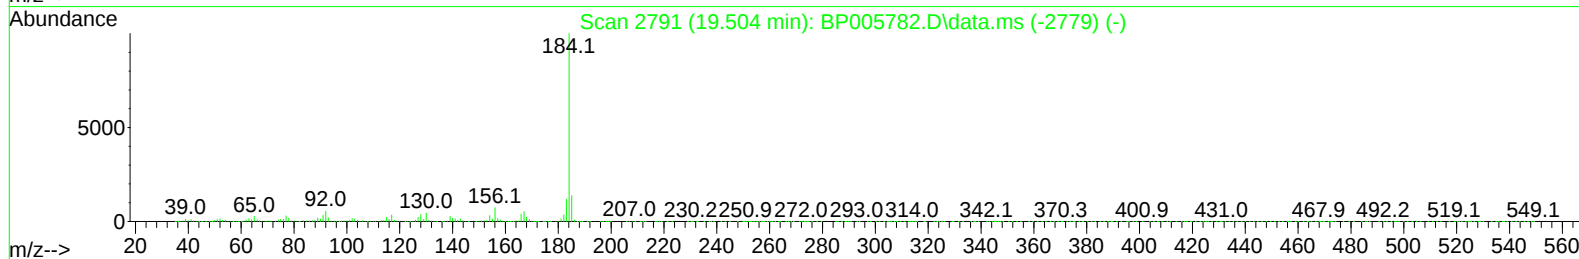
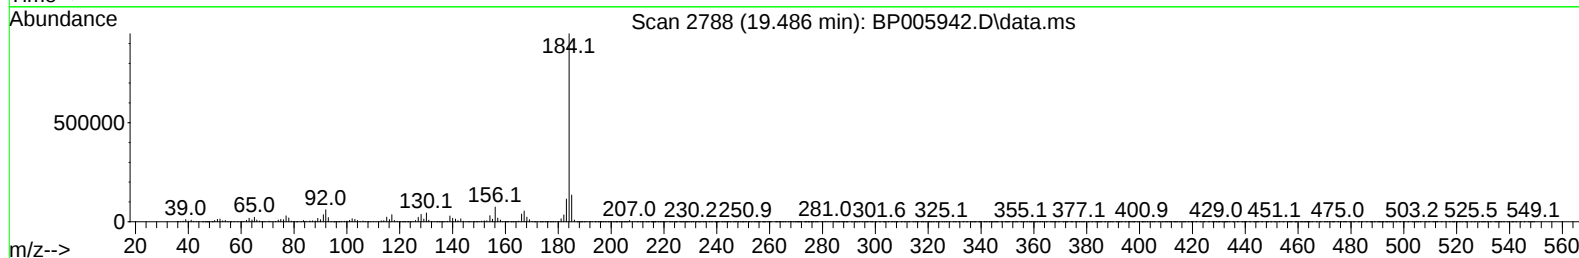


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061621\
 Data File : BP005942.D
 Acq On : 16 Jun 2021 09:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 11:26:48 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 14 13:15:03 2021
 Response via : Initial Calibration

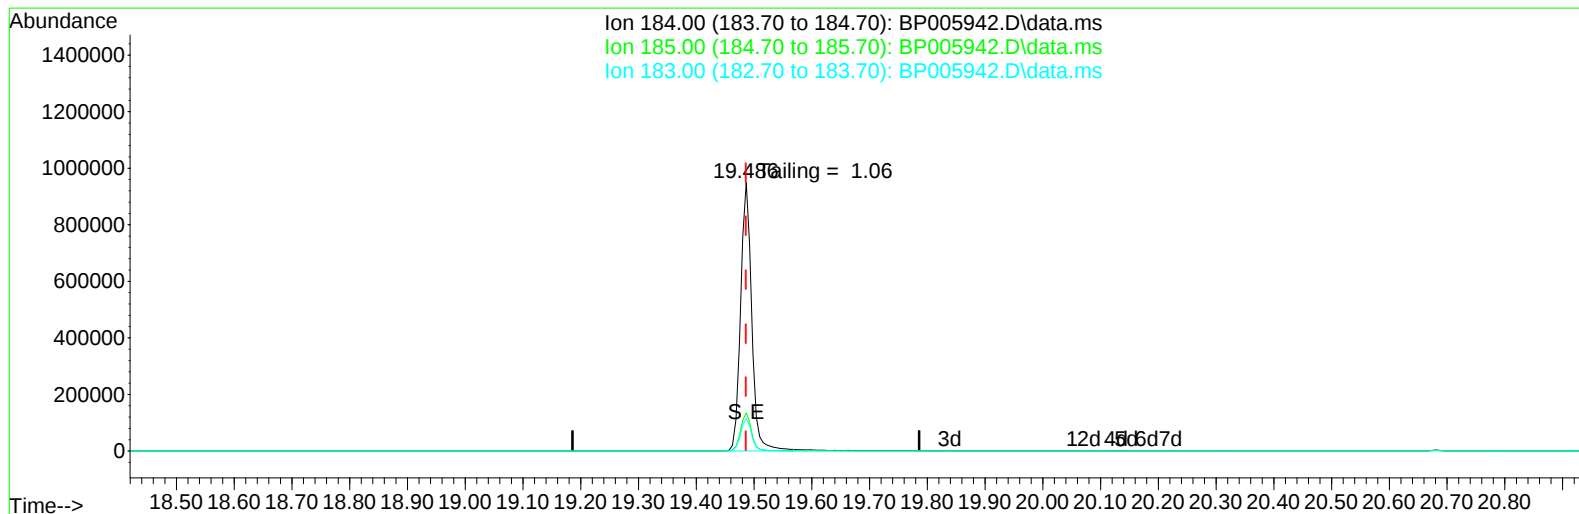

TIC: BP005942.D\data.ms

(77) Benzidine




19.486min (+ 0.000) 1689373.51 ng m

response 1300642

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.22
183.00	11.90	12.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061621\
 Data File : BP005942.D
 Acq On : 16 Jun 2021 09:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 11:26:48 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 14 13:15:03 2021
 Response via : Initial Calibration

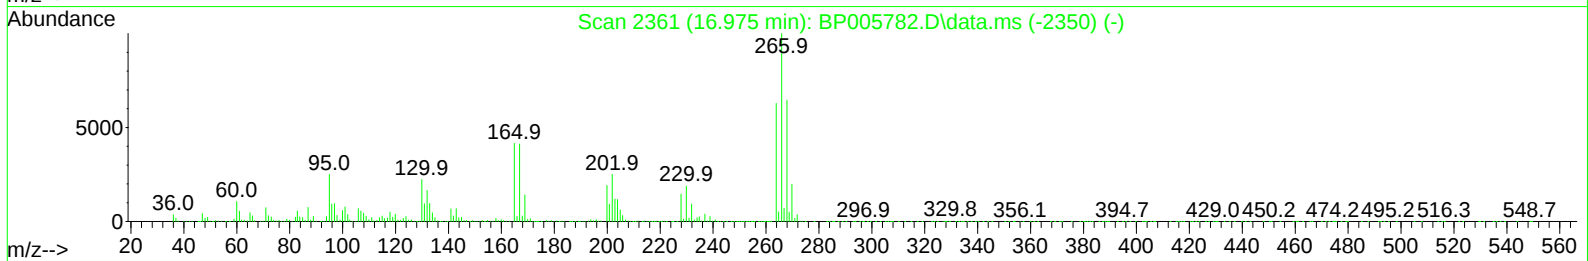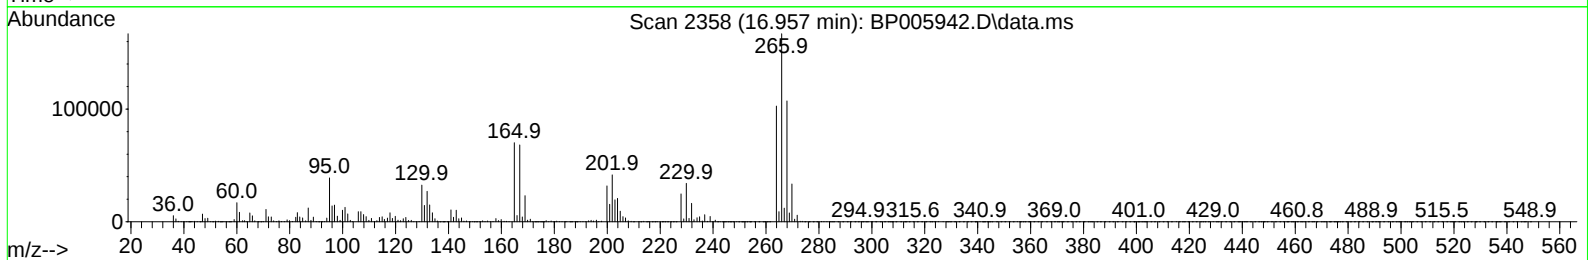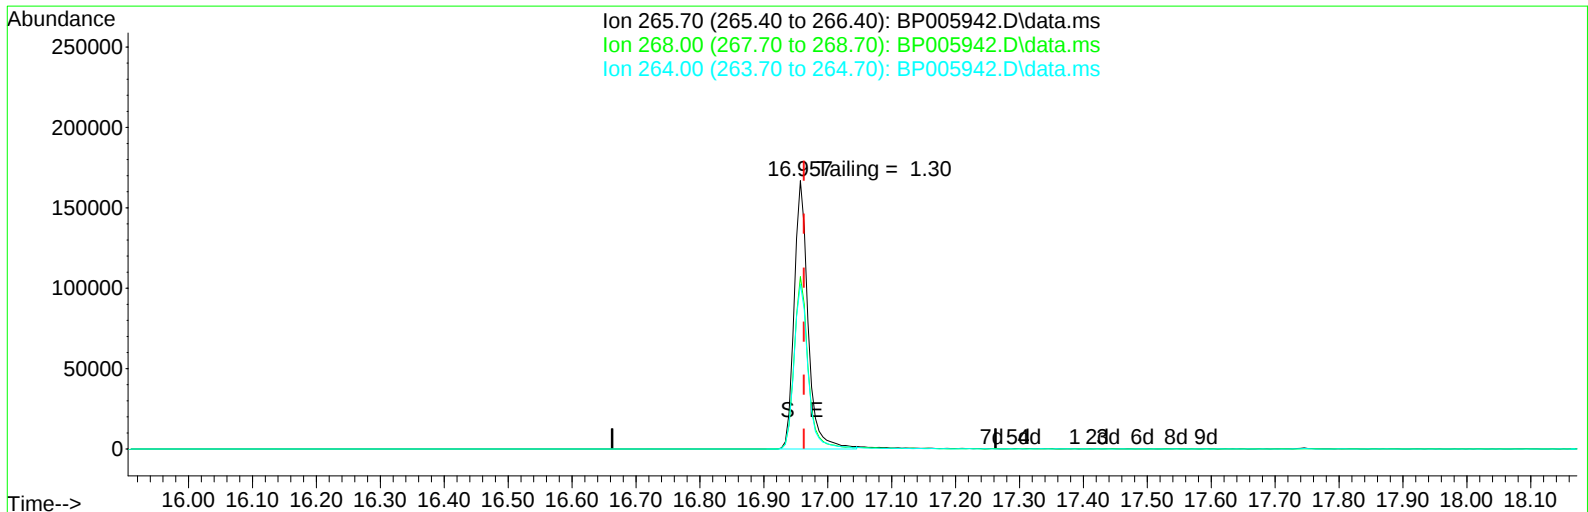

TIC: BP005942.D\data.ms

(70) Pentachlorophenol (C)

16.957min (-0.006) 20418.29 ng m

response 257982

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.23
264.00	62.90	61.50
0.00	0.00	0.00