

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061621\
 Data File : BP005949.D
 Acq On : 16 Jun 2021 14:12
 Operator : CG/JU
 Sample : M2672-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 17-B6(12-16)

Quant Time: Jun 16 14:45:10 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 16 11:35:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	75178	20.000	ng	0.00
21) Naphthalene-d8	10.733	136	288723	20.000	ng	0.00
39) Acenaphthene-d10	14.557	164	187145	20.000	ng	0.00
64) Phenanthrene-d10	17.304	188	403967	20.000	ng	0.00
76) Chrysene-d12	21.374	240	464347	20.000	ng	0.00
86) Perylene-d12	23.786	264	521083	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.504	112	556856	118.857	ng	0.00
7) Phenol-d6	7.104	99	662264	109.059	ng	0.00
23) Nitrobenzene-d5	9.098	82	409948	69.612	ng	0.00
42) 2,4,6-Tribromophenol	16.045	330	348953	108.656	ng	0.00
45) 2-Fluorobiphenyl	13.186	172	954110	66.947	ng	0.00
79) Terphenyl-d14	19.851	244	1667773	67.253	ng	0.00
Target Compounds						
60) Diethylphthalate	15.374	149	34595	2.241	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061621\
Data File : BP005949.D
Acq On : 16 Jun 2021 14:12
Operator : CG/JU
Sample : M2672-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
17-B6(12-16)

Quant Time: Jun 16 14:45:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 11:35:30 2021
Response via : Initial Calibration




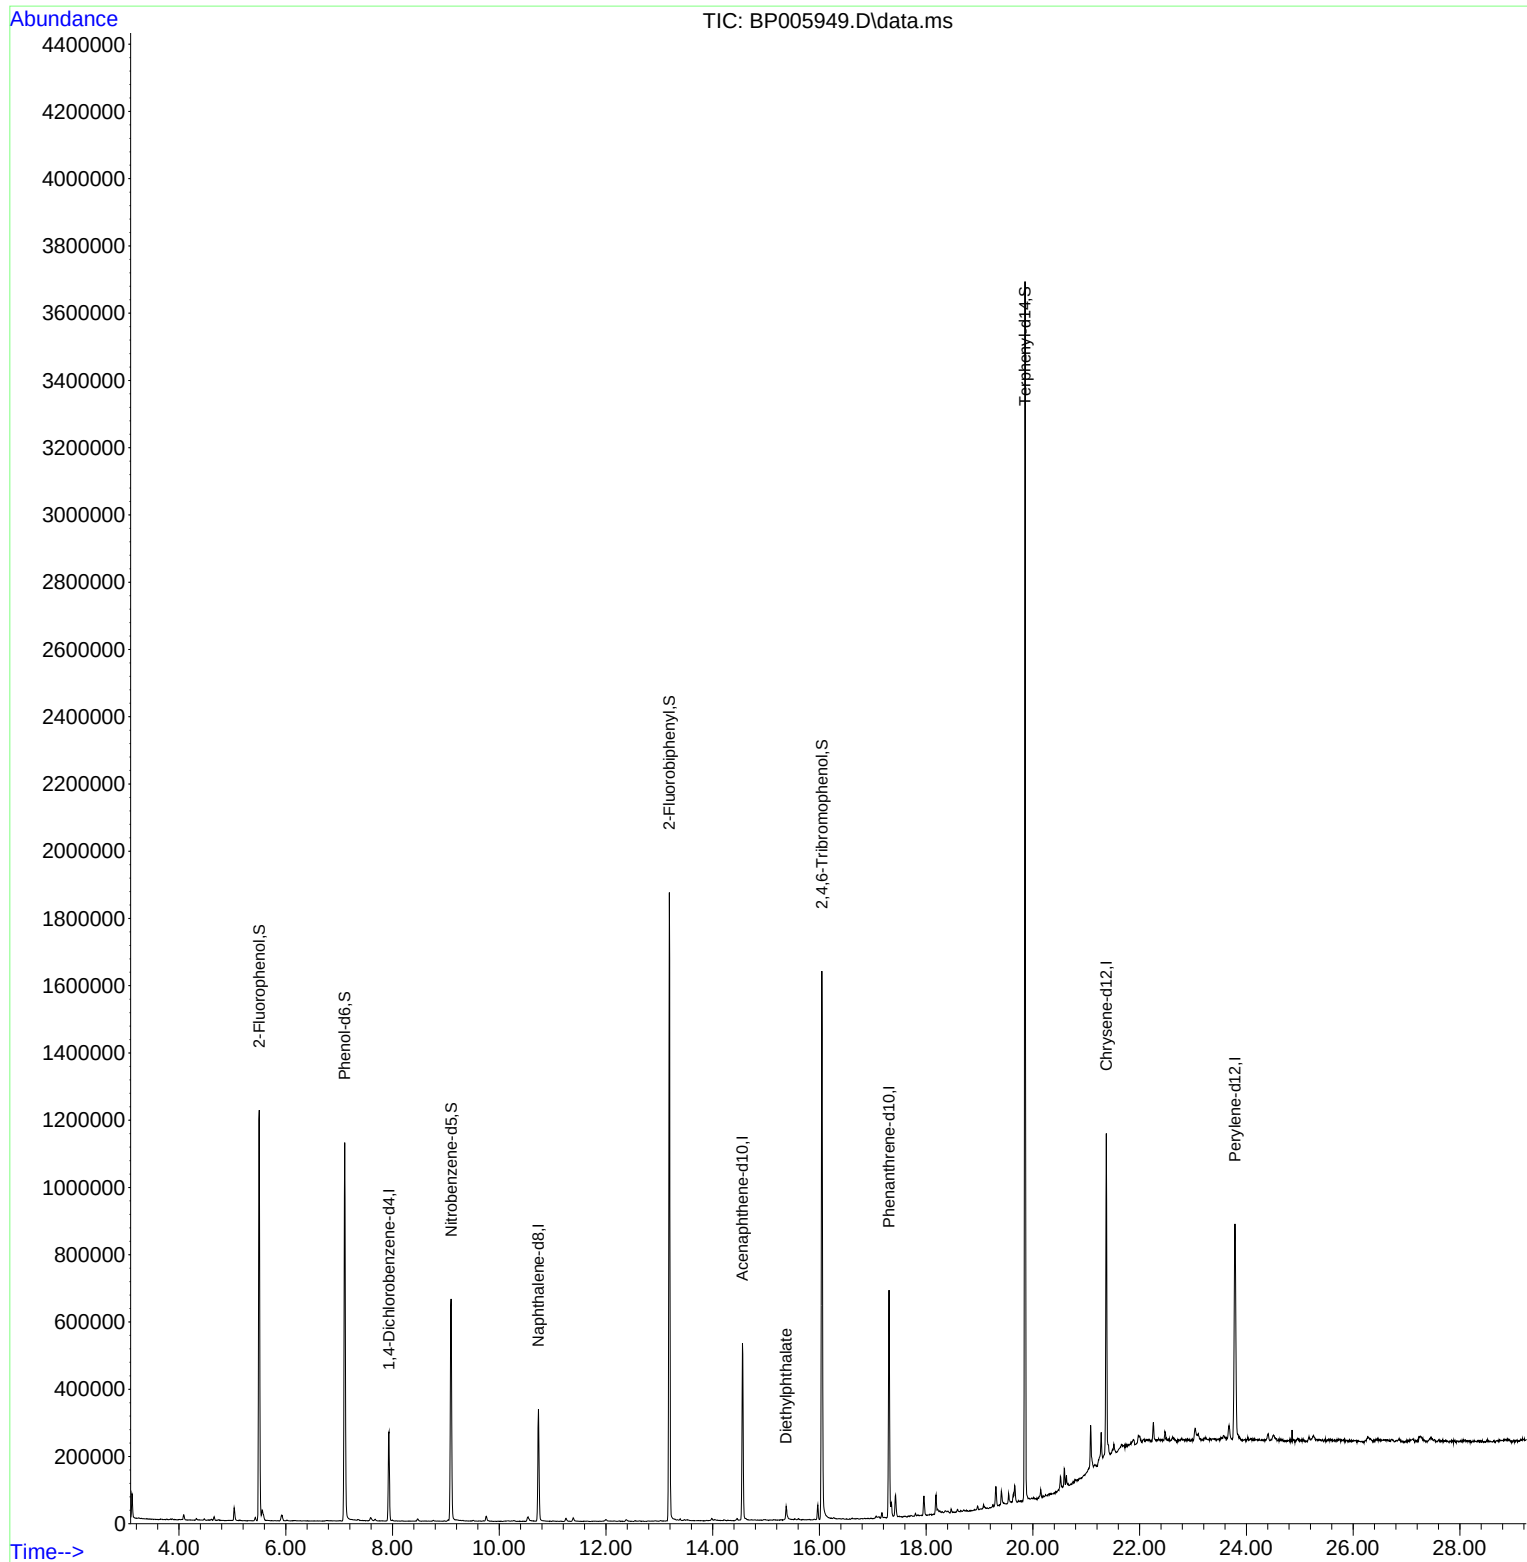


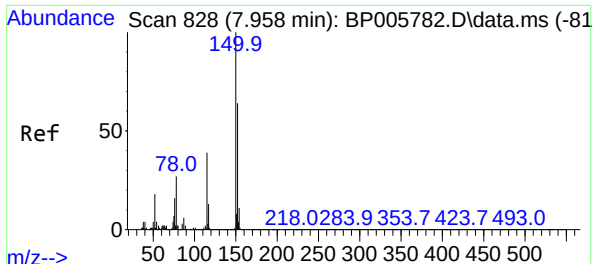

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.934 min Scan# 824
Delta R.T. 0.006 min
Lab File: BP005949.D
Acq: 16 Jun 2021 14:12




Instrument :
BNA_P
ClientSampleId :
17-B6(12-16)


Tgt Ion:152 Resp: 75178
Ion Ratio Lower Upper
152 100
150 155.6 125.6 188.4
115 61.4 48.5 72.7

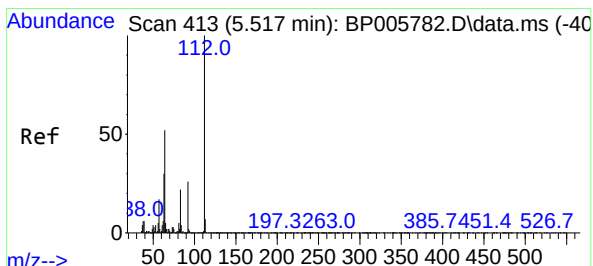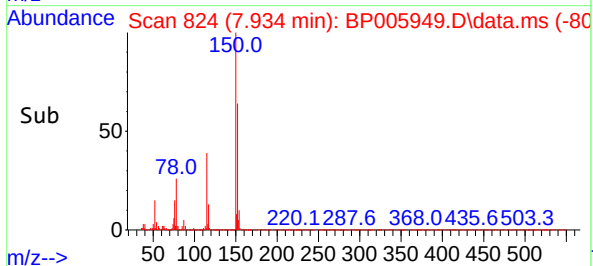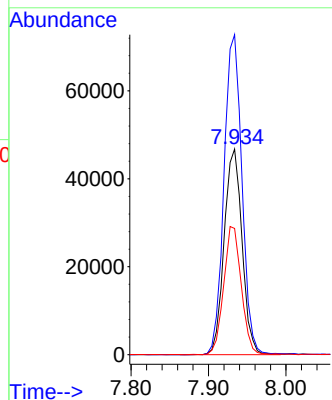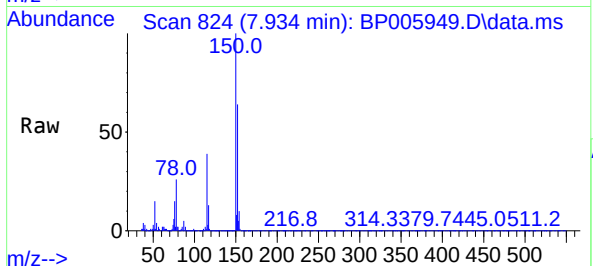

#5
2-Fluorophenol
Concen: 118.857 ng
RT: 5.504 min Scan# 411
Delta R.T. 0.006 min
Lab File: BP005949.D
Acq: 16 Jun 2021 14:12

Tgt Ion:112 Resp: 556856
Ion Ratio Lower Upper
112 100
64 49.5 41.4 62.2
63 27.3 23.8 35.8


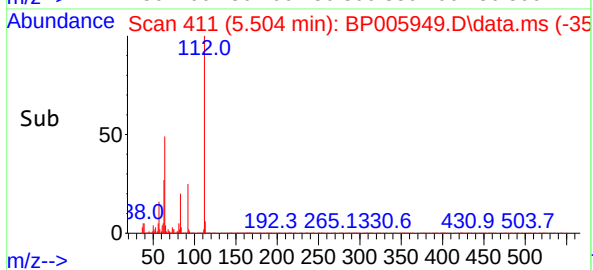
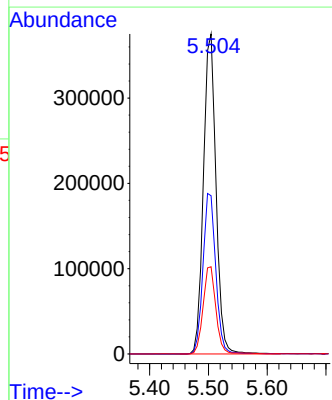
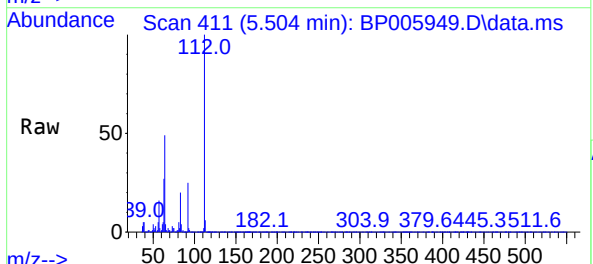


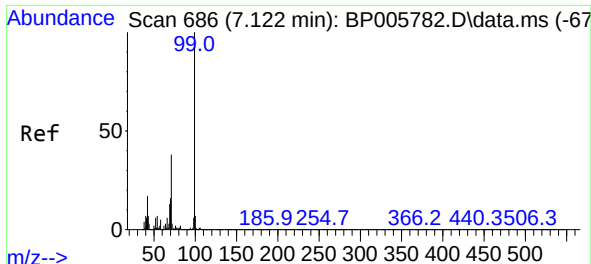

#7
Phenol-d6
Concen: 109.059 ng
RT: 7.104 min Scan# 683
Delta R.T. -0.000 min
Lab File: BP005949.D
Acq: 16 Jun 2021 14:12




Instrument :
BNA_P
ClientSampleId :
17-B6(12-16)


Tgt Ion: 99 Resp: 662264
Ion Ratio Lower Upper
99 100
42 15.5 13.4 20.0
71 37.1 30.6 46.0

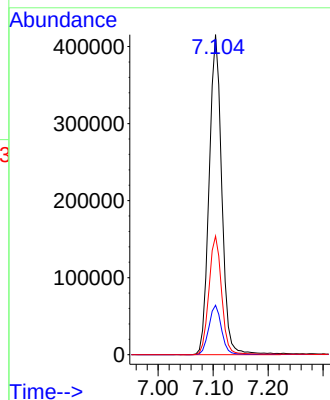

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.733 min Scan# 1300
Delta R.T. -0.000 min
Lab File: BP005949.D
Acq: 16 Jun 2021 14:12

Tgt Ion: 136 Resp: 288723
Ion Ratio Lower Upper
136 100
137 10.8 8.6 12.8
54 5.3 4.6 6.8
68 5.0 3.6 5.4


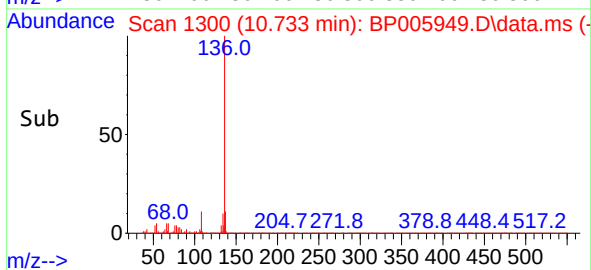
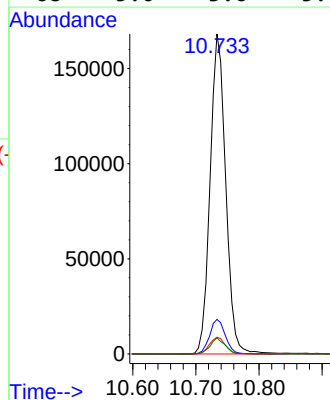
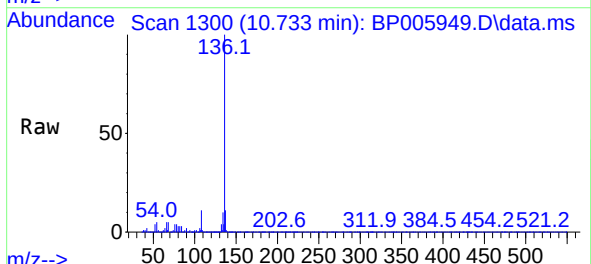


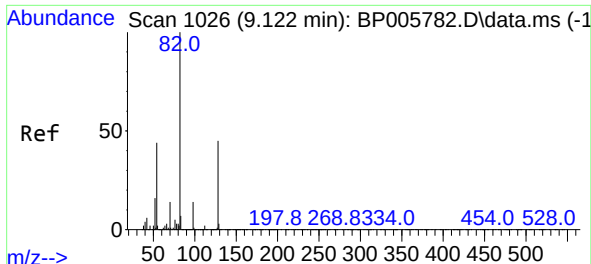

#23
Nitrobenzene-d5
Concen: 69.612 ng
RT: 9.098 min Scan# 1022
Delta R.T. 0.006 min
Lab File: BP005949.D
Acq: 16 Jun 2021 14:12




Instrument :
BNA_P
ClientSampleId :
17-B6(12-16)


Tgt Ion: 82 Resp: 409948
Ion Ratio Lower Upper
82 100
128 46.3 35.7 53.5
54 40.8 35.0 52.4

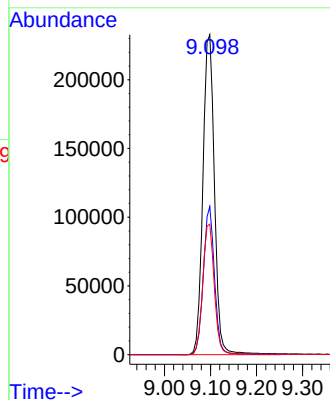

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.557 min Scan# 1950
Delta R.T. -0.000 min
Lab File: BP005949.D
Acq: 16 Jun 2021 14:12

Tgt Ion: 164 Resp: 187145
Ion Ratio Lower Upper
164 100
162 103.5 80.2 120.2
160 45.3 34.5 51.7


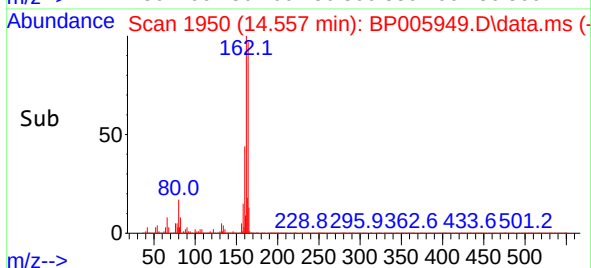
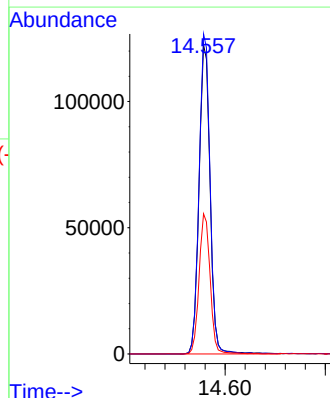
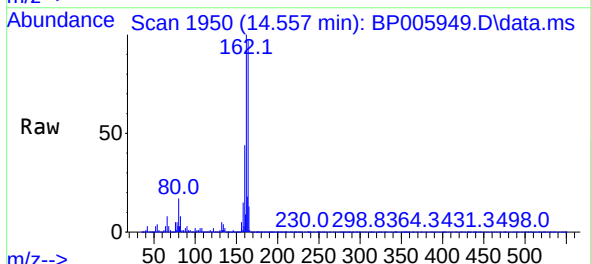


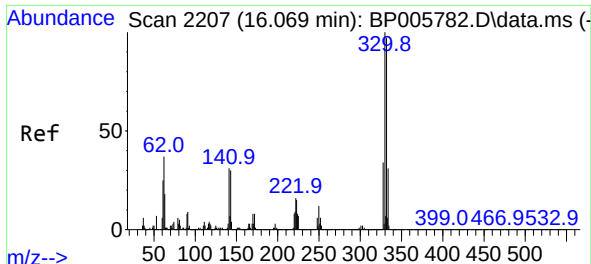

#42
2,4,6-Tribromophenol
Concen: 108.656 ng
RT: 16.045 min Scan# 2203
Delta R.T. -0.006 min
Lab File: BP005949.D
Acq: 16 Jun 2021 14:12




Instrument :
BNA_P
ClientSampleId :
17-B6(12-16)


Tgt Ion:330 Resp: 348953
Ion Ratio Lower Upper
330 100
332 99.2 77.8 116.8
141 29.8 25.4 38.2

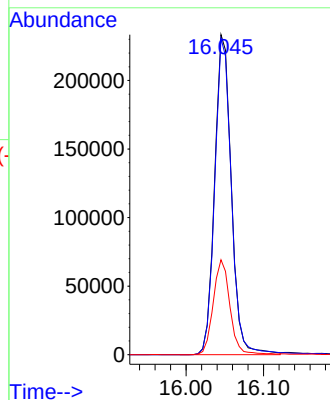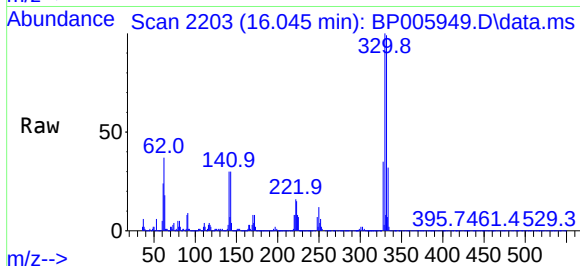

#45
2-Fluorobiphenyl
Concen: 66.947 ng
RT: 13.186 min Scan# 1717
Delta R.T. -0.000 min
Lab File: BP005949.D
Acq: 16 Jun 2021 14:12

Tgt Ion:172 Resp: 954110
Ion Ratio Lower Upper
172 100
171 34.8 27.9 41.9
170 23.0 18.6 27.8


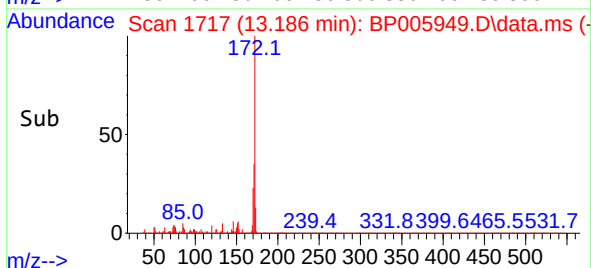
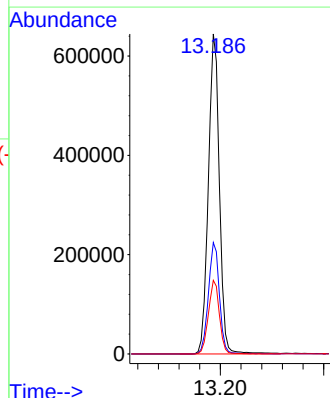
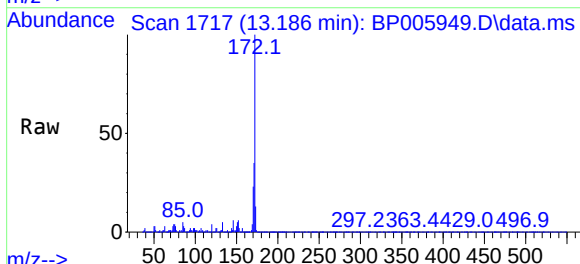




#60
Diethylphthalate
Concen: 2.241 ng
RT: 15.374 min Scan# 2089
Delta R.T. -0.006 min
Lab File: BP005949.D
Acq: 16 Jun 2021 14:12




Instrument :
BNA_P
ClientSampleId :
17-B6(12-16)


Tgt Ion:	149	Resp:	34595
Ion Ratio	Lower	Upper	
149	100		
177	22.4	17.5	26.3
150	13.5	9.9	14.9

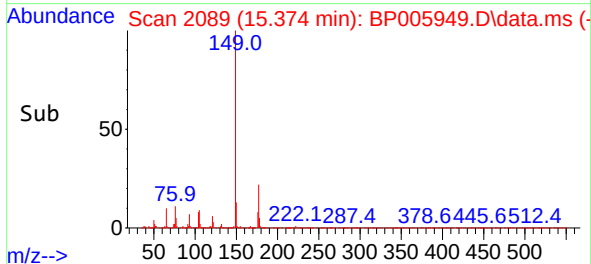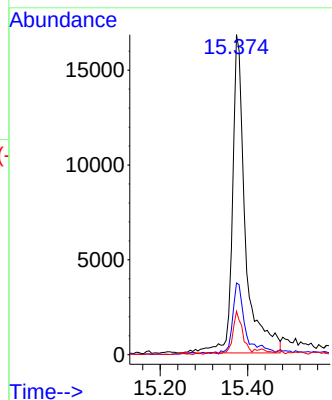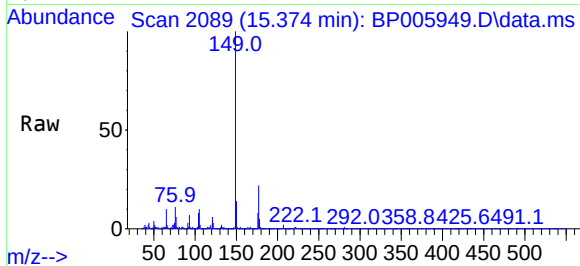

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.304 min Scan# 2417
Delta R.T. -0.000 min
Lab File: BP005949.D
Acq: 16 Jun 2021 14:12

Tgt Ion:	188	Resp:	403967
Ion Ratio	Lower	Upper	
188	100		
94	7.4	5.6	8.4
80	7.9	6.3	9.5


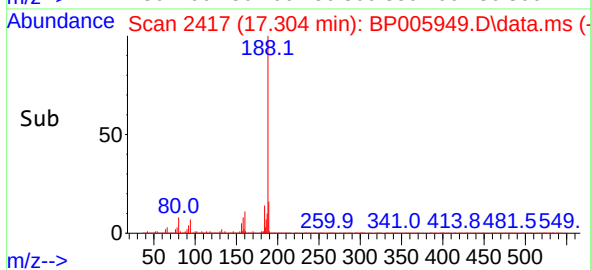
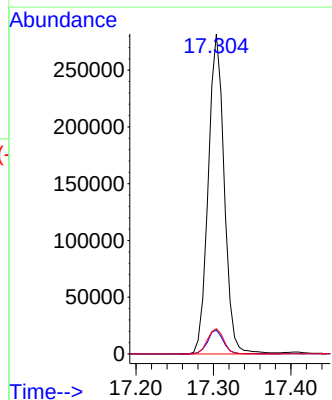
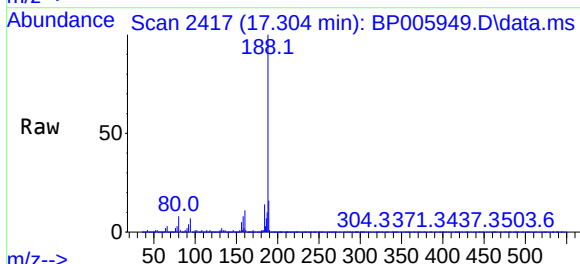




#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.374 min Scan# 3109
Delta R.T. -0.006 min
Lab File: BP005949.D
Acq: 16 Jun 2021 14:12




Instrument :
BNA_P
ClientSampleId :
17-B6(12-16)


Tgt Ion:240 Resp: 464347
Ion Ratio Lower Upper
240 100
120 8.6 6.5 9.7
236 25.6 20.6 31.0

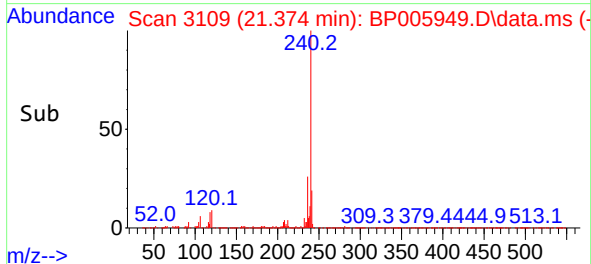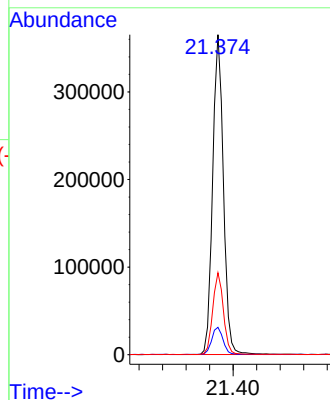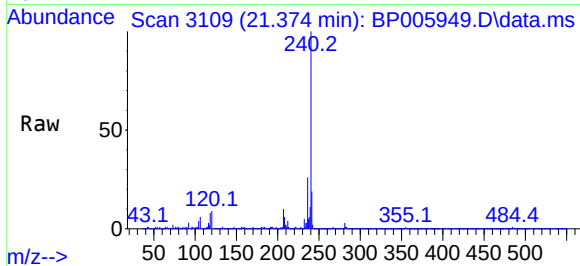

#79
Terphenyl-d14
Concen: 67.253 ng
RT: 19.851 min Scan# 2850
Delta R.T. -0.006 min
Lab File: BP005949.D
Acq: 16 Jun 2021 14:12


Tgt Ion:244 Resp: 1667773
Ion Ratio Lower Upper
244 100
212 7.4 6.0 9.0
122 9.2 7.1 10.7

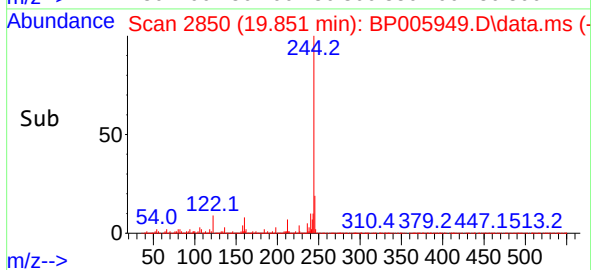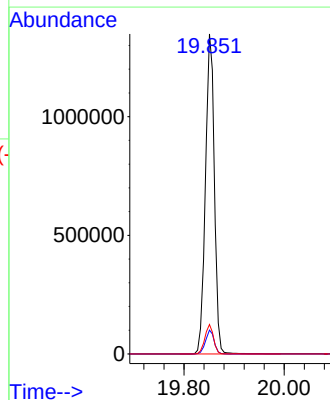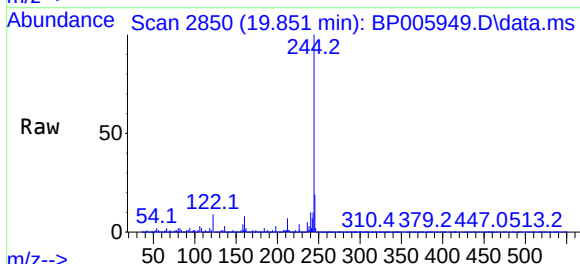

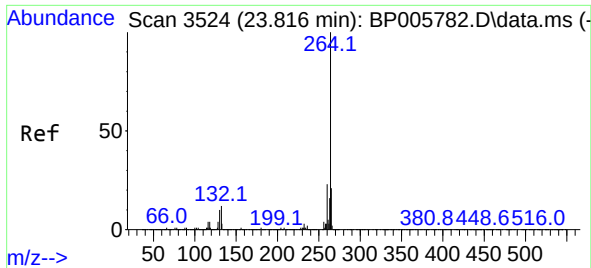

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.786 min Scan# 3519
 Delta R.T. -0.006 min
 Lab File: BP005949.D
 Acq: 16 Jun 2021 14:12

Instrument :
 BNA_P
 ClientSampleId :
 17-B6(12-16)

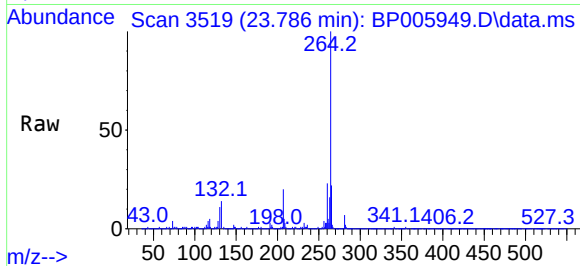

Tgt Ion:264 Resp: 521083

Ion	Ratio	Lower	Upper
264	100		
260	23.5	18.6	28.0
265	22.1	17.6	26.4

