
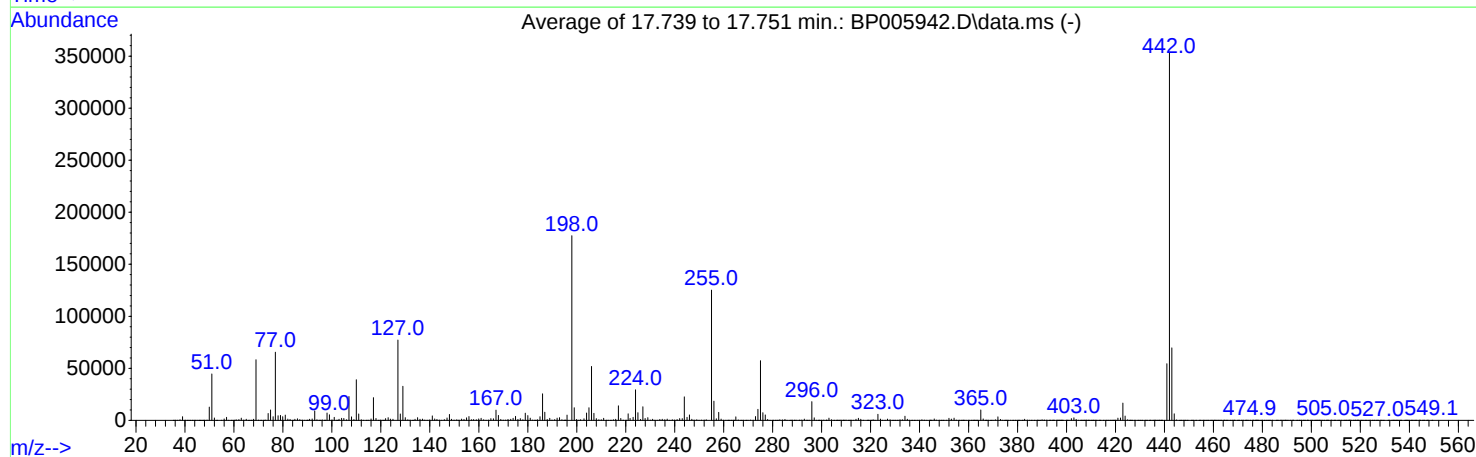


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061621\
 Data File : BP005942.D
 Acq On : 16 Jun 2021 09:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 16 11:35:30 2021

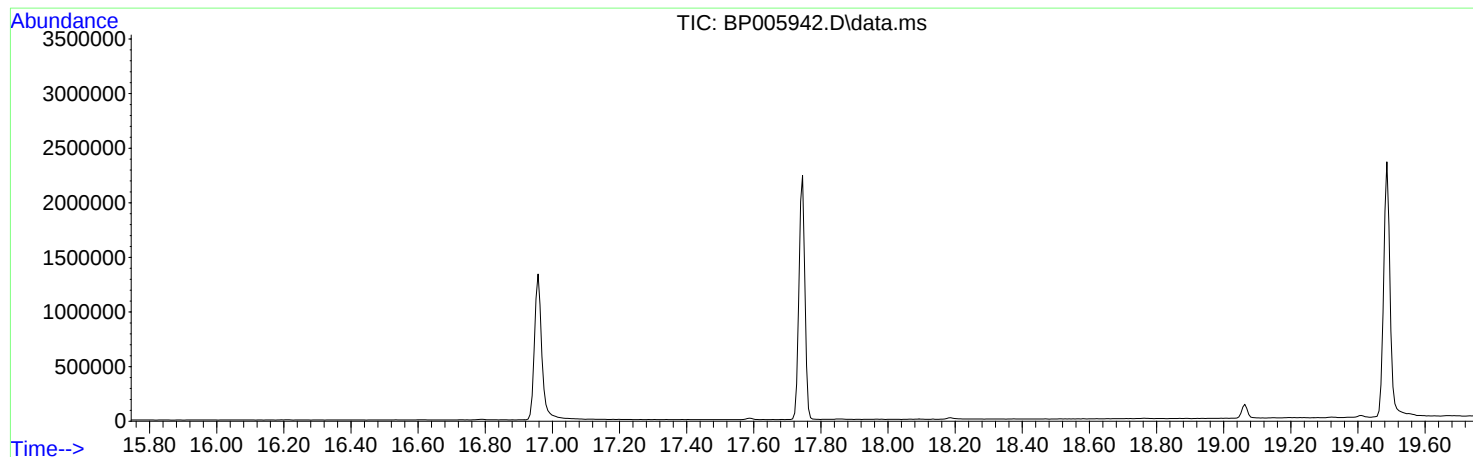




AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.1	44546	PASS
68	69	0.00	2	1.8	1035	PASS
69	198	0.00	100	32.8	58236	PASS
70	69	0.00	2	0.6	364	PASS
127	198	10	80	43.5	77209	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	177467	PASS
199	198	5	9	6.8	12103	PASS
275	198	10	60	32.3	57392	PASS
365	198	1	100	5.6	9958	PASS
441	198	0.01	100	30.7	54424	PASS
442	442	100	100	100.0	353472	PASS
443	442	15	24	19.7	69667	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061621\
 Data File : BP005942.D
 Acq On : 16 Jun 2021 09:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 16 11:26:48 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 14 13:15:03 2021
 Response via : Initial Calibration

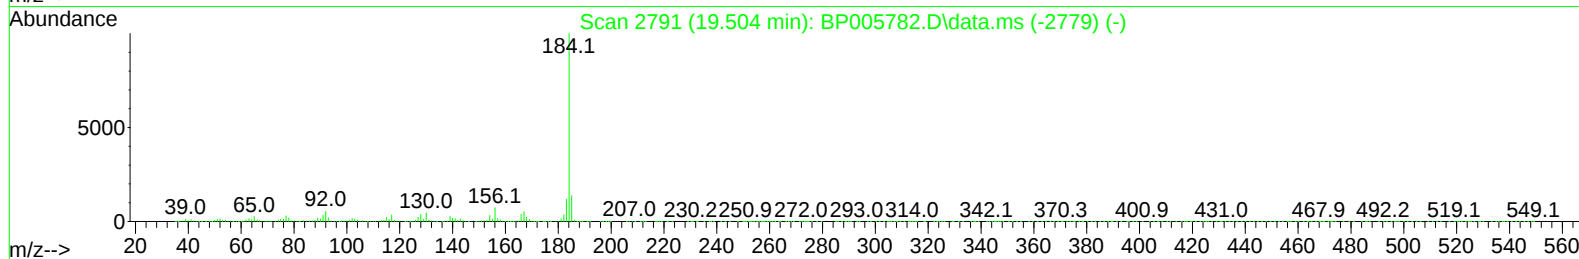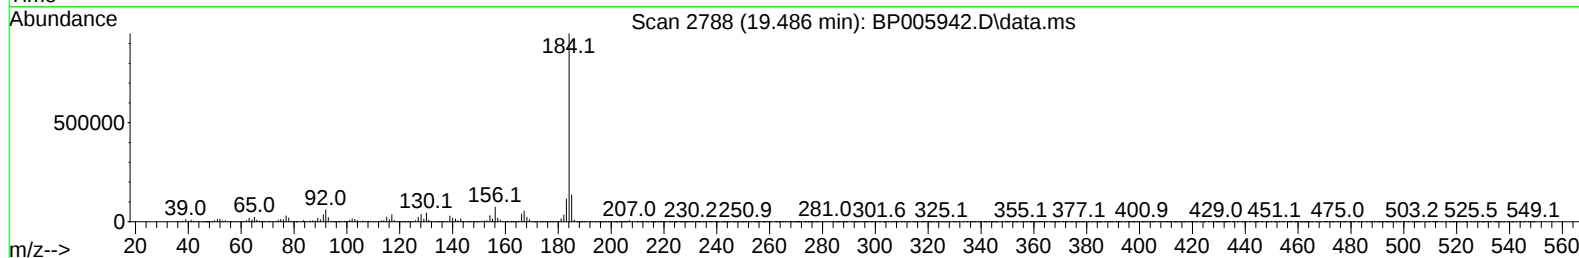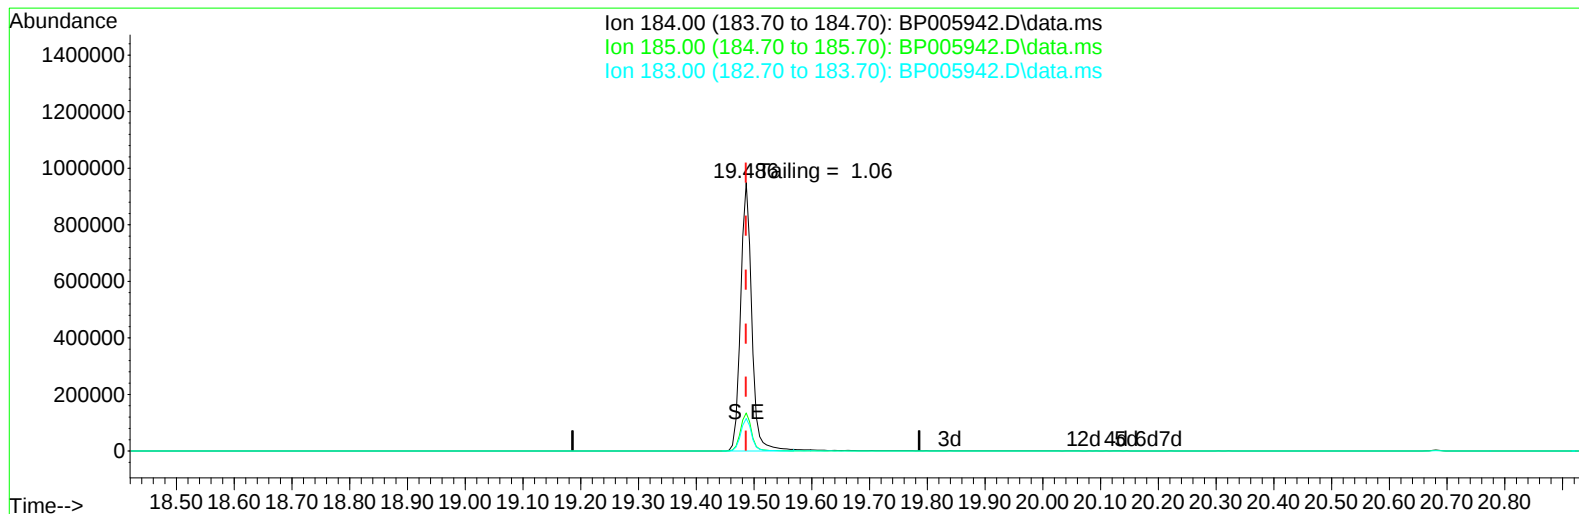

TIC: BP005942.D\data.ms

(77) Benzidine

19.486min (+ 0.000) 1689373.51 ng m




response 1300642

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.22
183.00	11.90	12.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061621\
Data File : BP005942.D
Acq On : 16 Jun 2021 09:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 16 11:26:48 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 14 13:15:03 2021
Response via : Initial Calibration

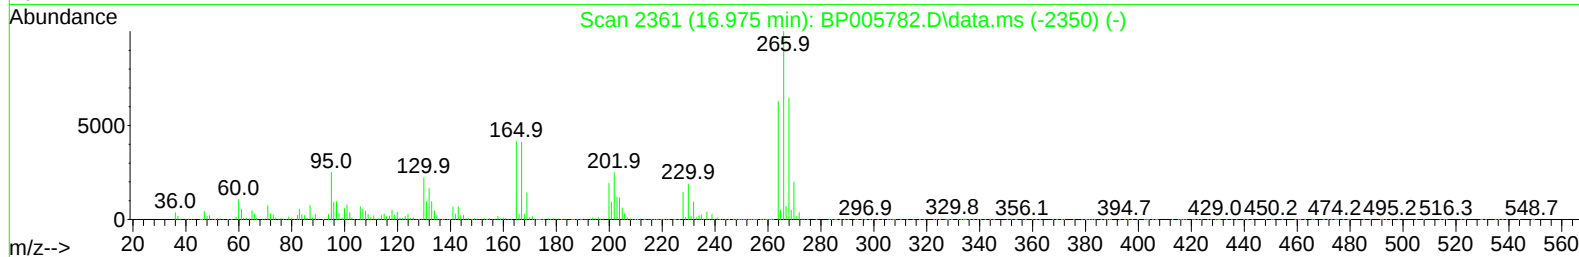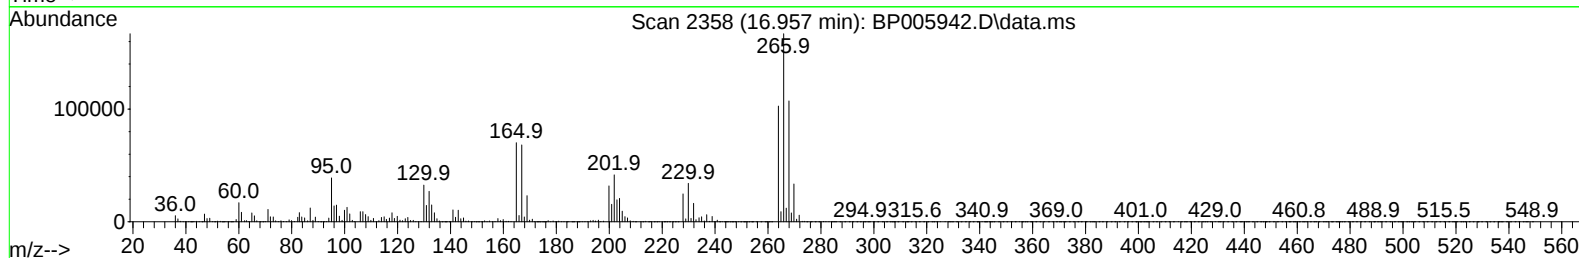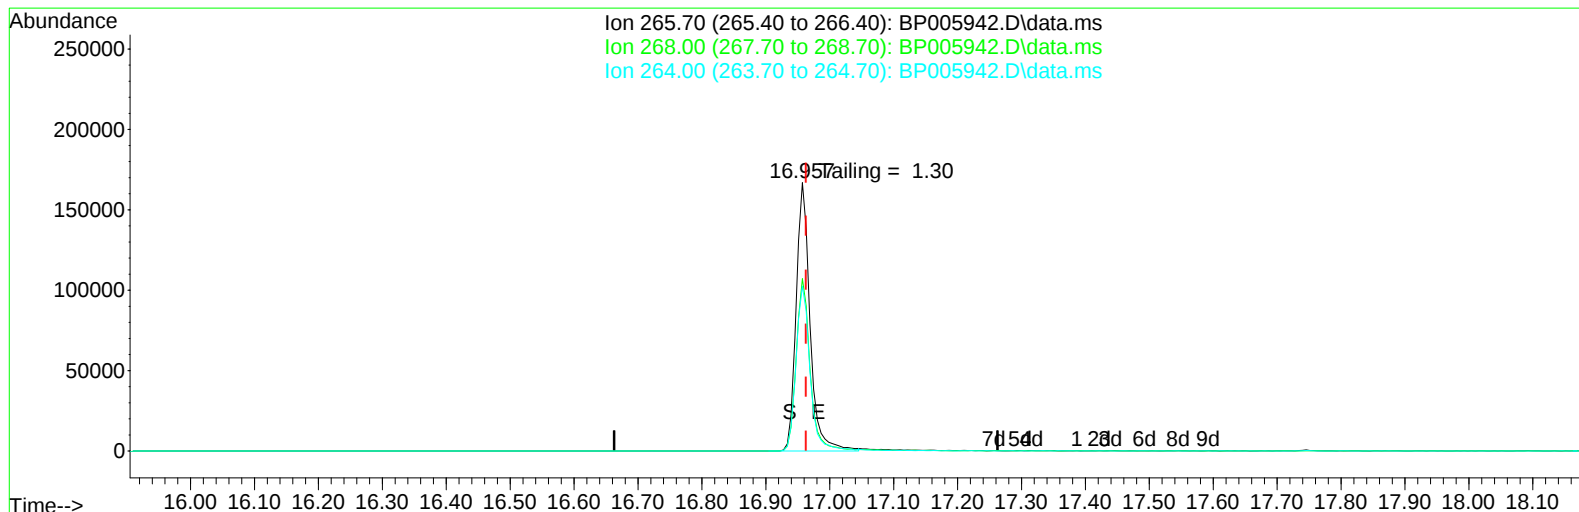

TIC: BP005942.D\data.ms

(70) Pentachlorophenol (C)

16.957min (-0.006) 20418.29 ng m

response 257982

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.23
264.00	62.90	61.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/16/2021	BNA_P	<u>BP005942.D</u>
Compound Name	Response	Retention Time
DDT	774353	20.68
DDD	9283	20.25
DDE	2587	19.76
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11870	786223	1.51

Instrument :
BNA_P
ClientSampleId :
DFTPP