


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061625\
 Data File : BP024954.D
 Acq On : 16 Jun 2025 10:12
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-Tune.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 29 08:52:24 2022

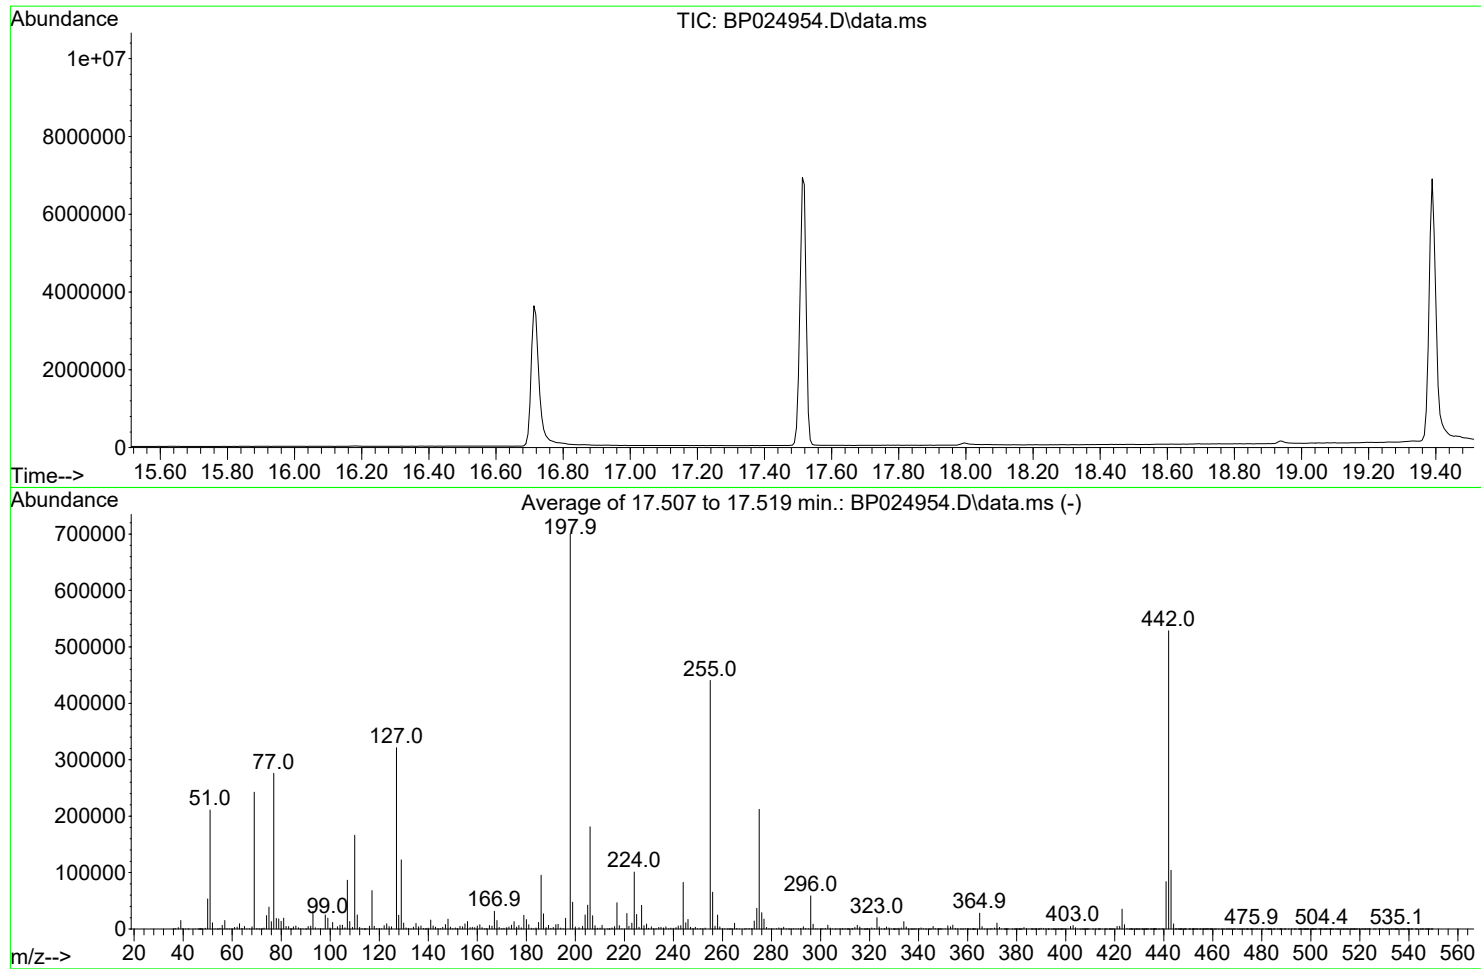

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.7	4125	PASS
69	69	100	100	100.0	242495	PASS
70	69	0.00	2	0.4	1073	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	699861	PASS
199	198	5	9	6.8	47614	PASS
365	198	1	100	4.0	28085	PASS
441	443	0.01	150	80.8	84032	PASS
442	442	100	100	100.0	528640	PASS
443	442	15	24	19.7	103980	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/16/2025	BNA_P	<u>BP024954.D</u>
Compound Name	Response	Retention Time
DDT	2334210	20.671
DDD	110076	20.218
DDE	7204	19.683
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
117280	2451490	4.78

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061625\
Data File : BP024954.D
Acq On : 16 Jun 2025 10:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 16 11:32:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

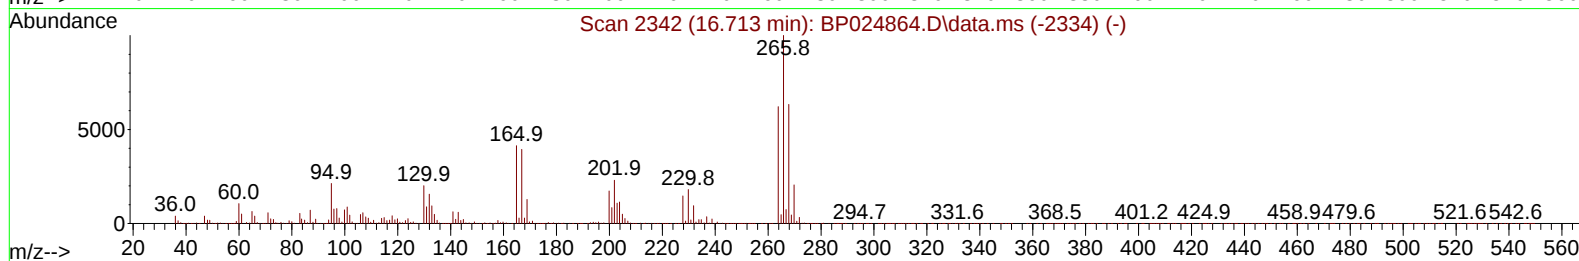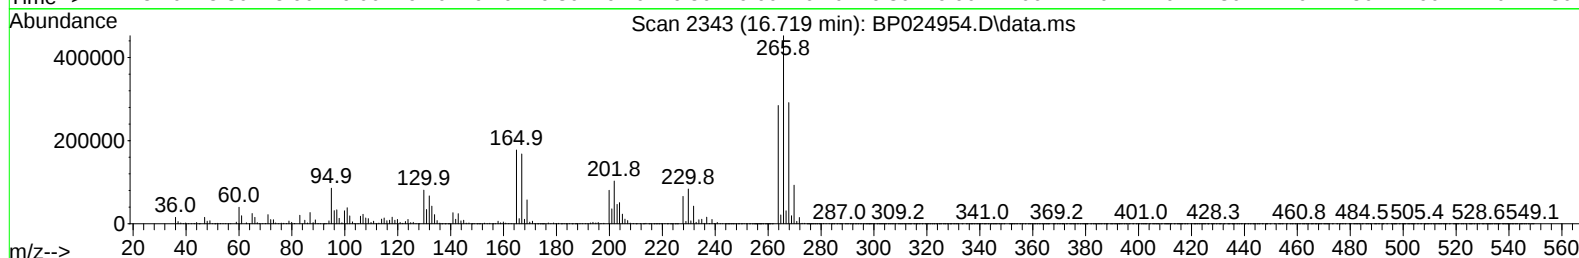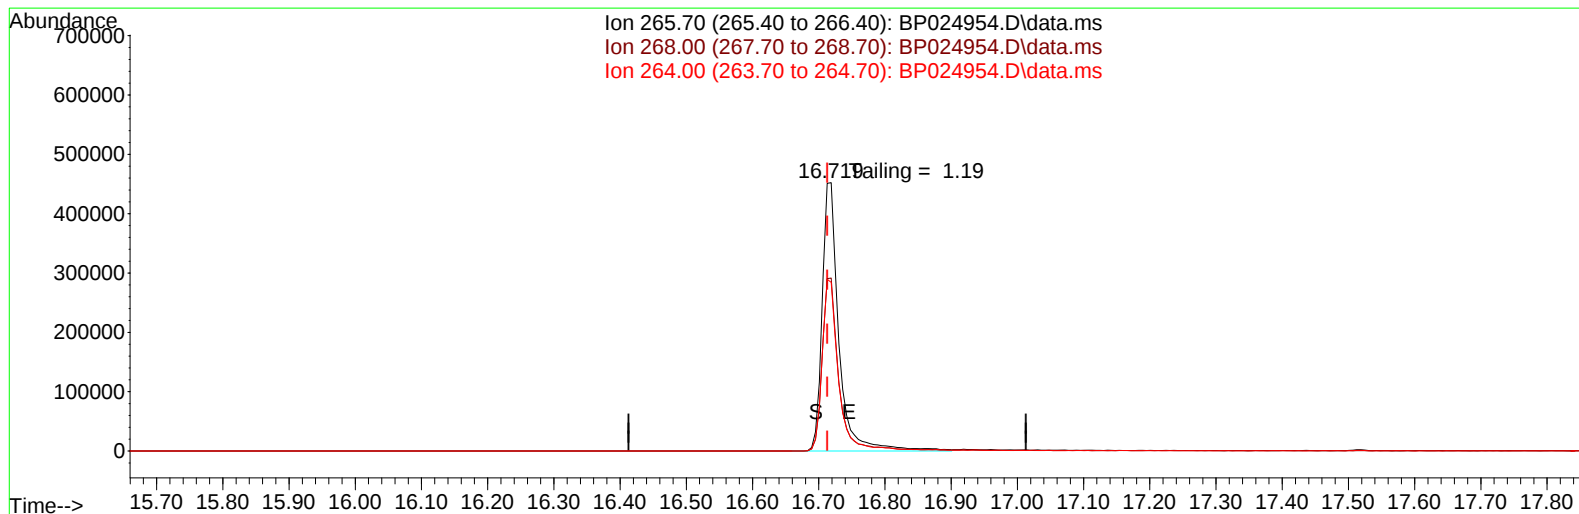

TIC: BP024954.D\data.ms

(70) Pentachlorophenol (C)

16.719min (+ 0.006) 374470.64 ng




response 784698

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.45
264.00	62.10	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061625\
Data File : BP024954.D
Acq On : 16 Jun 2025 10:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 16 11:32:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

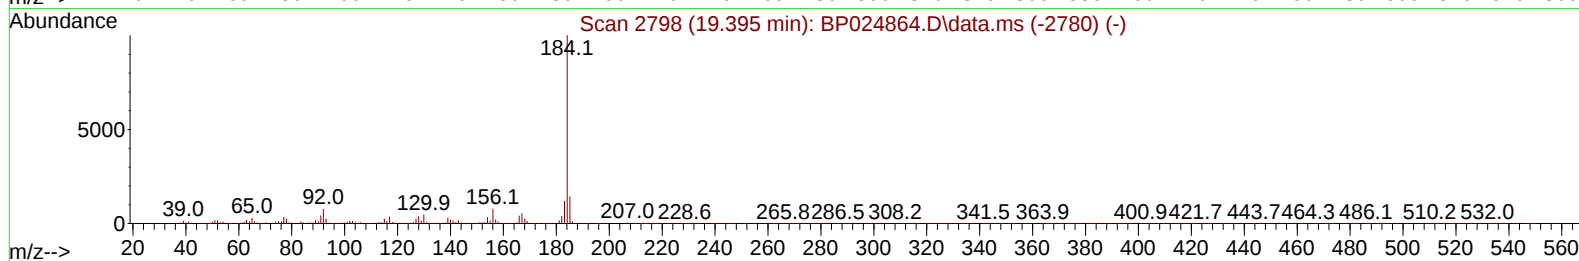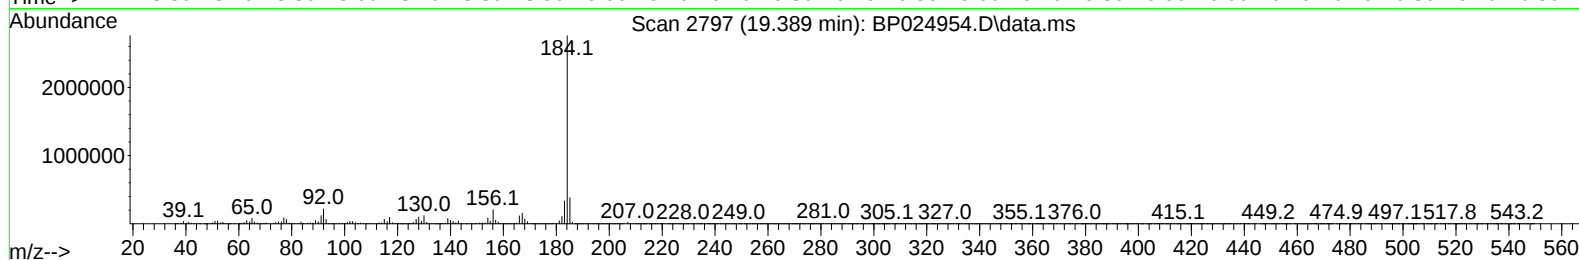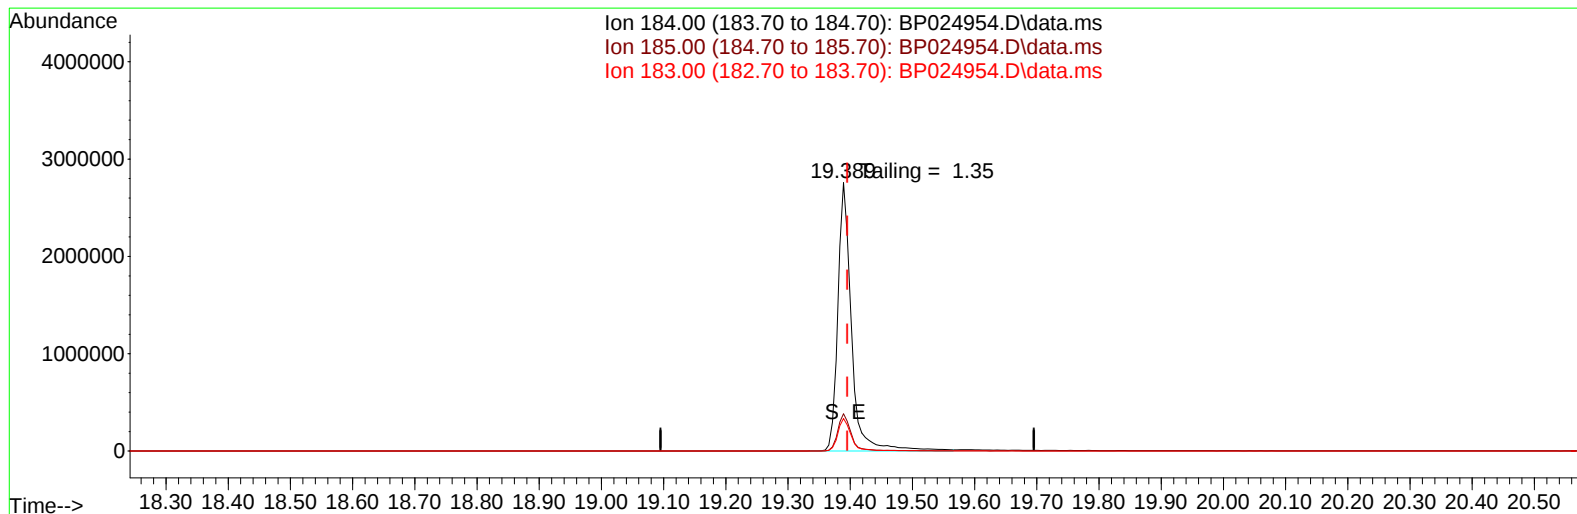

TIC: BP024954.D\data.ms

(77) Benzidine

19.389min (-0.006) 71912.45 ng

response 4207243

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.88
183.00	11.90	12.09
0.00	0.00	0.00