
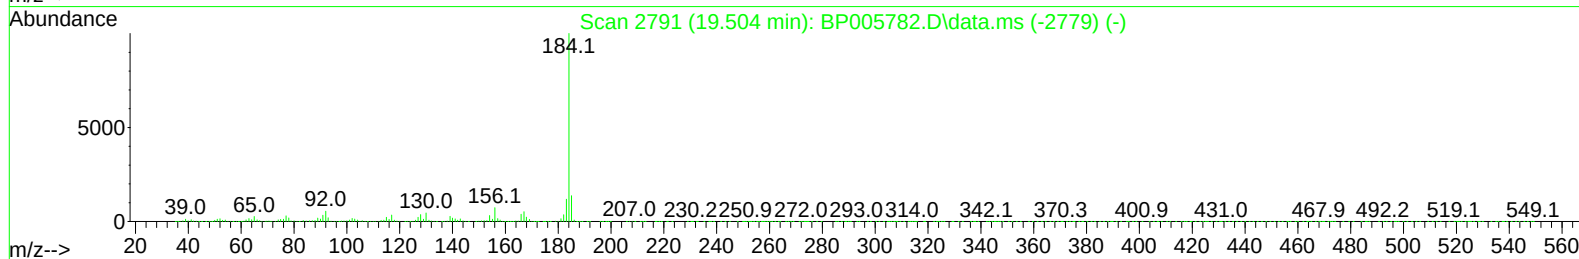
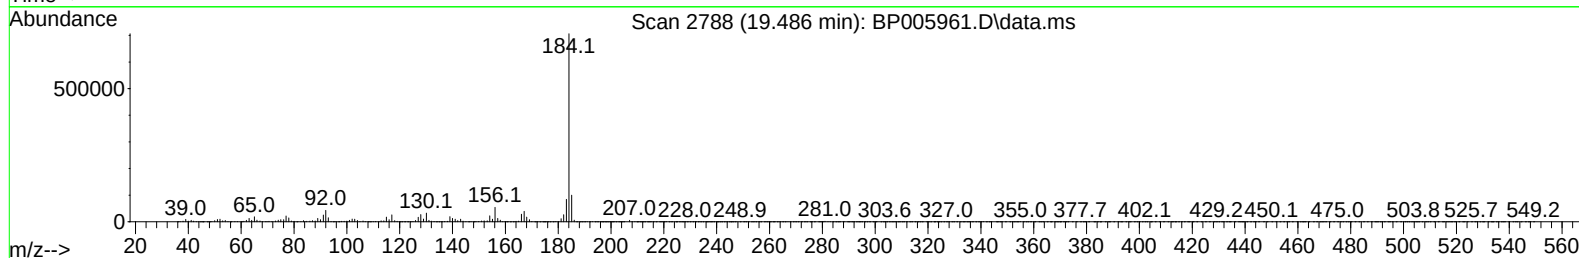


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP061721\  
Data File : BP005961.D  
Acq On : 17 Jun 2021 10:15  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 13:41:55 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP060821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jun 16 11:35:30 2021  
Response via : Initial Calibration

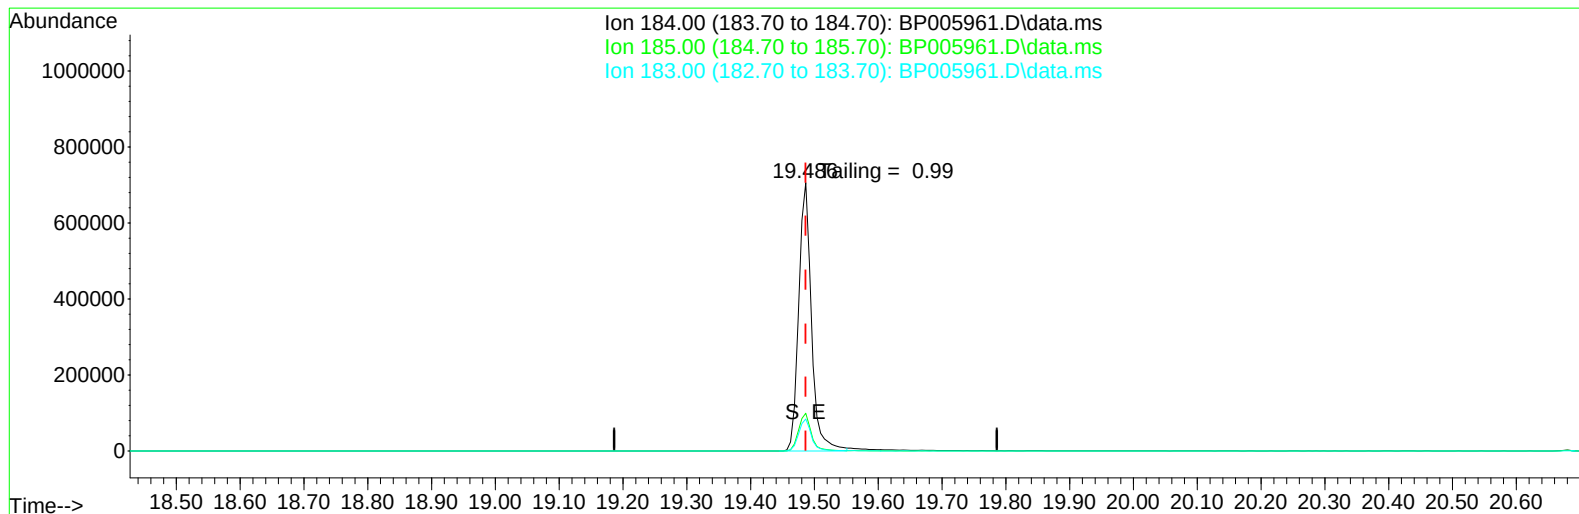

TIC: BP005961.D\data.ms

**(77) Benzidine**




19.486min (+ 0.000) 36969.48 ng

response 1005424

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.70  | 14.09  |
| 183.00 | 11.90  | 11.95  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP061721\  
Data File : BP005961.D  
Acq On : 17 Jun 2021 10:15  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 13:41:55 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP060821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jun 16 11:35:30 2021  
Response via : Initial Calibration

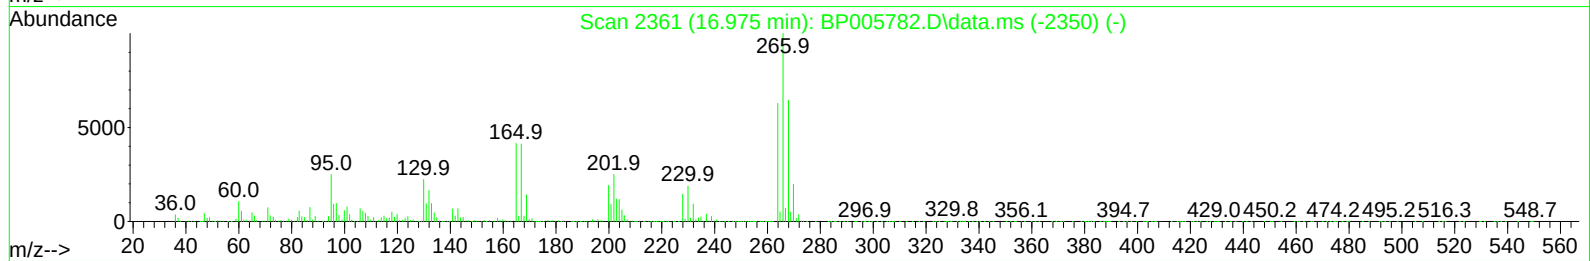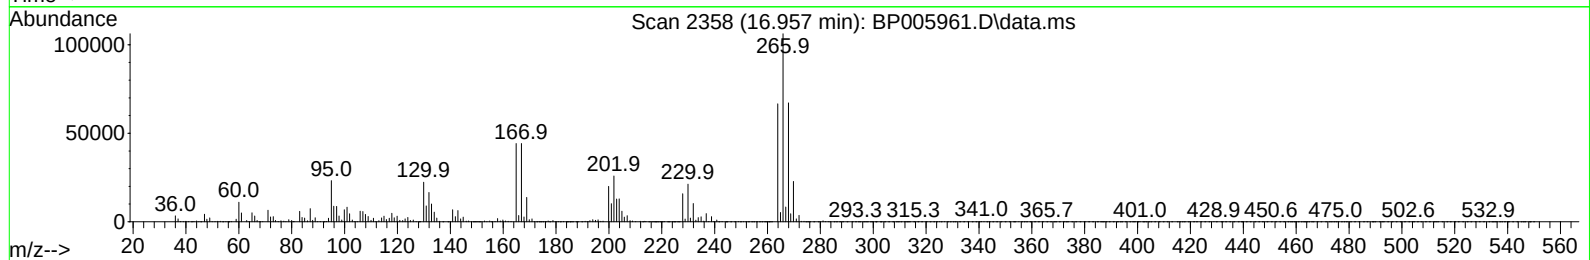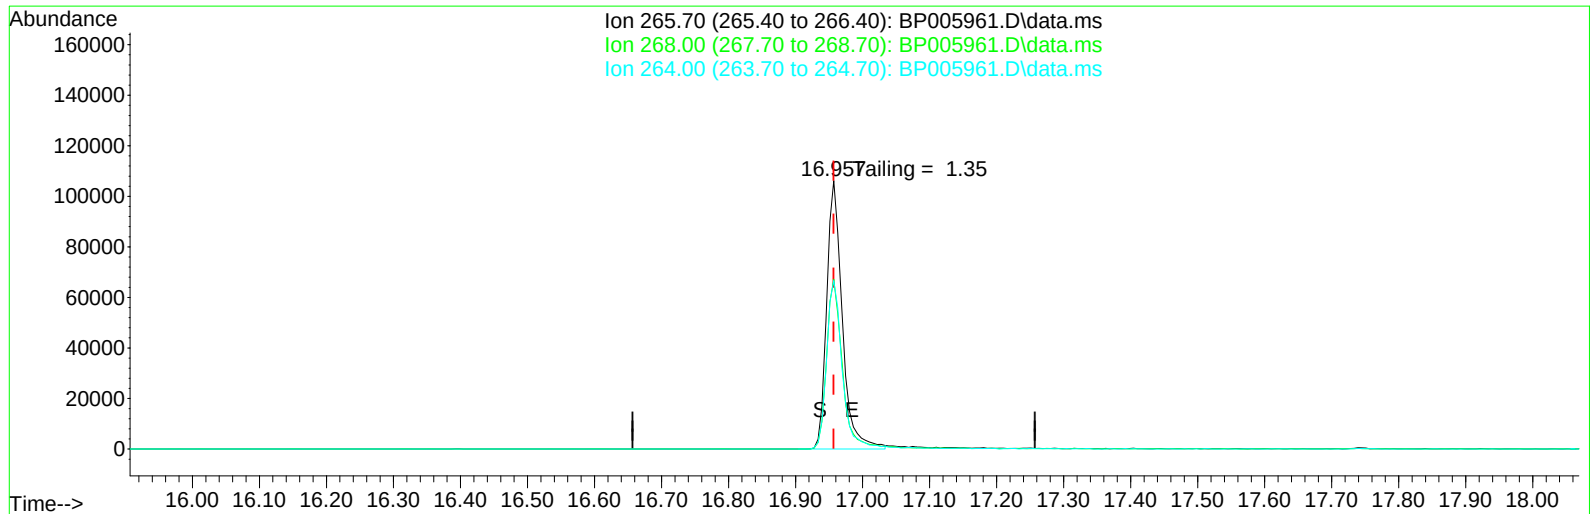

TIC: BP005961.D\data.ms

**(70) Pentachlorophenol (C)**

**16.957min (+ 0.000) 349928.82 ng**

**response 173619**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.50  | 63.21  |
| 264.00 | 62.90  | 62.71  |
| 0.00   | 0.00   | 0.00   |