
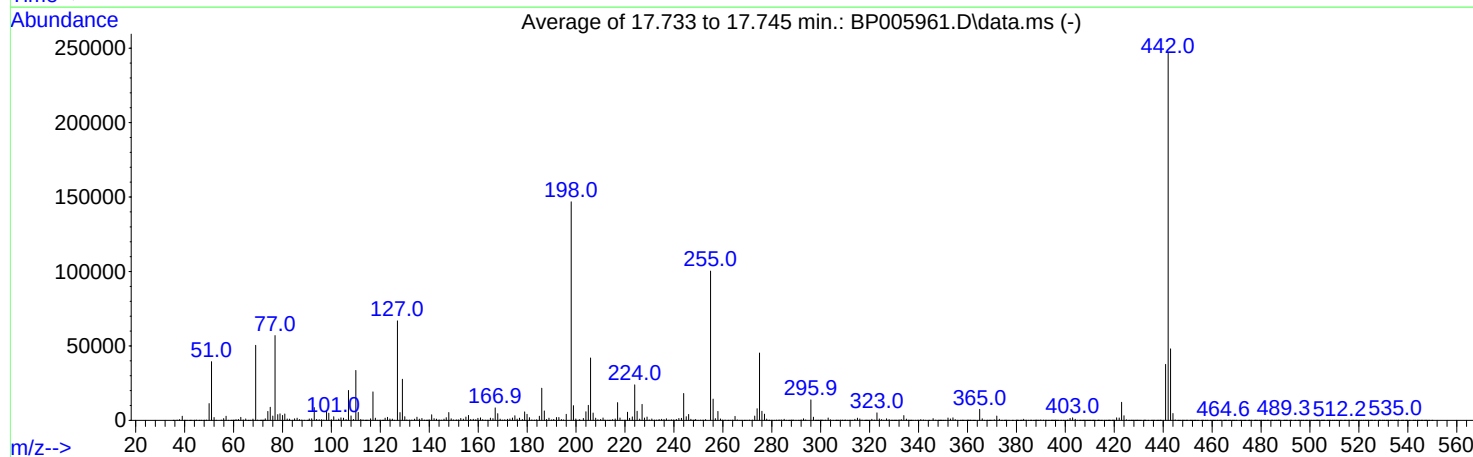


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061721\
 Data File : BP005961.D
 Acq On : 17 Jun 2021 10:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 16 11:35:30 2021

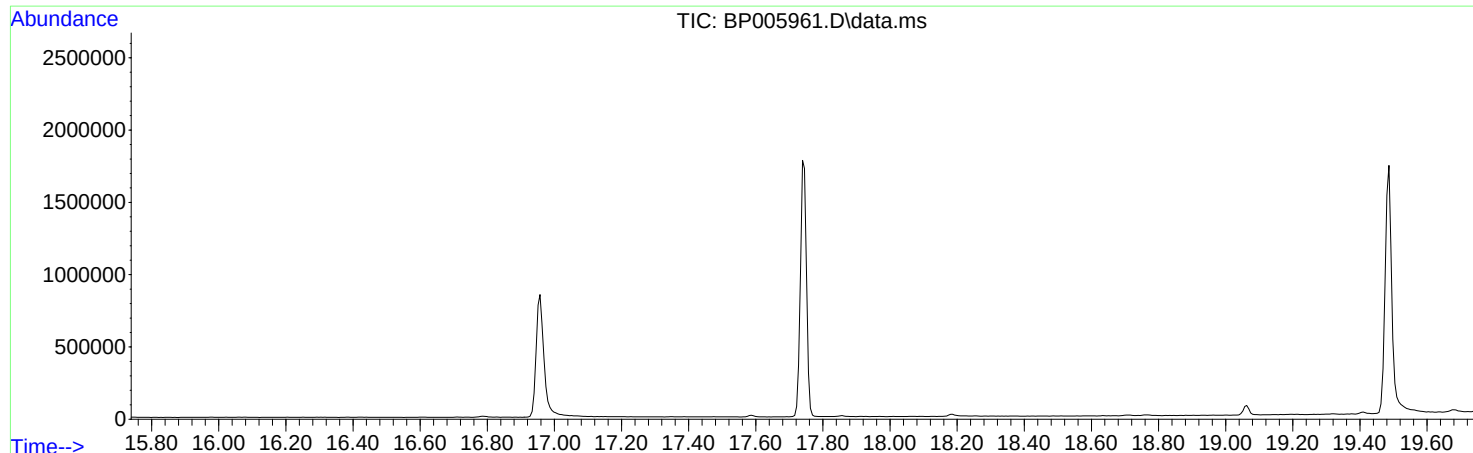




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	39449	PASS
68	69	0.00	2	1.8	903	PASS
69	198	0.00	100	34.3	50362	PASS
70	69	0.00	2	0.6	279	PASS
127	198	10	80	45.5	66844	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	146861	PASS
199	198	5	9	6.7	9862	PASS
275	198	10	60	30.8	45243	PASS
365	198	1	100	5.0	7396	PASS
441	198	0.01	100	25.6	37624	PASS
442	442	100	100	100.0	247101	PASS
443	442	15	24	19.4	48043	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061721\
 Data File : BP005961.D
 Acq On : 17 Jun 2021 10:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 17 13:41:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 16 11:35:30 2021
 Response via : Initial Calibration

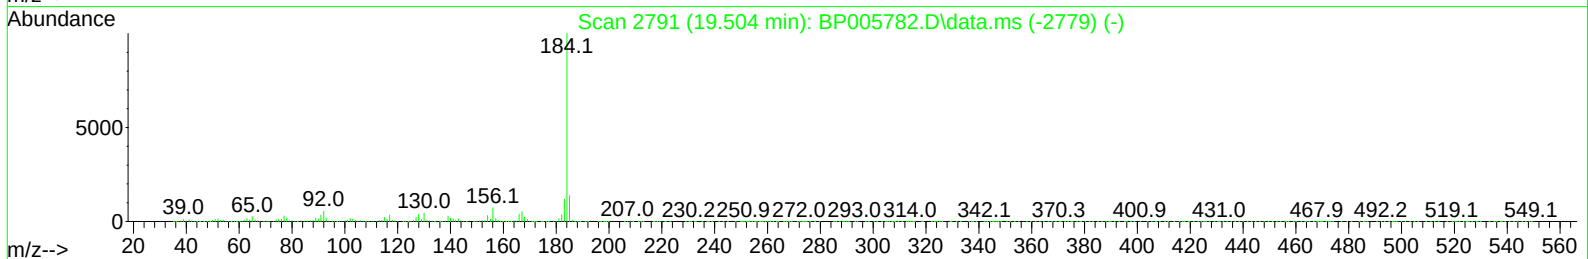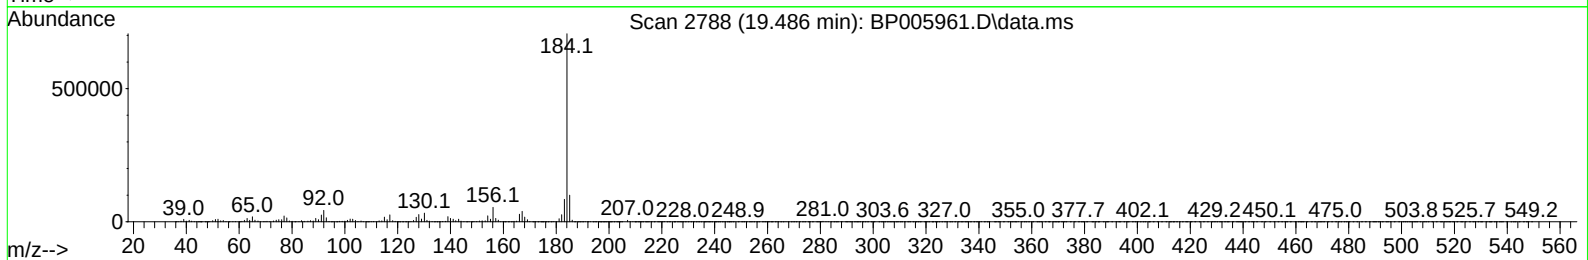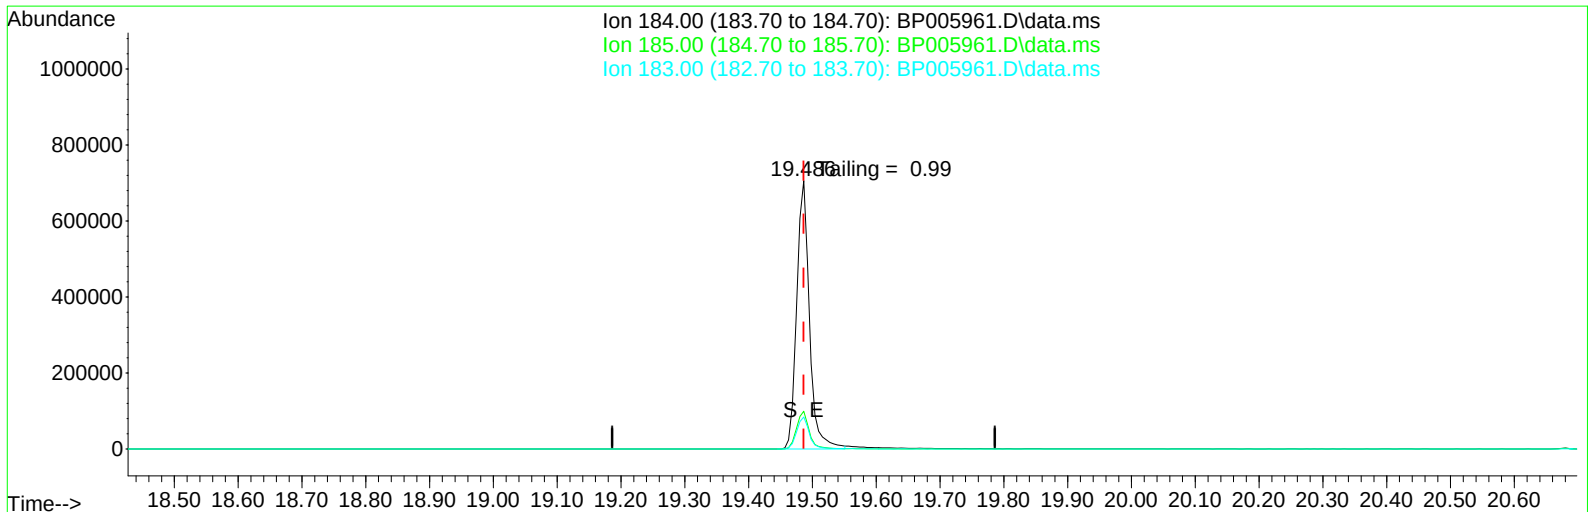

TIC: BP005961.D\data.ms

(77) Benzidine

19.486min (+ 0.000) 36969.48 ng




response 1005424

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.09
183.00	11.90	11.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061721\
 Data File : BP005961.D
 Acq On : 17 Jun 2021 10:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 17 13:41:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 16 11:35:30 2021
 Response via : Initial Calibration

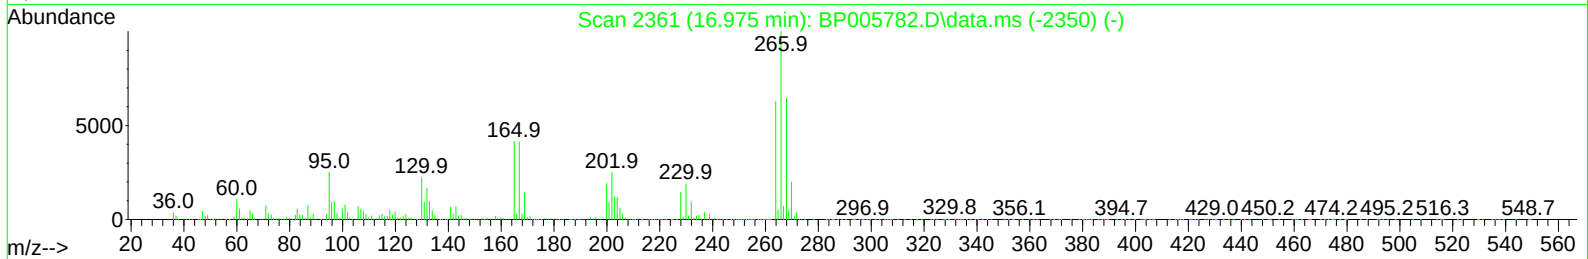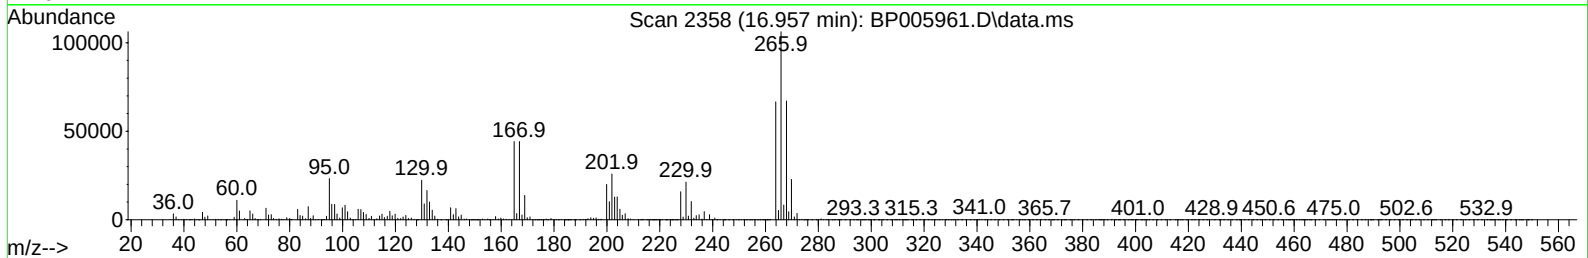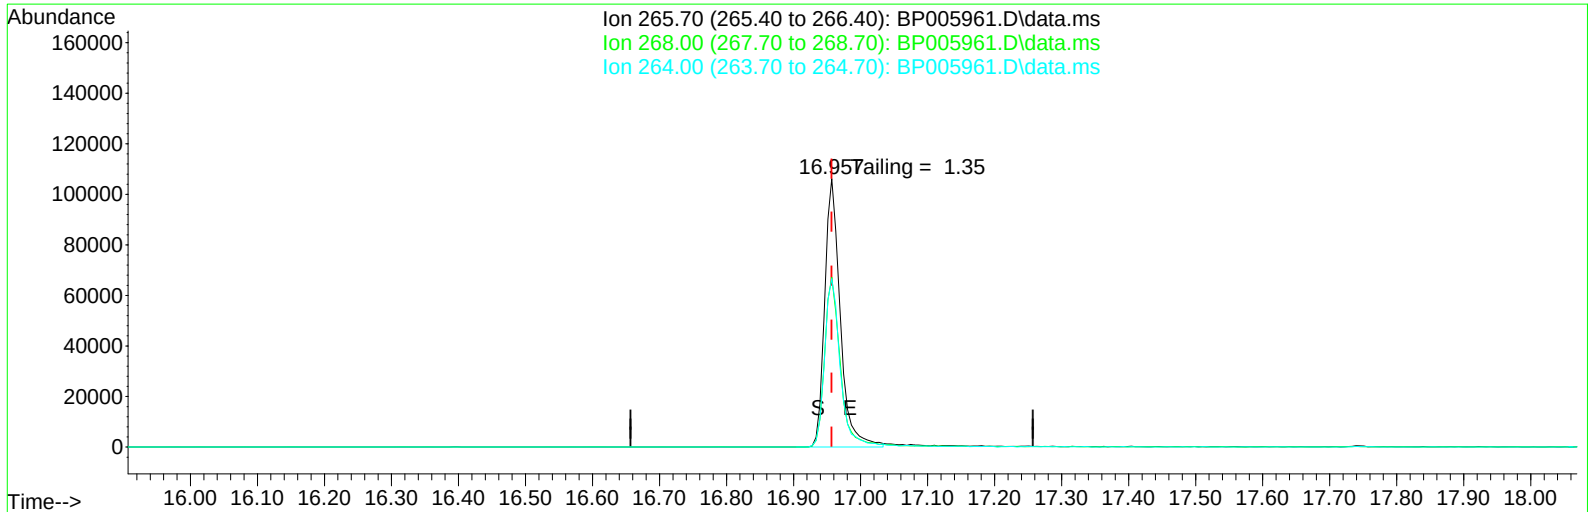

TIC: BP005961.D\data.ms

(70) Pentachlorophenol (C)

16.957min (+ 0.000) 349928.82 ng

response 173619

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.21
264.00	62.90	62.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/17/2021	BNA_P	<u>BP005961.D</u>
Compound Name	Response	Retention Time
DDT	593351	20.68
DDD	10688	20.25
DDE	2251	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12939	606290	2.13