
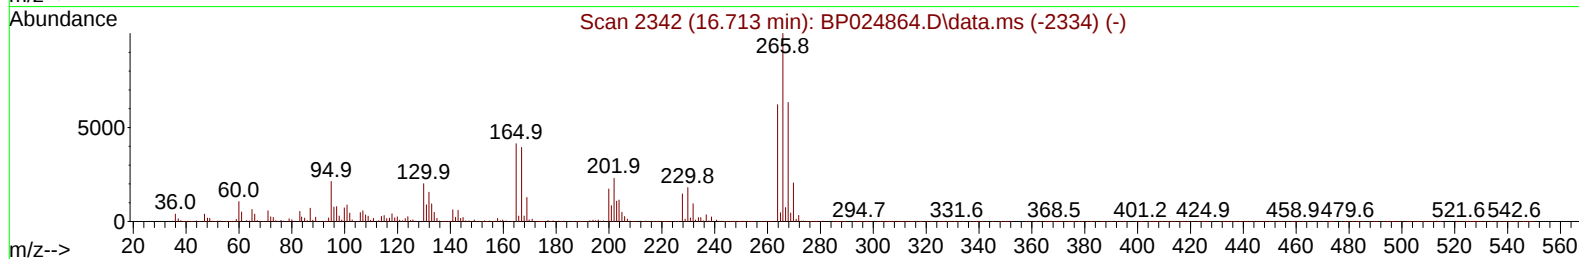
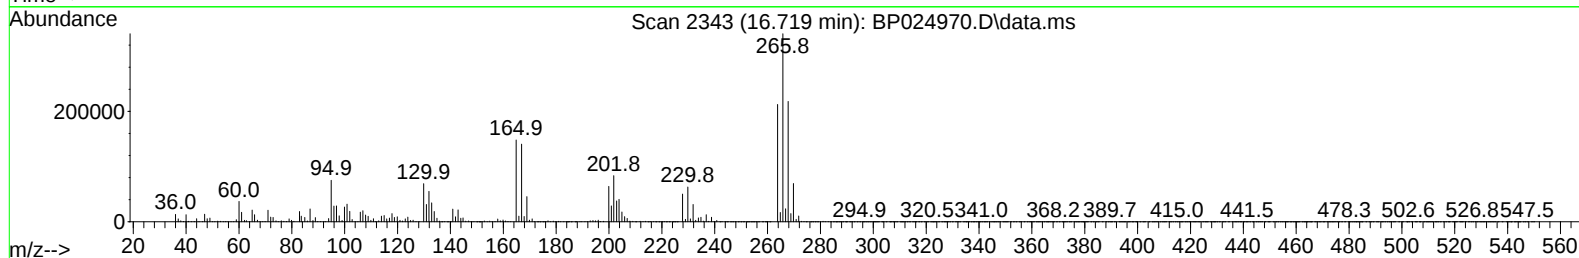


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061725\
Data File : BP024970.D
Acq On : 17 Jun 2025 10:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 19:06:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

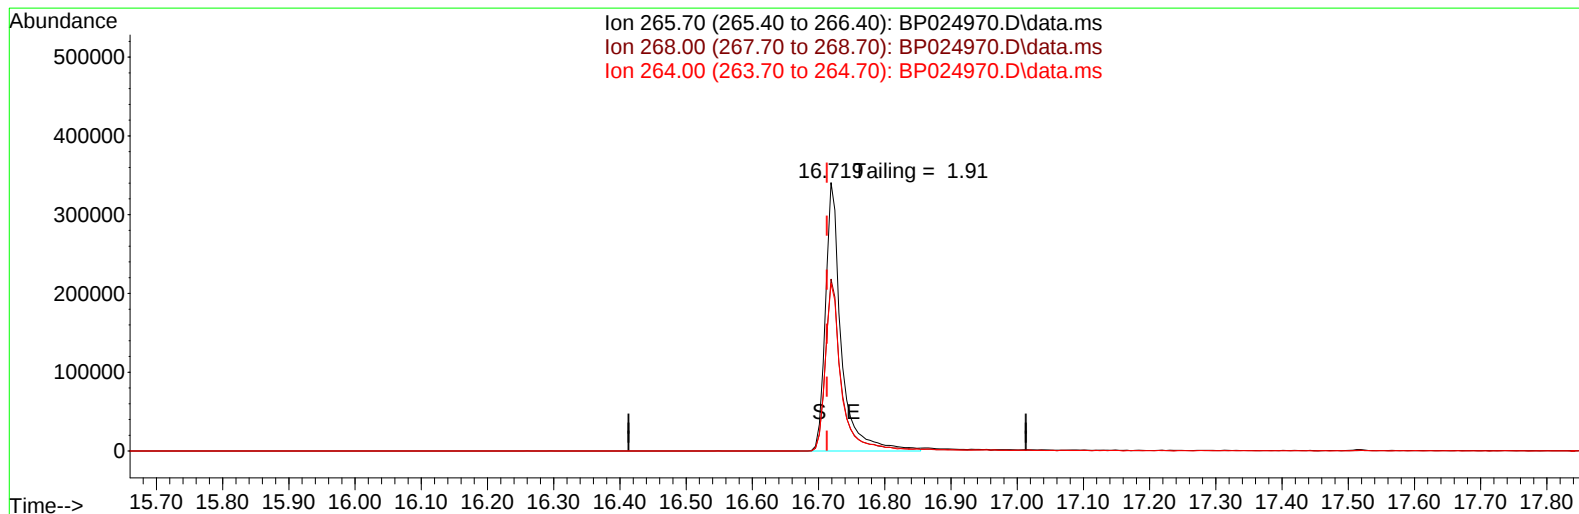

TIC: BP024970.D\data.ms

(70) Pentachlorophenol (C)




16.719min (+ 0.006) 144164.25 ng

response 565406

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.02
264.00	62.10	62.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061725\
Data File : BP024970.D
Acq On : 17 Jun 2025 10:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 19:06:36 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

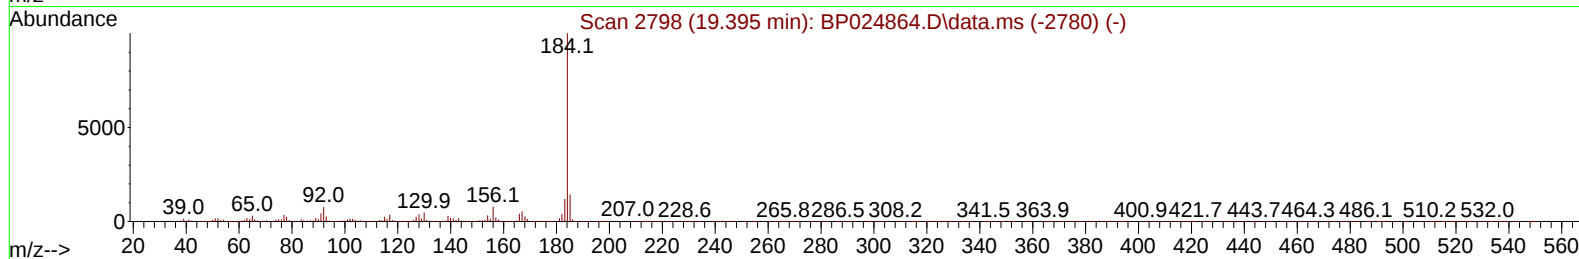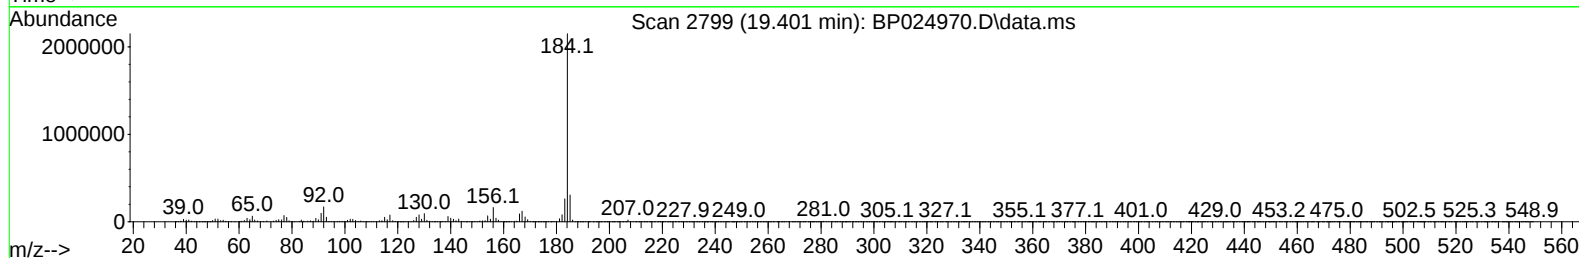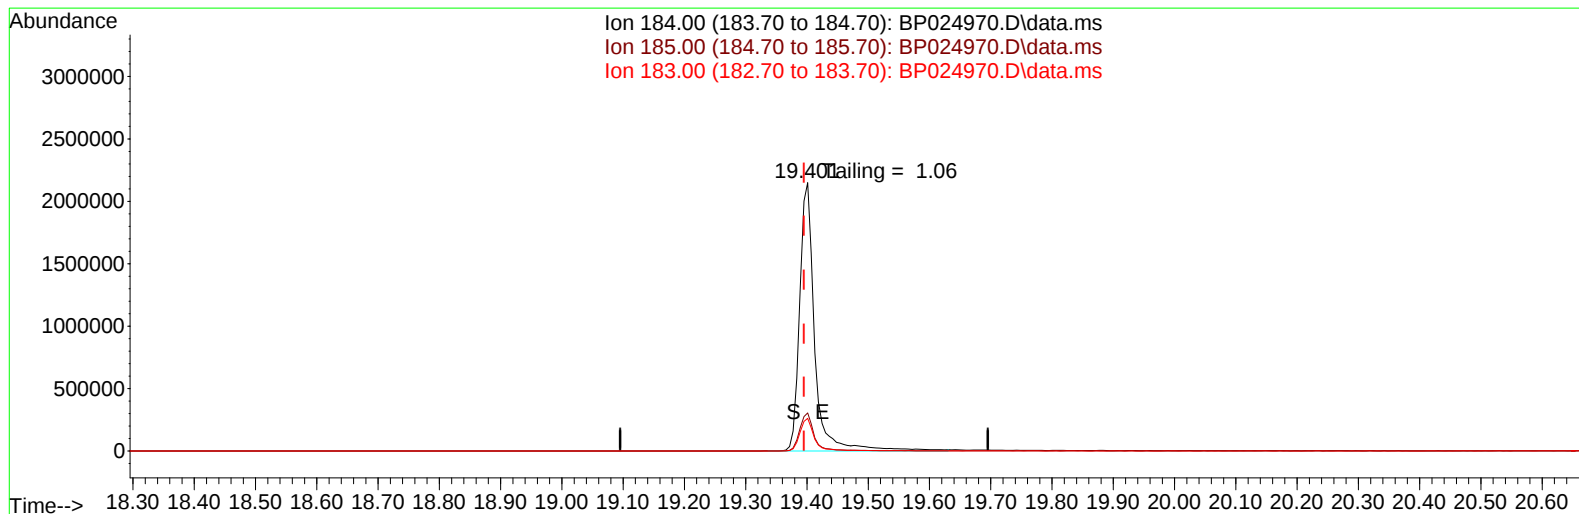

TIC: BP024970.D\data.ms

(77) Benzidine**19.401min (+ 0.006) 60269.07 ng****response 3690309**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.19
183.00	11.90	12.18
0.00	0.00	0.00