
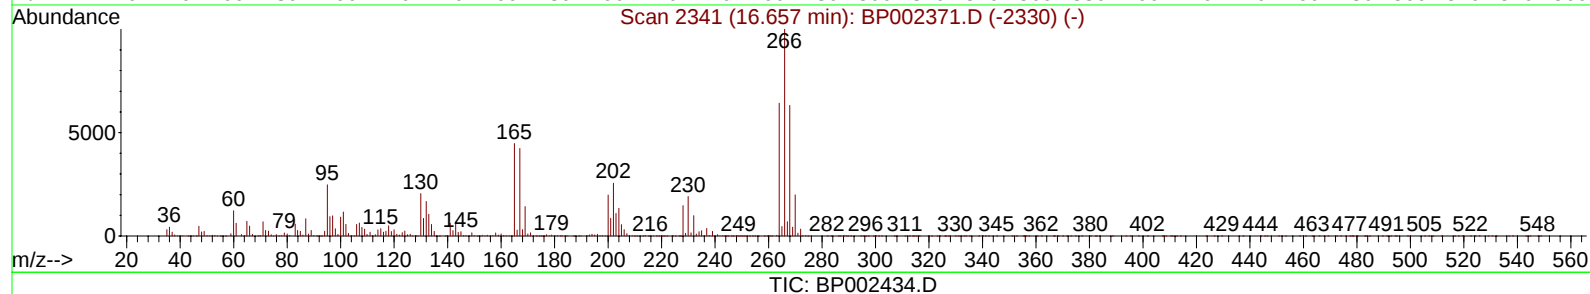
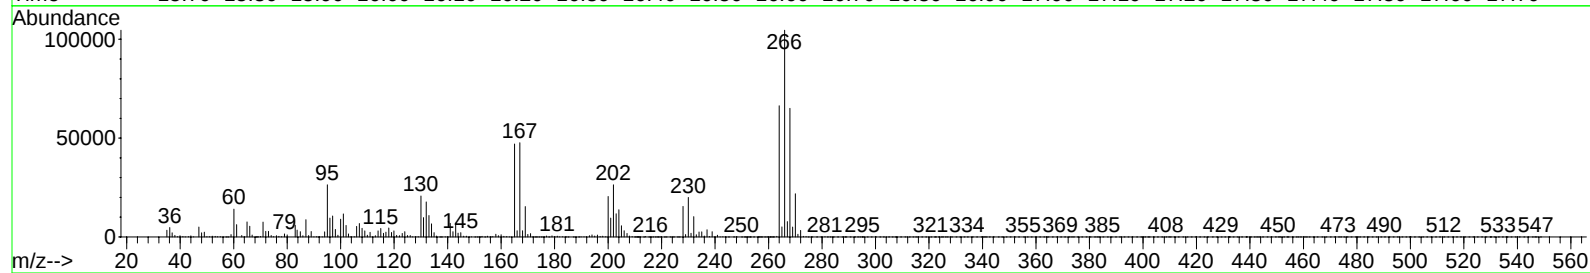


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061820\
Data File : BP002434.D
Acq On : 18 Jun 2020 08:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 17:57:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 15:08:53 2020
Response via : Initial Calibration

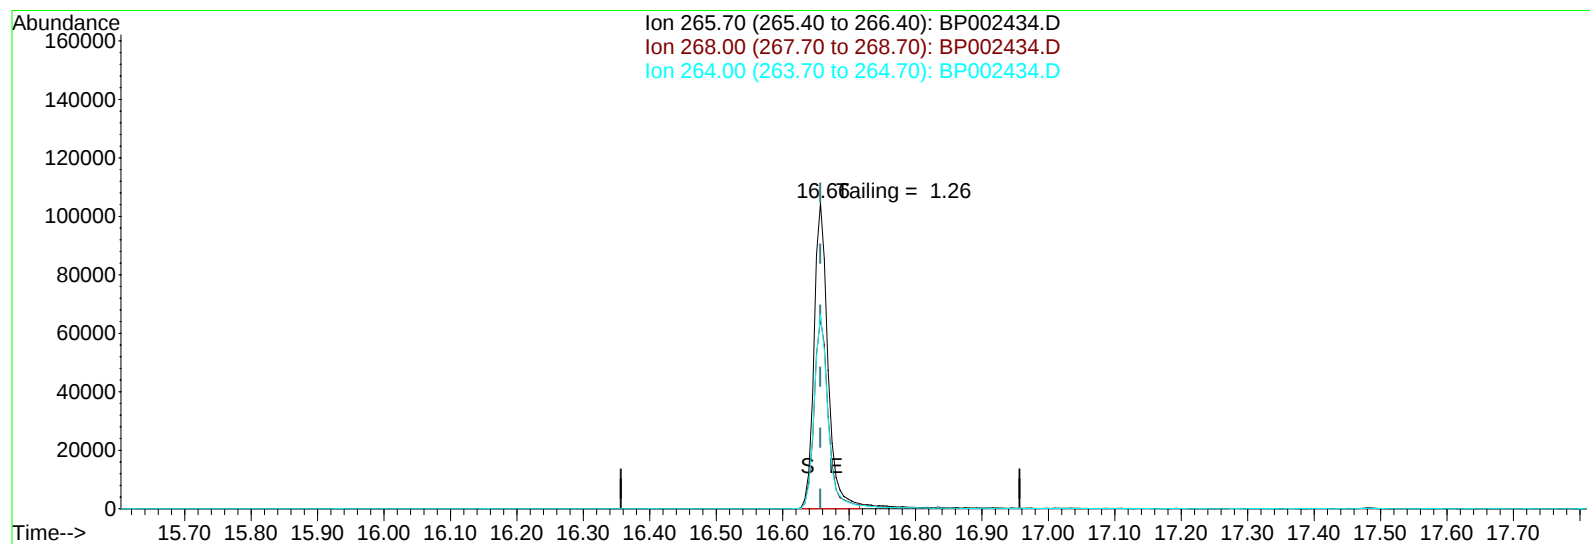

TIC: BP002434.D

(70) Pentachlorophenol (C)




16.657min (+0.000) 73651.58ng

response 156803

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	62.20
264.00	64.20	63.50
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP061820\
 Data File : BP002434.D
 Acq On : 18 Jun 2020 08:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 17:57:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 15:08:53 2020
 Response via : Initial Calibration

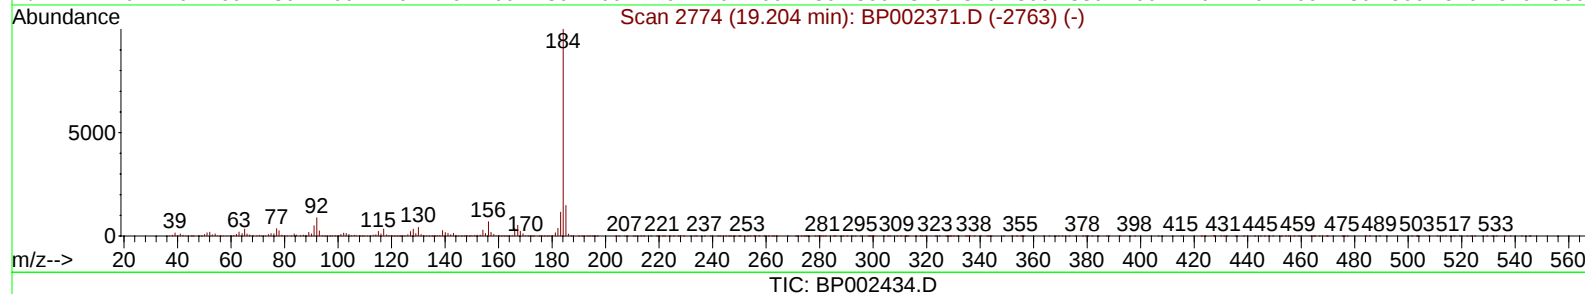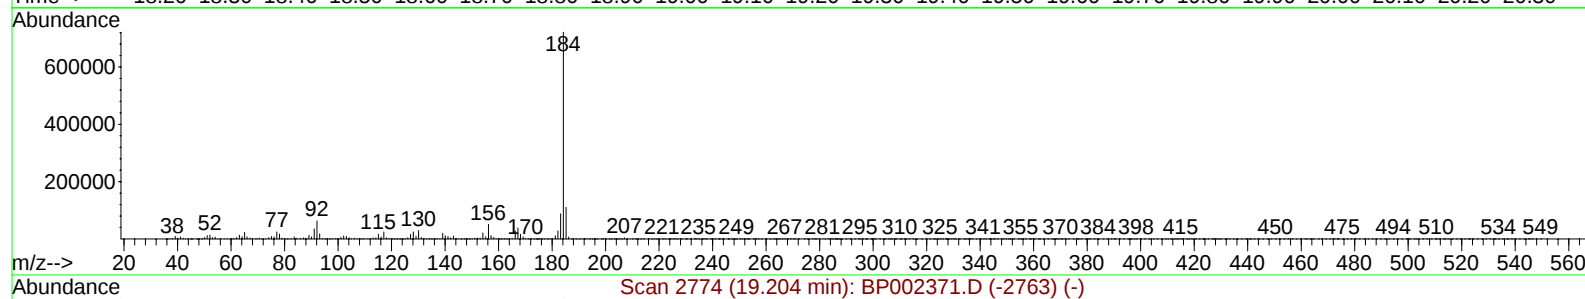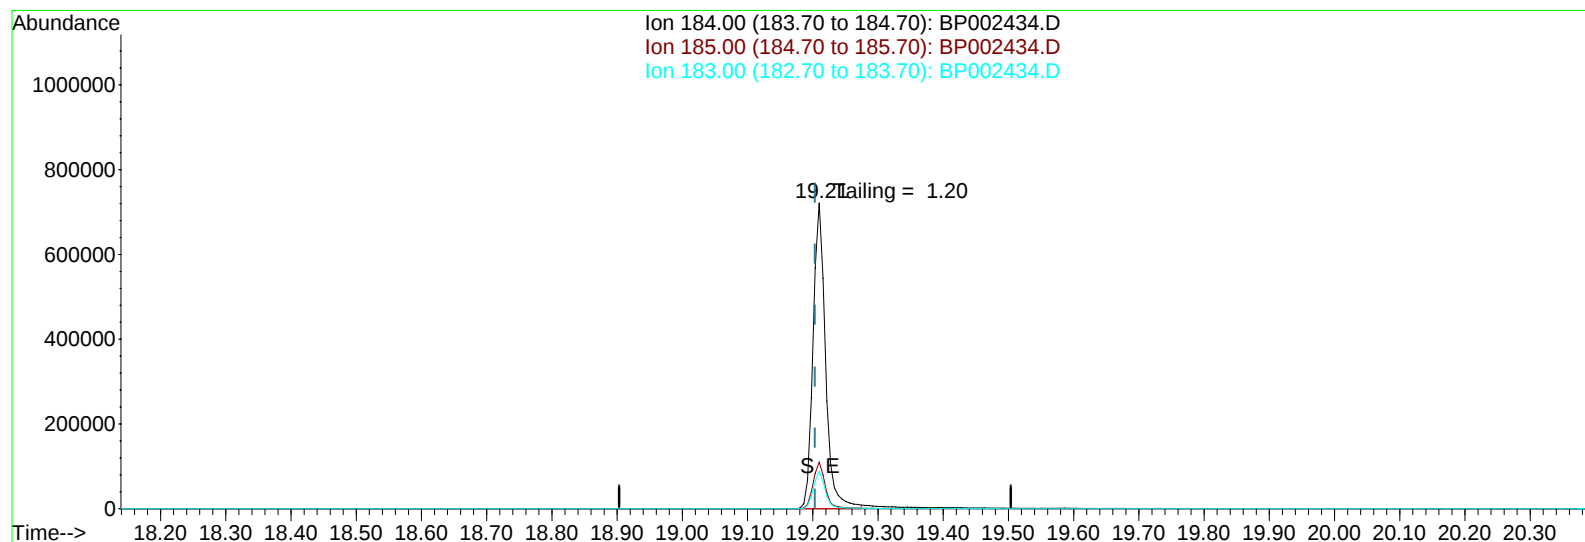

(77) Benzidine

19.210min (+0.006) 3546.20ng

response 980754

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	15.31
183.00	11.50	12.12
0.00	0.00	0.00