
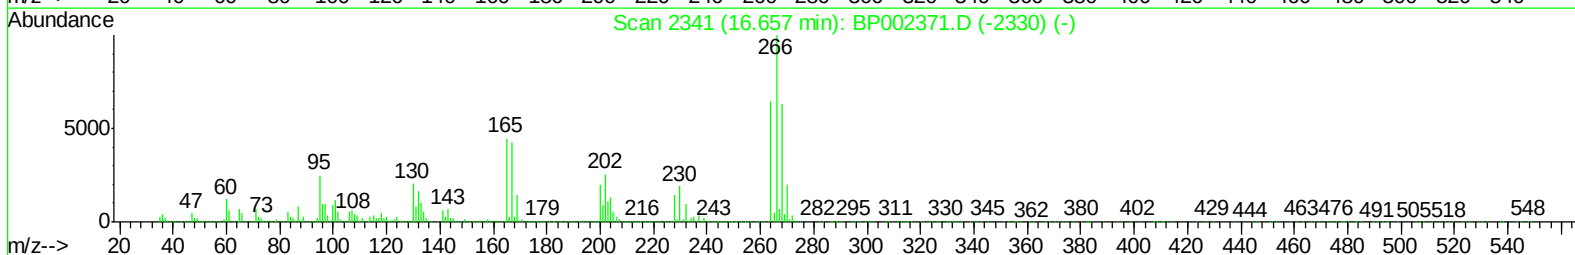
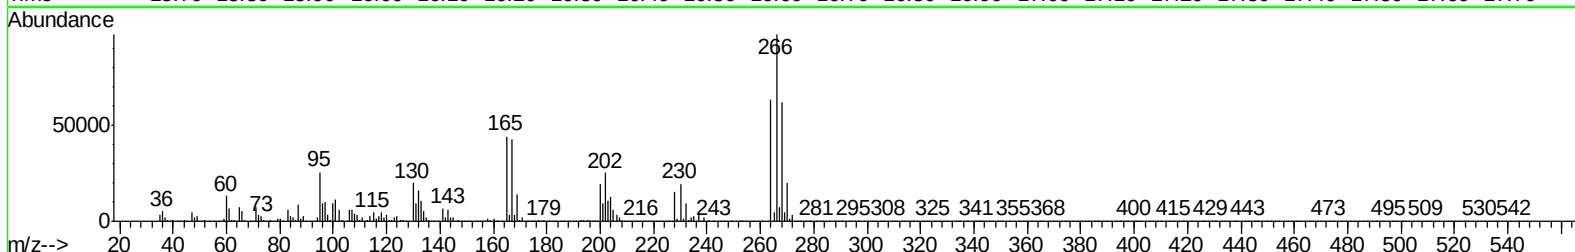


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP061820\
Data File : BP002437.D
Acq On : 18 Jun 2020 12:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 18:03:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 15:08:53 2020
Response via : Initial Calibration

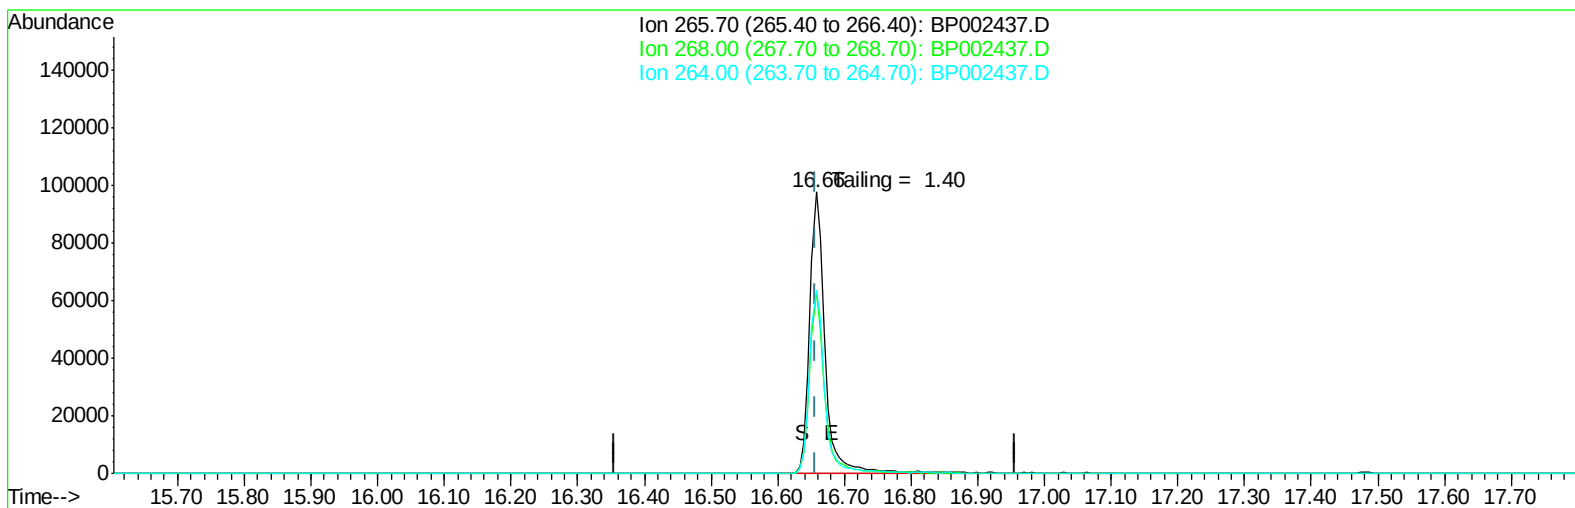

TIC: BP002437.D

(70) Pentachlorophenol (C)




16.657min (+0.001) 129114.60ng

response 149089

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	63.92
264.00	64.20	64.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP061820\
 Data File : BP002437.D
 Acq On : 18 Jun 2020 12:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 18:03:08 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 15:08:53 2020
 Response via : Initial Calibration

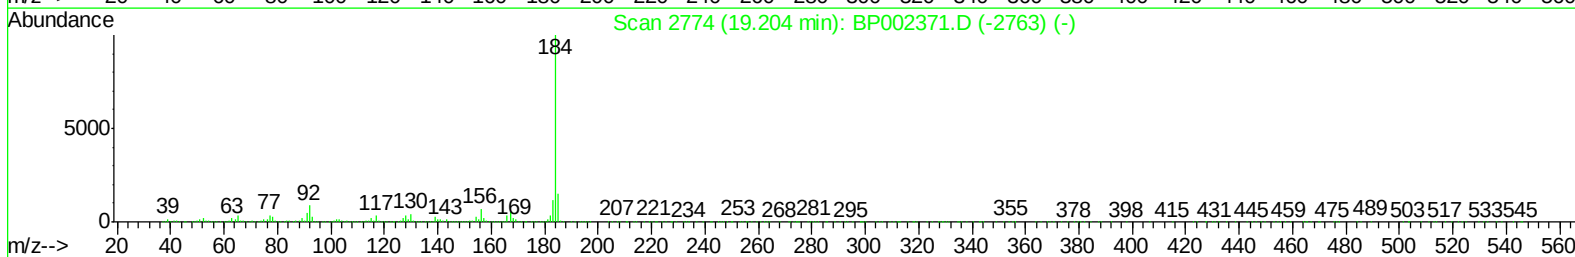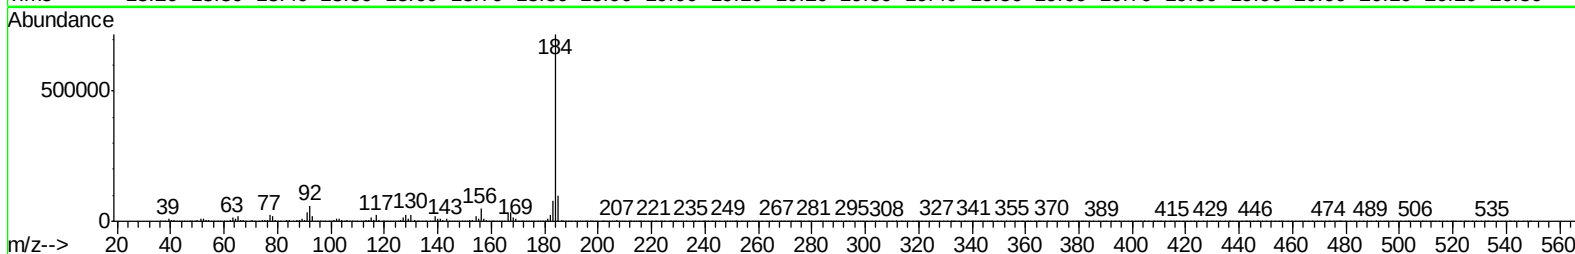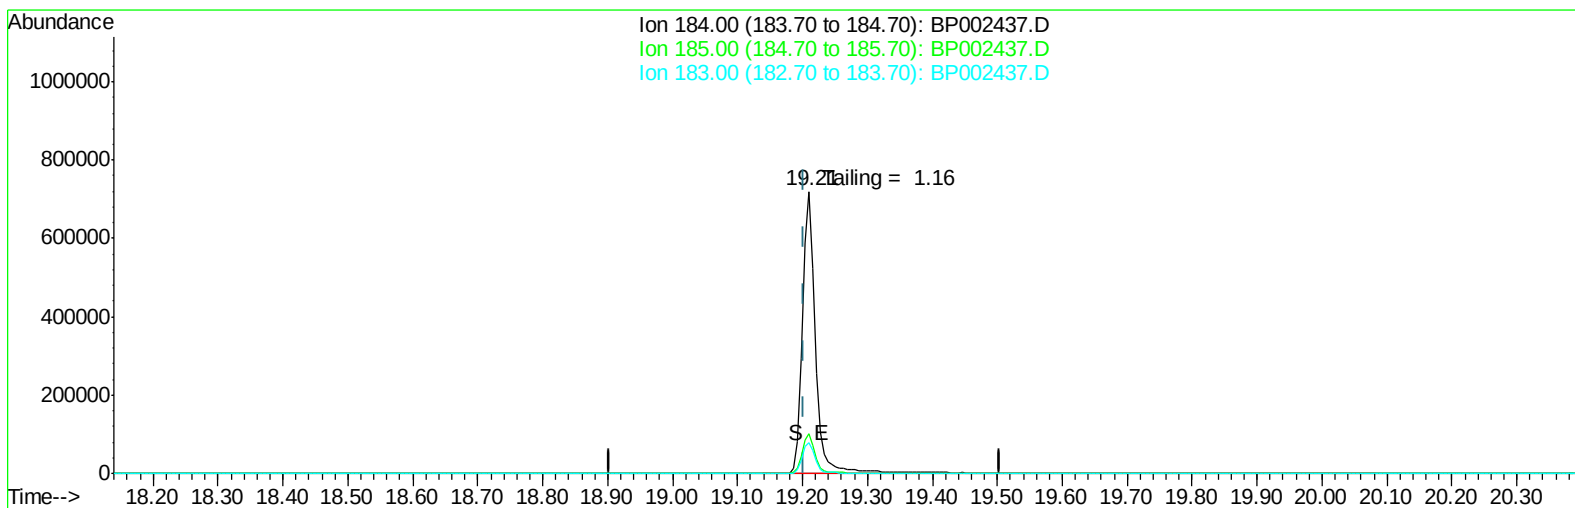

TIC: BP002437.D

(77) Benzidine

19.210min (+0.006) 6639.21ng

response 1001385

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	13.99
183.00	11.50	11.07
0.00	0.00	0.00